

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029418.D
 Acq On : 07 Dec 2022 15:34
 Operator : SY/MD
 Sample : VV1207WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK292

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029418.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	221064	223064	14.45%	1.794%
2	1.555	152	160	180	rVB	164831	193272	12.52%	1.554%
3	2.101	319	330	345	rBV	326365	471641	30.56%	3.793%
4	2.233	368	371	372	rBV2	478	311	0.02%	0.003%
5	2.288	380	388	396	rVB	2190	3062	0.20%	0.025%
6	2.500	446	454	466	rVB2	5638	9012	0.58%	0.072%
7	2.577	475	478	481	rBV	242	212	0.01%	0.002%
8	2.609	485	488	490	rVB2	432	216	0.01%	0.002%
9	2.651	497	501	505	rBV2	295	266	0.02%	0.002%
10	2.818	549	553	556	rBV2	401	265	0.02%	0.002%
11	3.085	631	636	640	rBV2	291	303	0.02%	0.002%
12	3.207	668	674	676	rBV	309	236	0.02%	0.002%
13	3.256	685	689	694	rBV2	258	290	0.02%	0.002%
14	3.429	738	743	751	rVB3	403	575	0.04%	0.005%
15	3.471	751	756	758	rBV	344	257	0.02%	0.002%
16	3.867	868	879	914	rBV	122652	328548	21.29%	2.642%
17	4.275	1004	1006	1008	rBV2	374	221	0.01%	0.002%
18	4.339	1009	1026	1055	rVV	240488	591330	38.31%	4.756%
19	4.619	1109	1113	1120	rVV3	390	442	0.03%	0.004%
20	4.674	1125	1130	1135	rVB4	554	539	0.03%	0.004%
21	4.773	1156	1161	1164	rVB2	344	254	0.02%	0.002%
22	4.809	1168	1172	1175	rVV3	320	271	0.02%	0.002%
23	4.825	1175	1177	1182	rVB2	307	229	0.01%	0.002%
24	4.931	1205	1210	1212	rBV	376	317	0.02%	0.003%
25	5.037	1223	1243	1277	rBV2	587406	1543420	100.00%	12.413%
26	5.259	1308	1312	1316	rBV4	411	326	0.02%	0.003%
27	5.387	1346	1352	1354	rBV3	329	316	0.02%	0.003%
28	5.403	1355	1357	1362	rVB3	395	294	0.02%	0.002%
29	5.535	1395	1398	1402	rBV2	341	294	0.02%	0.002%
30	5.606	1407	1420	1468	rVV	535854	1076898	69.77%	8.661%
31	5.899	1502	1511	1520	rBV5	4973	9313	0.60%	0.075%
32	6.059	1547	1561	1584	rBV	329825	681096	44.13%	5.478%
33	6.333	1641	1646	1648	rBV3	291	280	0.02%	0.002%
34	6.407	1662	1669	1672	rBV3	272	329	0.02%	0.003%
35	6.625	1728	1737	1739	rBV5	1044	1378	0.09%	0.011%
36	6.834	1800	1802	1806	rVB	342	234	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029418.D
 Acq On : 07 Dec 2022 15:34
 Operator : SY/MD
 Sample : VV1207WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK292

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.857	1806	1809	1812	rBV3	353	275	0.02%	0.002%
38	6.979	1835	1847	1876	rVV	199271	364980	23.65%	2.935%
39	7.307	1936	1949	1990	rBV	758972	1318657	85.44%	10.605%
40	7.529	2015	2018	2023	rBV3	386	376	0.02%	0.003%
41	7.612	2033	2044	2072	rBV	136293	239237	15.50%	1.924%
42	7.937	2138	2145	2149	rBV2	592	862	0.06%	0.007%
43	7.972	2152	2156	2163	rVB5	655	605	0.04%	0.005%
44	8.082	2178	2190	2220	rBV	432896	762589	49.41%	6.133%
45	8.378	2280	2282	2287	rVB3	379	215	0.01%	0.002%
46	8.516	2320	2325	2330	rBV5	494	586	0.04%	0.005%
47	8.596	2346	2350	2354	rVV4	334	398	0.03%	0.003%
48	8.693	2378	2380	2386	rVB2	307	224	0.01%	0.002%
49	8.844	2414	2427	2451	rBV	756798	1244596	80.64%	10.010%
50	9.008	2472	2478	2487	rVV5	1123	1624	0.11%	0.013%
51	9.043	2487	2489	2495	rVB3	607	386	0.03%	0.003%
52	9.088	2501	2503	2506	rBV3	430	276	0.02%	0.002%
53	9.133	2513	2517	2531	rVB2	977	1518	0.10%	0.012%
54	9.188	2531	2534	2536	rBV2	377	233	0.02%	0.002%
55	9.210	2538	2541	2543	rVB3	500	322	0.02%	0.003%
56	9.233	2543	2548	2552	rBV3	234	229	0.01%	0.002%
57	9.378	2589	2593	2599	rBV2	317	354	0.02%	0.003%
58	9.413	2599	2604	2606	rBV3	233	251	0.02%	0.002%
59	9.529	2636	2640	2642	rBV2	377	270	0.02%	0.002%
60	9.554	2646	2648	2649	rBV	521	215	0.01%	0.002%
61	9.622	2666	2669	2672	rVV2	300	224	0.01%	0.002%
62	9.693	2687	2691	2693	rVB3	381	276	0.02%	0.002%
63	9.709	2693	2696	2700	rBV2	316	328	0.02%	0.003%
64	9.773	2713	2716	2719	rBV	406	246	0.02%	0.002%
65	9.863	2741	2744	2747	rBV2	343	304	0.02%	0.002%
66	9.882	2748	2750	2755	rVB2	322	217	0.01%	0.002%
67	9.921	2755	2762	2763	rBV2	778	775	0.05%	0.006%
68	10.069	2806	2808	2813	rVB3	367	280	0.02%	0.002%
69	10.146	2827	2832	2834	rBV2	252	219	0.01%	0.002%
70	10.207	2838	2851	2872	rVV	505658	794354	51.47%	6.389%
71	10.387	2904	2907	2912	rBB3	321	258	0.02%	0.002%
72	10.442	2922	2924	2933	rVB3	348	348	0.02%	0.003%
73	10.480	2933	2936	2939	rVB2	368	226	0.01%	0.002%
74	10.529	2946	2951	2955	rBV3	926	920	0.06%	0.007%
75	10.635	2982	2984	2989	rBV3	355	394	0.03%	0.003%
76	10.728	3010	3013	3015	rBV	294	225	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029418.D
 Acq On : 07 Dec 2022 15:34
 Operator : SY/MD
 Sample : VV1207WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK292

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.847	3046	3050	3053	rBV4	595	515	0.03%	0.004%
78	10.908	3063	3069	3075	rBV2	956	1291	0.08%	0.010%
79	11.085	3120	3124	3128	rBV3	454	413	0.03%	0.003%
80	11.175	3144	3152	3159	rBV3	1580	2564	0.17%	0.021%
81	11.239	3159	3172	3202	rBV	835410	1289462	83.55%	10.370%
82	11.612	3275	3288	3317	rBV	777082	1237783	80.20%	9.955%
83	11.770	3334	3337	3343	rVB5	443	414	0.03%	0.003%
84	11.850	3359	3362	3367	rBV4	418	366	0.02%	0.003%
85	11.918	3380	3383	3388	rVB3	454	340	0.02%	0.003%
86	11.940	3388	3390	3395	rVB4	373	228	0.01%	0.002%
87	12.172	3458	3462	3464	rBV3	490	310	0.02%	0.002%
88	12.332	3504	3512	3517	rBV6	948	1407	0.09%	0.011%
89	12.387	3526	3529	3531	rBV2	620	381	0.02%	0.003%
90	12.773	3645	3649	3651	rBV2	361	243	0.02%	0.002%
91	12.824	3662	3665	3673	rBV5	416	467	0.03%	0.004%
92	12.985	3712	3715	3720	rVB3	516	458	0.03%	0.004%
93	13.024	3723	3727	3729	rBV3	621	461	0.03%	0.004%
94	13.130	3756	3760	3763	rBV4	526	406	0.03%	0.003%
95	13.249	3791	3797	3810	rVB5	3207	5011	0.32%	0.040%
96	13.345	3822	3827	3829	rBV4	613	566	0.04%	0.005%
97	13.368	3832	3834	3836	rVB	663	254	0.02%	0.002%
98	13.496	3868	3874	3883	rVB4	4936	6821	0.44%	0.055%
99	13.644	3918	3920	3922	rBV2	543	296	0.02%	0.002%
100	13.734	3940	3948	3957	rVB7	3261	5461	0.35%	0.044%




Sum of corrected areas: 12434101

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029418.D
Acq On : 07 Dec 2022 15:34
Operator : SY/MD
Sample : VV1207WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK292

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

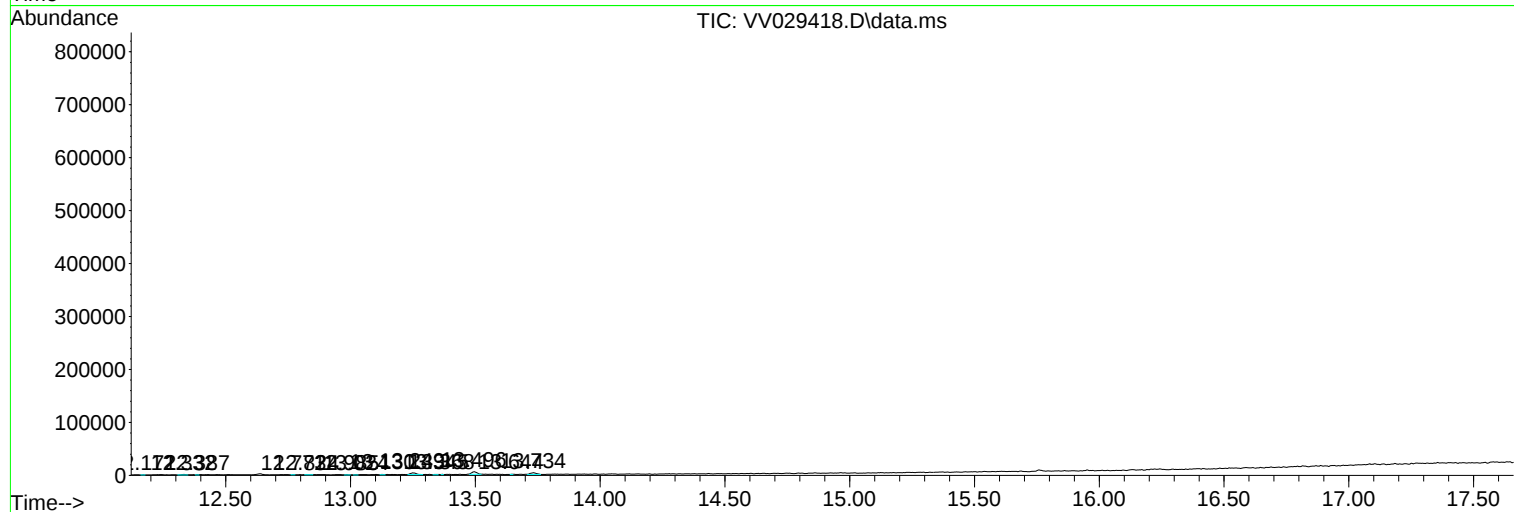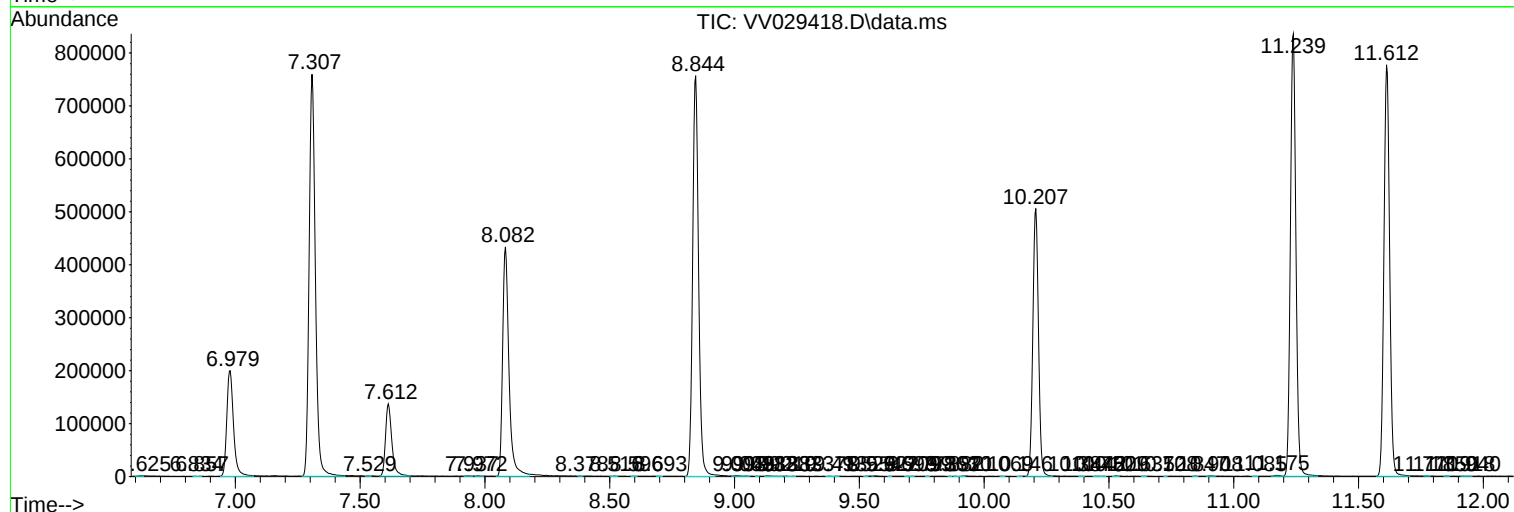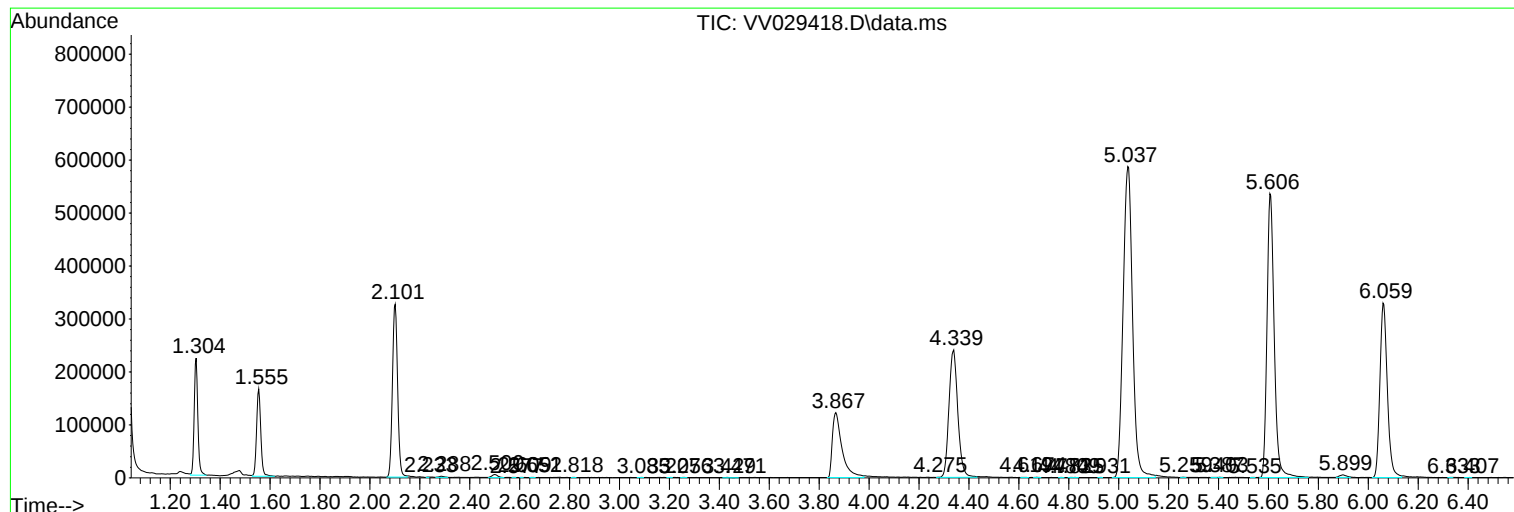

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029418.D
Acq On : 07 Dec 2022 15:34
Operator : SY/MD
Sample : VV1207WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK292

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029418.D
Acq On : 07 Dec 2022 15:34
Operator : SY/MD
Sample : VV1207WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK292

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc