

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029419.D
 Acq On : 07 Dec 2022 15:58
 Operator : SY/MD
 Sample : VV1207MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK293

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VV029419.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	205983	206980	13.47%	1.669%
2	1.552	151	159	182	rVB	160366	191480	12.46%	1.544%
3	2.031	306	308	311	rBV2	410	197	0.01%	0.002%
4	2.101	316	330	344	rBV	313848	456352	29.70%	3.681%
5	2.285	384	387	397	rVB	1857	2072	0.13%	0.017%
6	2.429	429	432	438	rVB3	490	466	0.03%	0.004%
7	2.500	444	454	463	rVB	5643	9425	0.61%	0.076%
8	2.606	482	487	497	rVV2	471	875	0.06%	0.007%
9	2.754	530	533	536	rBV3	430	336	0.02%	0.003%
10	2.789	540	544	549	rBV3	318	358	0.02%	0.003%
11	2.915	575	583	587	rBV3	258	326	0.02%	0.003%
12	3.072	629	632	637	rVB3	362	309	0.02%	0.002%
13	3.101	638	641	645	rBV	283	193	0.01%	0.002%
14	3.162	658	660	664	rVB2	311	195	0.01%	0.002%
15	3.224	676	679	685	rVB	349	279	0.02%	0.002%
16	3.416	734	739	744	rVB3	300	380	0.02%	0.003%
17	3.596	792	795	798	rBV2	313	261	0.02%	0.002%
18	3.619	798	802	805	rVV	350	280	0.02%	0.002%
19	3.867	869	879	918	rBV	127614	344061	22.39%	2.775%
20	4.336	1008	1025	1057	rBV	235188	583014	37.94%	4.702%
21	4.616	1109	1112	1114	rBV2	377	221	0.01%	0.002%
22	4.648	1118	1122	1126	rVB4	336	336	0.02%	0.003%
23	4.899	1193	1200	1203	rBV2	298	357	0.02%	0.003%
24	4.947	1211	1215	1220	rBV3	343	241	0.02%	0.002%
25	5.037	1224	1243	1292	rBV2	587886	1536720	100.00%	12.394%
26	5.243	1305	1307	1311	rBV3	302	223	0.01%	0.002%
27	5.362	1340	1344	1348	rBV3	307	284	0.02%	0.002%
28	5.394	1350	1354	1358	rVV3	355	332	0.02%	0.003%
29	5.420	1360	1362	1365	rVB2	423	236	0.02%	0.002%
30	5.471	1371	1378	1380	rBV2	456	533	0.03%	0.004%
31	5.555	1400	1404	1407	rBV3	250	208	0.01%	0.002%
32	5.609	1407	1421	1449	rBV	521071	1062557	69.14%	8.570%
33	5.899	1501	1511	1527	rBV2	5345	10735	0.70%	0.087%
34	5.985	1535	1538	1540	rBV2	304	201	0.01%	0.002%
35	6.059	1548	1561	1599	rBV	328201	686913	44.70%	5.540%
36	6.281	1628	1630	1631	rBV	467	197	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029419.D
 Acq On : 07 Dec 2022 15:58
 Operator : SY/MD
 Sample : VV1207MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK293

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.339	1645	1648	1652	rBV3	408	326	0.02%	0.003%
38	6.381	1656	1661	1663	rVB2	448	344	0.02%	0.003%
39	6.407	1663	1669	1675	rBV	473	574	0.04%	0.005%
40	6.529	1704	1707	1712	rBV3	224	198	0.01%	0.002%
41	6.622	1725	1736	1738	rBV5	995	1439	0.09%	0.012%
42	6.728	1765	1769	1772	rBV4	349	221	0.01%	0.002%
43	6.863	1808	1811	1817	rVB4	416	424	0.03%	0.003%
44	6.892	1817	1820	1823	rBV3	311	264	0.02%	0.002%
45	6.976	1834	1846	1880	rBV	195819	362158	23.57%	2.921%
46	7.159	1895	1903	1911	rBV7	900	1489	0.10%	0.012%
47	7.201	1913	1916	1923	rVB3	584	626	0.04%	0.005%
48	7.233	1923	1926	1930	rBV4	461	351	0.02%	0.003%
49	7.307	1933	1949	1981	rBV	729382	1296649	84.38%	10.458%
50	7.612	2033	2044	2072	rVV	139492	240309	15.64%	1.938%
51	7.927	2139	2142	2146	rBV3	684	640	0.04%	0.005%
52	7.989	2159	2161	2166	rVB2	338	214	0.01%	0.002%
53	8.082	2179	2190	2217	rBV	450338	783292	50.97%	6.317%
54	8.481	2312	2314	2319	rVB3	409	234	0.02%	0.002%
55	8.747	2394	2397	2403	rVB3	392	374	0.02%	0.003%
56	8.844	2414	2427	2464	rBV	768395	1247173	81.16%	10.059%
57	9.059	2491	2494	2497	rBV3	525	370	0.02%	0.003%
58	9.191	2532	2535	2539	rVB2	305	224	0.01%	0.002%
59	9.239	2547	2550	2554	rBV4	339	273	0.02%	0.002%
60	9.307	2565	2571	2575	rVB	377	345	0.02%	0.003%
61	9.365	2586	2589	2593	rVB2	353	318	0.02%	0.003%
62	9.397	2593	2599	2602	rBV3	416	419	0.03%	0.003%
63	9.480	2620	2625	2628	rBV2	178	212	0.01%	0.002%
64	9.542	2639	2644	2648	rBV4	520	699	0.05%	0.006%
65	9.574	2648	2654	2656	rVV2	427	443	0.03%	0.004%
66	9.657	2676	2680	2683	rBV2	316	265	0.02%	0.002%
67	9.831	2732	2734	2737	rBV2	281	214	0.01%	0.002%
68	9.873	2743	2747	2748	rBV2	310	254	0.02%	0.002%
69	9.898	2750	2755	2759	rVV3	442	486	0.03%	0.004%
70	10.027	2792	2795	2801	rVB2	366	309	0.02%	0.002%
71	10.204	2836	2850	2877	rVV	510212	817088	53.17%	6.590%
72	10.323	2883	2887	2891	rBV3	494	415	0.03%	0.003%
73	10.448	2923	2926	2932	rVB3	247	249	0.02%	0.002%
74	10.680	2994	2998	3000	rBV3	357	279	0.02%	0.002%
75	10.751	3018	3020	3025	rVB3	348	243	0.02%	0.002%
76	10.808	3034	3038	3040	rBV3	338	268	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029419.D
 Acq On : 07 Dec 2022 15:58
 Operator : SY/MD
 Sample : VV1207MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK293

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.844	3044	3049	3054	rVV4	647	636	0.04%	0.005%
78	11.001	3094	3098	3104	rBV4	372	413	0.03%	0.003%
79	11.053	3110	3114	3115	rBV2	273	218	0.01%	0.002%
80	11.085	3122	3124	3127	rVB	432	225	0.01%	0.002%
81	11.169	3146	3150	3158	rBV3	1457	1921	0.13%	0.015%
82	11.239	3158	3172	3192	rBV	828134	1284148	83.56%	10.357%
83	11.387	3217	3218	3225	rVB3	428	328	0.02%	0.003%
84	11.429	3228	3231	3235	rVB4	384	236	0.02%	0.002%
85	11.490	3246	3250	3253	rBV3	225	202	0.01%	0.002%
86	11.612	3275	3288	3310	rBV	792456	1236814	80.48%	9.975%
87	11.779	3338	3340	3346	rVB3	644	515	0.03%	0.004%
88	11.818	3351	3352	3356	rVB3	383	206	0.01%	0.002%
89	11.841	3356	3359	3362	rBV4	461	364	0.02%	0.003%
90	11.979	3399	3402	3404	rVB3	469	272	0.02%	0.002%
91	12.487	3555	3560	3563	rBV3	498	481	0.03%	0.004%
92	12.538	3573	3576	3578	rBV	439	266	0.02%	0.002%
93	12.631	3602	3605	3613	rVB5	1374	1569	0.10%	0.013%
94	12.770	3645	3648	3653	rVV4	474	450	0.03%	0.004%
95	12.866	3675	3678	3680	rBV	769	378	0.02%	0.003%
96	13.249	3792	3797	3805	rVB6	2415	3096	0.20%	0.025%
97	13.500	3867	3875	3881	rBV2	3736	6347	0.41%	0.051%
98	13.599	3903	3906	3907	rBV2	832	511	0.03%	0.004%
99	13.664	3924	3926	3928	rBV2	462	245	0.02%	0.002%
100	14.172	4081	4084	4085	rBV2	735	440	0.03%	0.004%



Sum of corrected areas: 12399086

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029419.D
Acq On : 07 Dec 2022 15:58
Operator : SY/MD
Sample : VV1207MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK293

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

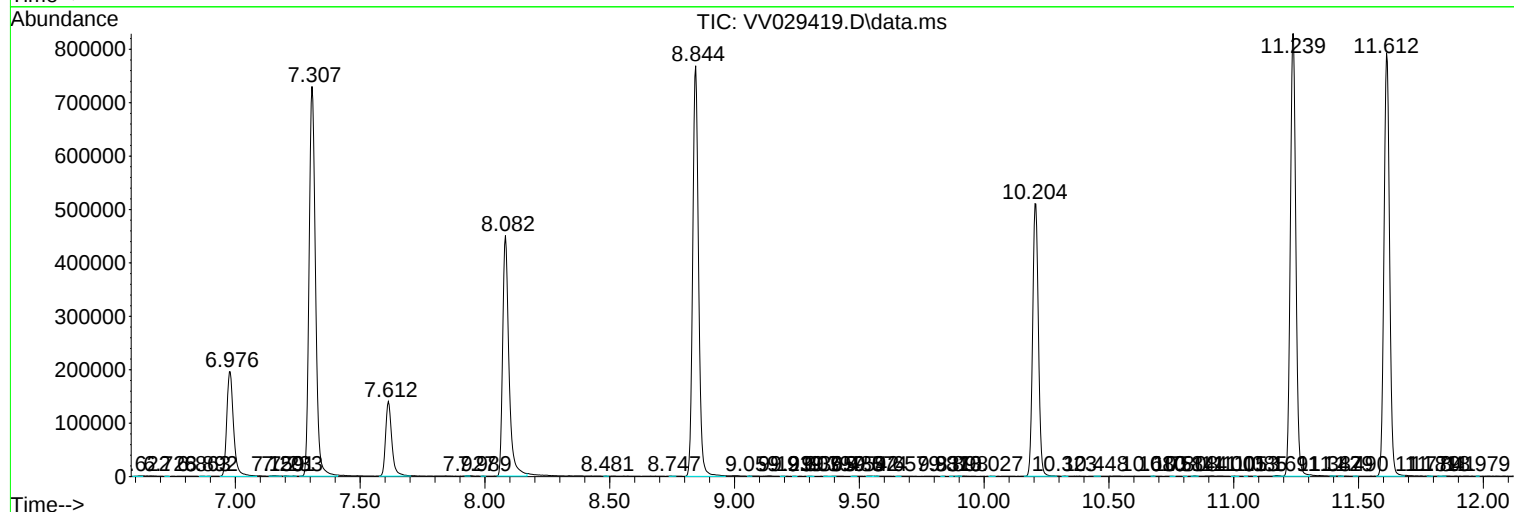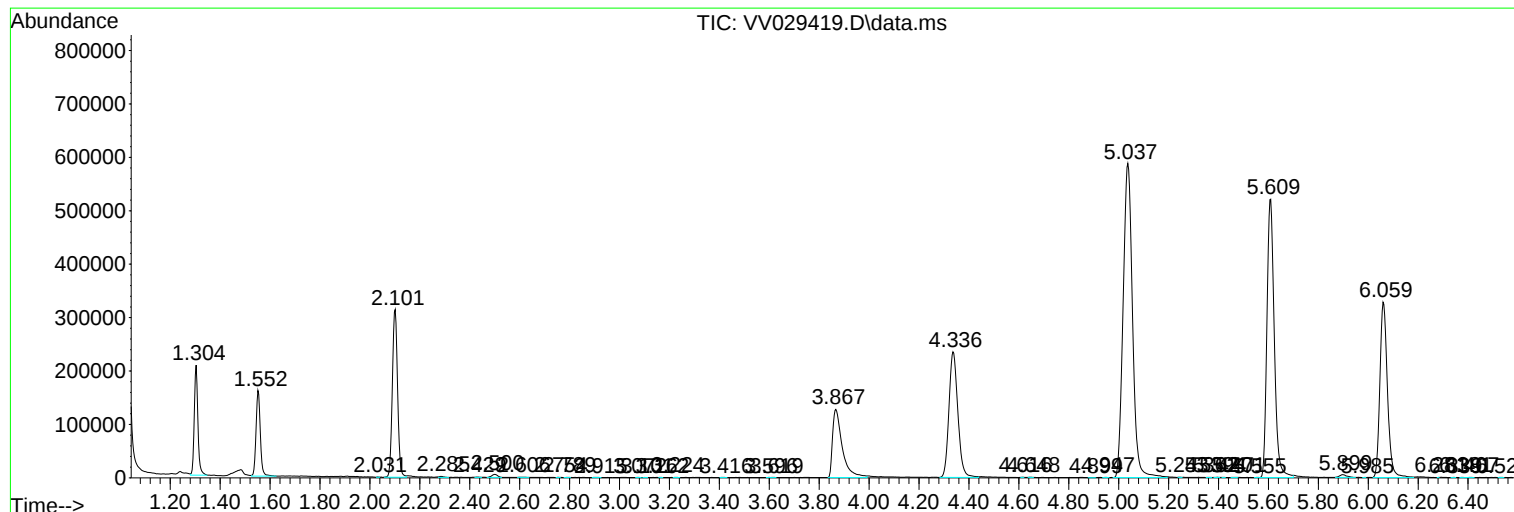

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029419.D
Acq On : 07 Dec 2022 15:58
Operator : SY/MD
Sample : VV1207MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK293

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029419.D
Acq On : 07 Dec 2022 15:58
Operator : SY/MD
Sample : VV1207MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK293

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc