

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029420.D
 Acq On : 07 Dec 2022 16:23
 Operator : SY/MD
 Sample : VV1207MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK294

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VV029420.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	219999	223494	13.89%	1.727%
2	1.552	151	159	185	rVB	170219	200063	12.44%	1.546%
3	2.098	318	329	345	rBV	339041	486553	30.25%	3.759%
4	2.285	379	387	395	rBV3	1626	2345	0.15%	0.018%
5	2.336	400	403	404	rBV	340	202	0.01%	0.002%
6	2.423	425	430	432	rBV	525	454	0.03%	0.004%
7	2.436	432	434	439	rVB3	541	421	0.03%	0.003%
8	2.500	445	454	464	rVB3	6877	10890	0.68%	0.084%
9	2.577	475	478	483	rVB2	295	245	0.02%	0.002%
10	2.651	496	501	504	rBV4	267	240	0.01%	0.002%
11	2.725	521	524	527	rBV2	307	229	0.01%	0.002%
12	2.754	530	533	540	rVV2	512	522	0.03%	0.004%
13	2.818	550	553	555	rVV2	266	189	0.01%	0.001%
14	2.851	559	563	566	rBV2	401	335	0.02%	0.003%
15	3.050	620	625	626	rBV2	270	219	0.01%	0.002%
16	3.220	675	678	683	rVV3	417	379	0.02%	0.003%
17	3.265	689	692	695	rVV2	335	229	0.01%	0.002%
18	3.288	696	699	704	rVB2	388	323	0.02%	0.002%
19	3.391	724	731	733	rBV	162	198	0.01%	0.002%
20	3.564	782	785	790	rVB3	291	244	0.02%	0.002%
21	3.770	845	849	854	rBV2	323	308	0.02%	0.002%
22	3.867	866	879	926	rBV	127160	347814	21.62%	2.687%
23	4.201	980	983	986	rBV2	277	216	0.01%	0.002%
24	4.336	1007	1025	1056	rBV	244044	613941	38.17%	4.743%
25	4.677	1128	1131	1134	rVB4	362	215	0.01%	0.002%
26	4.693	1134	1136	1142	rVB	340	248	0.02%	0.002%
27	4.722	1142	1145	1148	rBV2	353	251	0.02%	0.002%
28	4.889	1195	1197	1204	rVB4	214	198	0.01%	0.002%
29	5.037	1223	1243	1279	rBV2	617661	1608502	100.00%	12.426%
30	5.269	1311	1315	1318	rBV2	317	291	0.02%	0.002%
31	5.326	1331	1333	1336	rVB	371	187	0.01%	0.001%
32	5.394	1351	1354	1357	rVB3	371	236	0.01%	0.002%
33	5.432	1363	1366	1370	rVB3	291	188	0.01%	0.001%
34	5.606	1407	1420	1450	rBV	550284	1111678	69.11%	8.588%
35	5.899	1500	1511	1528	rVB6	4603	11198	0.70%	0.087%
36	6.011	1541	1546	1547	rBV2	338	254	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029420.D
 Acq On : 07 Dec 2022 16:23
 Operator : SY/MD
 Sample : VV1207MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK294

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.059	1547	1561	1594	rBV	348070	710054	44.14%	5.485%
38	6.362	1653	1655	1660	rBV4	255	228	0.01%	0.002%
39	6.619	1728	1735	1736	rBV4	1029	872	0.05%	0.007%
40	6.670	1748	1751	1753	rBV2	449	367	0.02%	0.003%
41	6.744	1770	1774	1777	rBV2	299	306	0.02%	0.002%
42	6.937	1830	1834	1835	rBV2	329	214	0.01%	0.002%
43	6.976	1835	1846	1877	rVV	204760	374882	23.31%	2.896%
44	7.149	1895	1900	1902	rBV2	652	700	0.04%	0.005%
45	7.252	1929	1932	1934	rBV2	693	462	0.03%	0.004%
46	7.307	1936	1949	1990	rVV	773192	1369222	85.12%	10.578%
47	7.612	2033	2044	2072	rBV	140120	247164	15.37%	1.909%
48	7.915	2134	2138	2140	rBV	318	283	0.02%	0.002%
49	8.082	2179	2190	2227	rBV	457935	809468	50.32%	6.253%
50	8.371	2278	2280	2285	rVB3	440	328	0.02%	0.003%
51	8.702	2378	2383	2386	rBV2	248	207	0.01%	0.002%
52	8.844	2414	2427	2455	rBV	792652	1300336	80.84%	10.045%
53	9.088	2499	2503	2505	rVB4	363	221	0.01%	0.002%
54	9.130	2512	2516	2522	rVB4	670	791	0.05%	0.006%
55	9.300	2567	2569	2573	rVB2	501	368	0.02%	0.003%
56	9.426	2602	2608	2611	rBV4	343	388	0.02%	0.003%
57	9.538	2637	2643	2647	rBV4	497	533	0.03%	0.004%
58	9.561	2647	2650	2656	rVV4	698	741	0.05%	0.006%
59	9.603	2660	2663	2666	rVB	301	191	0.01%	0.001%
60	9.654	2676	2679	2682	rBV2	267	214	0.01%	0.002%
61	9.924	2756	2763	2768	rVB5	622	822	0.05%	0.006%
62	9.956	2769	2773	2775	rBV2	384	276	0.02%	0.002%
63	9.989	2780	2783	2789	rVB2	420	348	0.02%	0.003%
64	10.027	2793	2795	2799	rBV3	368	267	0.02%	0.002%
65	10.053	2799	2803	2805	rVB3	371	213	0.01%	0.002%
66	10.207	2838	2851	2872	rBV	537330	840704	52.27%	6.495%
67	10.288	2874	2876	2879	rVB	471	223	0.01%	0.002%
68	10.362	2897	2899	2903	rVV2	421	327	0.02%	0.003%
69	10.458	2926	2929	2931	rBV2	336	225	0.01%	0.002%
70	10.571	2962	2964	2968	rVB2	547	341	0.02%	0.003%
71	10.603	2968	2974	2979	rBV3	348	399	0.02%	0.003%
72	10.661	2990	2992	2996	rVB	323	219	0.01%	0.002%
73	10.696	2996	3003	3004	rBV3	451	485	0.03%	0.004%
74	10.818	3037	3041	3044	rBV2	437	457	0.03%	0.004%
75	10.850	3048	3051	3055	rVB3	301	208	0.01%	0.002%
76	10.905	3065	3068	3073	rVB2	525	458	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029420.D
 Acq On : 07 Dec 2022 16:23
 Operator : SY/MD
 Sample : VV1207MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK294

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.172	3146	3151	3158	rVB4	1098	1474	0.09%	0.011%
78	11.239	3159	3172	3193	rBV	870028	1354788	84.23%	10.466%
79	11.532	3258	3263	3266	rBV2	377	366	0.02%	0.003%
80	11.612	3275	3288	3317	rVV	823281	1291274	80.28%	9.975%
81	11.834	3355	3357	3359	rBV3	409	200	0.01%	0.002%
82	11.924	3382	3385	3387	rBV2	370	223	0.01%	0.002%
83	12.024	3413	3416	3421	rBV3	449	276	0.02%	0.002%
84	12.214	3473	3475	3478	rBV2	373	265	0.02%	0.002%
85	12.278	3491	3495	3500	rBV5	532	600	0.04%	0.005%
86	12.397	3529	3532	3536	rBV4	400	268	0.02%	0.002%
87	12.419	3536	3539	3541	rBV3	528	328	0.02%	0.003%
88	12.493	3559	3562	3567	rBV3	352	292	0.02%	0.002%
89	12.525	3569	3572	3574	rVB3	520	301	0.02%	0.002%
90	12.542	3574	3577	3579	rBV2	377	248	0.02%	0.002%
91	12.580	3585	3589	3591	rBV3	370	274	0.02%	0.002%
92	12.596	3591	3594	3597	rVB3	543	334	0.02%	0.003%
93	12.612	3597	3599	3601	rBV2	383	218	0.01%	0.002%
94	12.696	3623	3625	3631	rBV	363	387	0.02%	0.003%
95	12.812	3657	3661	3663	rBV2	712	456	0.03%	0.004%
96	12.853	3671	3674	3677	rBV3	503	314	0.02%	0.002%
97	12.879	3680	3682	3685	rBV	337	211	0.01%	0.002%
98	13.033	3727	3730	3733	rBV3	440	384	0.02%	0.003%
99	13.249	3791	3797	3803	rBV4	2070	2811	0.17%	0.022%
100	13.300	3811	3813	3816	rBV2	474	336	0.02%	0.003%


Sum of corrected areas: 12944639

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029420.D
Acq On : 07 Dec 2022 16:23
Operator : SY/MD
Sample : VV1207MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK294

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

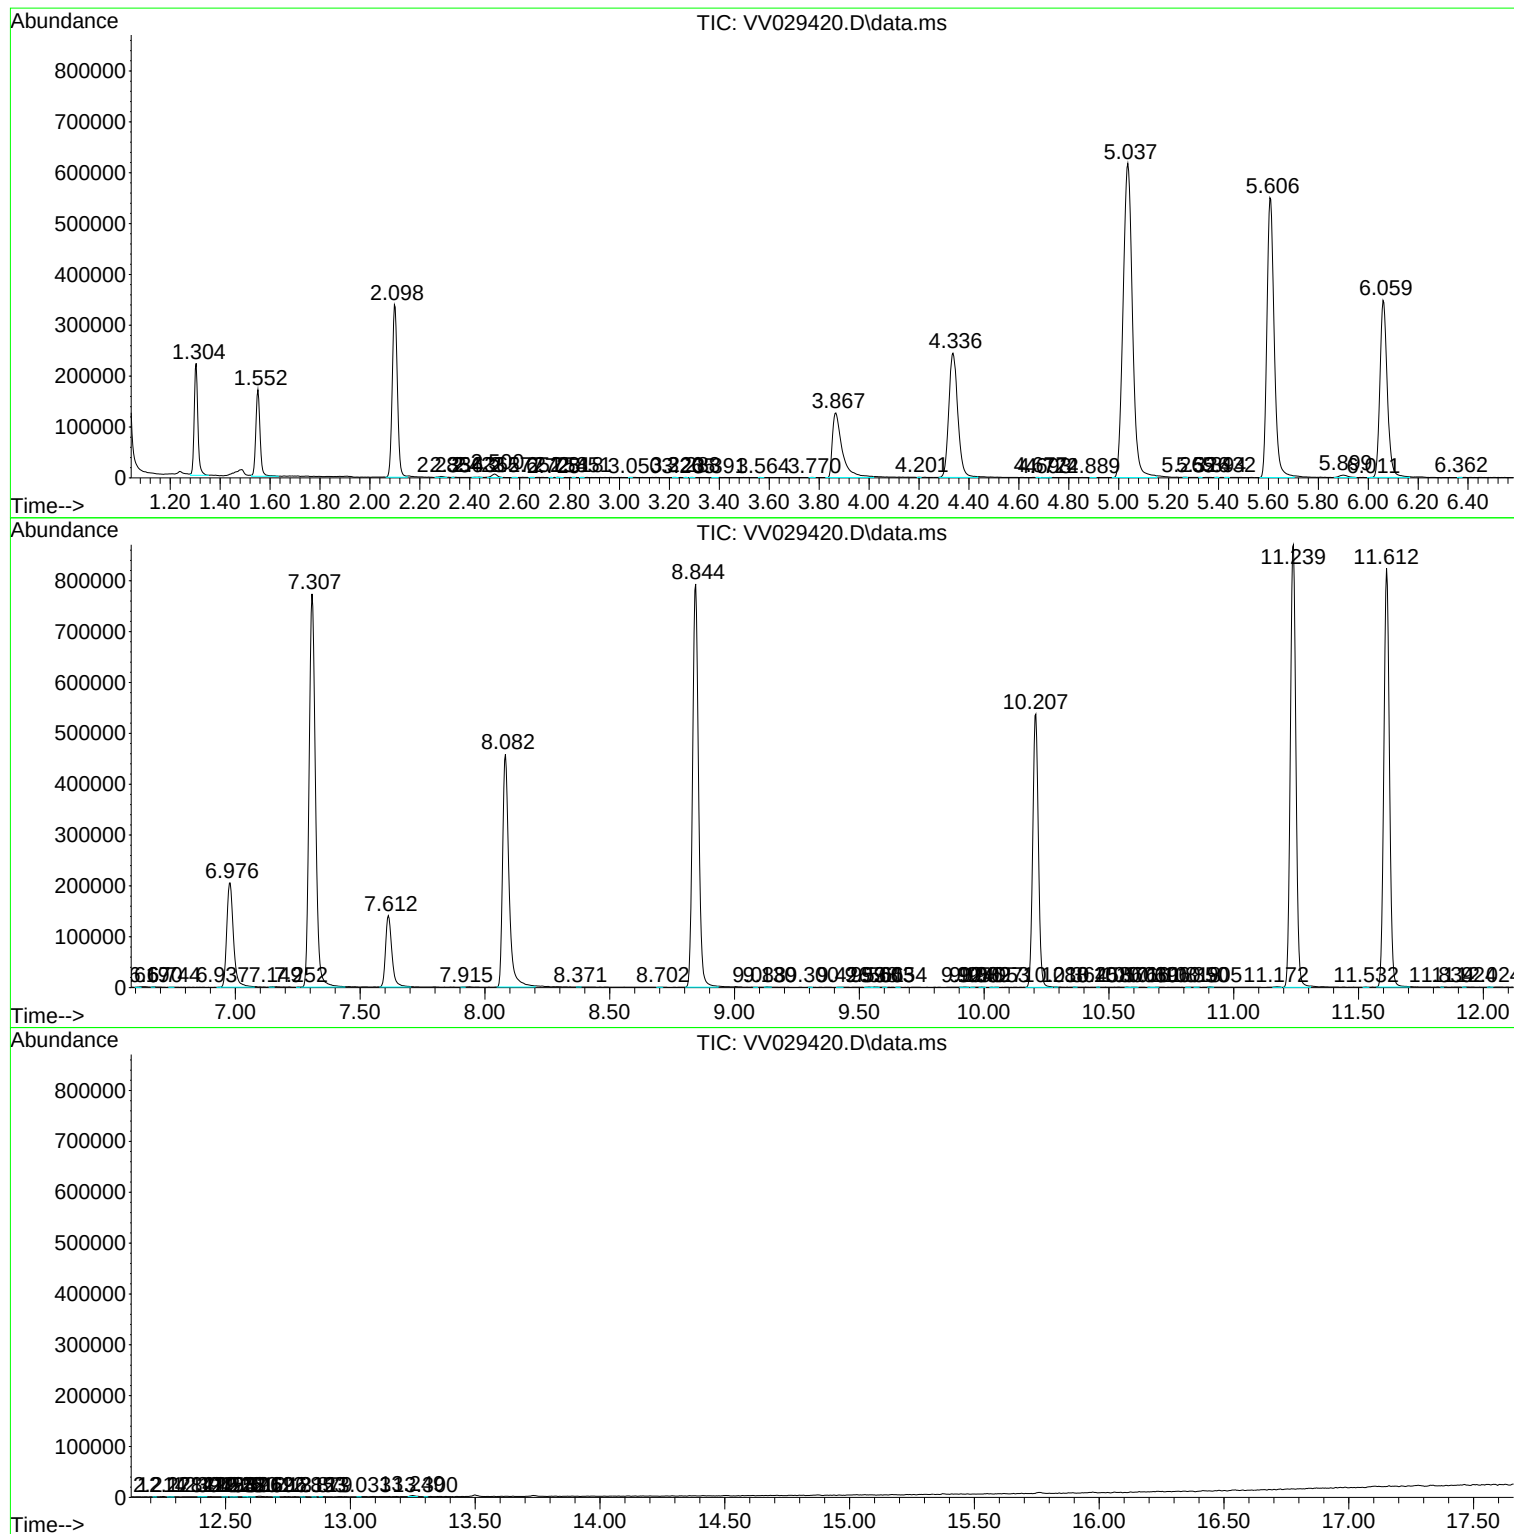

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029420.D
Acq On : 07 Dec 2022 16:23
Operator : SY/MD
Sample : VV1207MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK294

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029420.D
Acq On : 07 Dec 2022 16:23
Operator : SY/MD
Sample : VV1207MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK294

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc