

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029421.D
 Acq On : 07 Dec 2022 16:47
 Operator : SY/MD
 Sample : VV1207MBL03
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK295

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	211269	209510	13.77%	1.716%
2	1.561	154	162	178	rVB	162529	182444	11.99%	1.494%
3	1.966	286	288	290	rVB2	847	374	0.02%	0.003%
4	2.101	320	330	349	rBV	305652	445522	29.28%	3.649%
5	2.288	382	388	397	rVB3	1619	2603	0.17%	0.021%
6	2.500	446	454	467	rVB3	6363	10218	0.67%	0.084%
7	2.619	489	491	496	rVB2	541	341	0.02%	0.003%
8	2.780	538	541	545	rVV2	318	278	0.02%	0.002%
9	2.915	580	583	586	rVB2	375	279	0.02%	0.002%
10	2.973	598	601	605	rVB3	343	245	0.02%	0.002%
11	3.037	616	621	625	rVB2	326	270	0.02%	0.002%
12	3.166	656	661	663	rVV2	241	238	0.02%	0.002%
13	3.179	663	665	671	rVV3	398	311	0.02%	0.003%
14	3.211	671	675	678	rVV3	306	319	0.02%	0.003%
15	3.285	696	698	703	rVB3	239	227	0.01%	0.002%
16	3.510	763	768	771	rVV	342	254	0.02%	0.002%
17	3.645	806	810	816	rVB2	304	272	0.02%	0.002%
18	3.867	869	879	923	rBV	129234	351840	23.12%	2.882%
19	4.217	985	988	992	rBV4	348	259	0.02%	0.002%
20	4.339	1008	1026	1051	rBV	231289	579544	38.09%	4.747%
21	4.564	1092	1096	1098	rVB2	450	325	0.02%	0.003%
22	4.613	1108	1111	1113	rBV3	315	229	0.02%	0.002%
23	4.950	1212	1216	1221	rBV3	338	376	0.02%	0.003%
24	5.040	1224	1244	1287	rBV2	575394	1521640	100.00%	12.464%
25	5.487	1378	1383	1385	rVV	232	228	0.01%	0.002%
26	5.609	1407	1421	1463	rBV	513412	1052738	69.18%	8.623%
27	5.896	1501	1510	1522	rBV4	4883	9824	0.65%	0.080%
28	6.063	1548	1562	1598	rBV	327336	679822	44.68%	5.569%
29	6.195	1601	1603	1605	rBV2	499	309	0.02%	0.003%
30	6.314	1637	1640	1643	rVB4	387	236	0.02%	0.002%
31	6.362	1651	1655	1656	rBV	518	345	0.02%	0.003%
32	6.371	1656	1658	1664	rVB2	376	222	0.01%	0.002%
33	6.468	1686	1688	1691	rVB2	472	230	0.02%	0.002%
34	6.519	1700	1704	1706	rVB3	401	269	0.02%	0.002%
35	6.616	1725	1734	1735	rBV3	1172	1091	0.07%	0.009%
36	6.751	1773	1776	1780	rBV3	342	268	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029421.D
 Acq On : 07 Dec 2022 16:47
 Operator : SY/MD
 Sample : VV1207MBL03
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK295

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.831	1797	1801	1804	rVB2	300	242	0.02%	0.002%
38	6.854	1804	1808	1811	rBV3	380	357	0.02%	0.003%
39	6.979	1835	1847	1878	rBV	194162	362101	23.80%	2.966%
40	7.143	1894	1898	1900	rBV3	536	358	0.02%	0.003%
41	7.307	1936	1949	1978	rBV	718754	1283102	84.32%	10.510%
42	7.535	2017	2020	2023	rBV2	459	260	0.02%	0.002%
43	7.613	2034	2044	2074	rBV	134182	236503	15.54%	1.937%
44	7.818	2106	2108	2112	rVB4	416	329	0.02%	0.003%
45	7.931	2140	2143	2152	rVB3	828	960	0.06%	0.008%
46	8.082	2179	2190	2229	rBV	447593	798442	52.47%	6.540%
47	8.375	2278	2281	2283	rBV2	367	240	0.02%	0.002%
48	8.391	2283	2286	2290	rVV4	355	351	0.02%	0.003%
49	8.416	2293	2294	2298	rVB3	464	254	0.02%	0.002%
50	8.567	2339	2341	2345	rVB2	372	249	0.02%	0.002%
51	8.670	2369	2373	2376	rBV2	298	252	0.02%	0.002%
52	8.844	2414	2427	2466	rBV	738772	1214344	79.80%	9.947%
53	9.066	2491	2496	2499	rVV4	403	349	0.02%	0.003%
54	9.085	2499	2502	2509	rVB3	290	234	0.02%	0.002%
55	9.140	2514	2519	2521	rBV3	656	551	0.04%	0.005%
56	9.272	2556	2560	2563	rBV3	317	238	0.02%	0.002%
57	9.445	2606	2614	2615	rBV	229	225	0.01%	0.002%
58	9.535	2638	2642	2645	rBV3	496	439	0.03%	0.004%
59	9.600	2658	2662	2667	rBV4	274	268	0.02%	0.002%
60	9.690	2686	2690	2695	rVB2	401	326	0.02%	0.003%
61	9.719	2695	2699	2701	rBV2	401	275	0.02%	0.002%
62	9.792	2719	2722	2727	rVB2	314	247	0.02%	0.002%
63	9.889	2749	2752	2754	rBV2	417	262	0.02%	0.002%
64	9.928	2758	2764	2765	rBV3	417	318	0.02%	0.003%
65	9.966	2772	2776	2781	rBV2	265	350	0.02%	0.003%
66	10.050	2798	2802	2809	rVB3	285	300	0.02%	0.002%
67	10.137	2825	2829	2830	rBV2	359	284	0.02%	0.002%
68	10.207	2839	2851	2872	rBV	505344	793799	52.17%	6.502%
69	10.455	2924	2928	2931	rBV3	246	222	0.01%	0.002%
70	10.532	2946	2952	2959	rBV5	516	847	0.06%	0.007%
71	10.567	2960	2963	2967	rVV2	267	221	0.01%	0.002%
72	10.654	2985	2990	2999	rVB4	369	554	0.04%	0.005%
73	10.841	3046	3048	3052	rVB3	479	278	0.02%	0.002%
74	10.905	3065	3068	3076	rBV3	673	974	0.06%	0.008%
75	11.040	3106	3110	3111	rBV2	515	403	0.03%	0.003%
76	11.085	3120	3124	3129	rVB2	627	441	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029421.D
 Acq On : 07 Dec 2022 16:47
 Operator : SY/MD
 Sample : VV1207MBL03
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK295

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.117	3129	3134	3136	rBV3	367	238	0.02%	0.002%
78	11.149	3137	3144	3146	rBV4	423	491	0.03%	0.004%
79	11.175	3147	3152	3158	rVB3	908	1097	0.07%	0.009%
80	11.239	3158	3172	3192	rBV	812592	1244466	81.78%	10.194%
81	11.503	3247	3254	3257	rBV2	479	488	0.03%	0.004%
82	11.612	3274	3288	3318	rBV	755047	1193664	78.45%	9.777%
83	11.860	3361	3365	3369	rVB4	372	337	0.02%	0.003%
84	11.889	3369	3374	3376	rBV3	487	383	0.03%	0.003%
85	11.918	3378	3383	3388	rBV3	336	434	0.03%	0.004%
86	12.062	3425	3428	3432	rBV3	532	386	0.03%	0.003%
87	12.352	3515	3518	3521	rBV2	541	428	0.03%	0.004%
88	12.407	3533	3535	3539	rVB3	449	288	0.02%	0.002%
89	12.554	3576	3581	3587	rVB3	408	468	0.03%	0.004%
90	12.779	3648	3651	3654	rBV	277	263	0.02%	0.002%
91	12.924	3693	3696	3697	rBV2	516	293	0.02%	0.002%
92	12.943	3700	3702	3706	rVB2	499	331	0.02%	0.003%
93	13.149	3764	3766	3769	rBV3	344	225	0.01%	0.002%
94	13.169	3769	3772	3776	rVB3	765	569	0.04%	0.005%
95	13.204	3780	3783	3787	rVB3	438	351	0.02%	0.003%
96	13.252	3792	3798	3806	rVB8	1721	2832	0.19%	0.023%
97	13.387	3835	3840	3844	rBV4	665	771	0.05%	0.006%
98	13.497	3867	3874	3882	rBV3	2044	3422	0.22%	0.028%
99	14.030	4032	4040	4044	rBV8	885	1379	0.09%	0.011%
100	14.374	4145	4147	4150	rBV2	904	464	0.03%	0.004%




Sum of corrected areas: 12208317

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029421.D
Acq On : 07 Dec 2022 16:47
Operator : SY/MD
Sample : VV1207MBL03
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK295

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

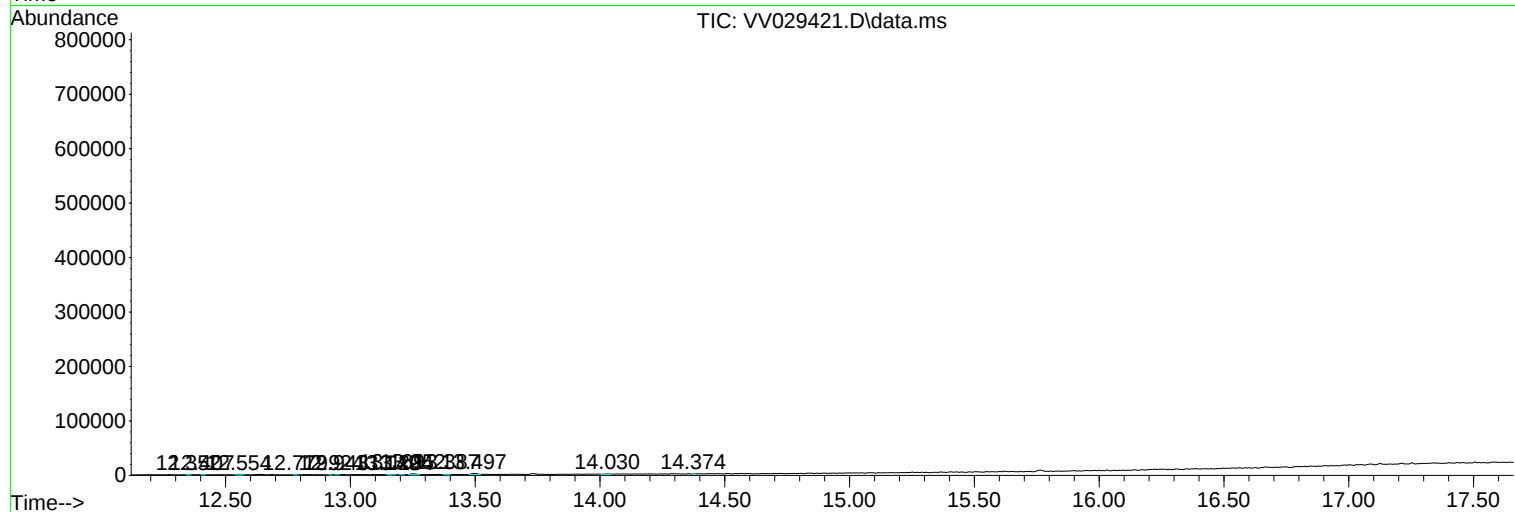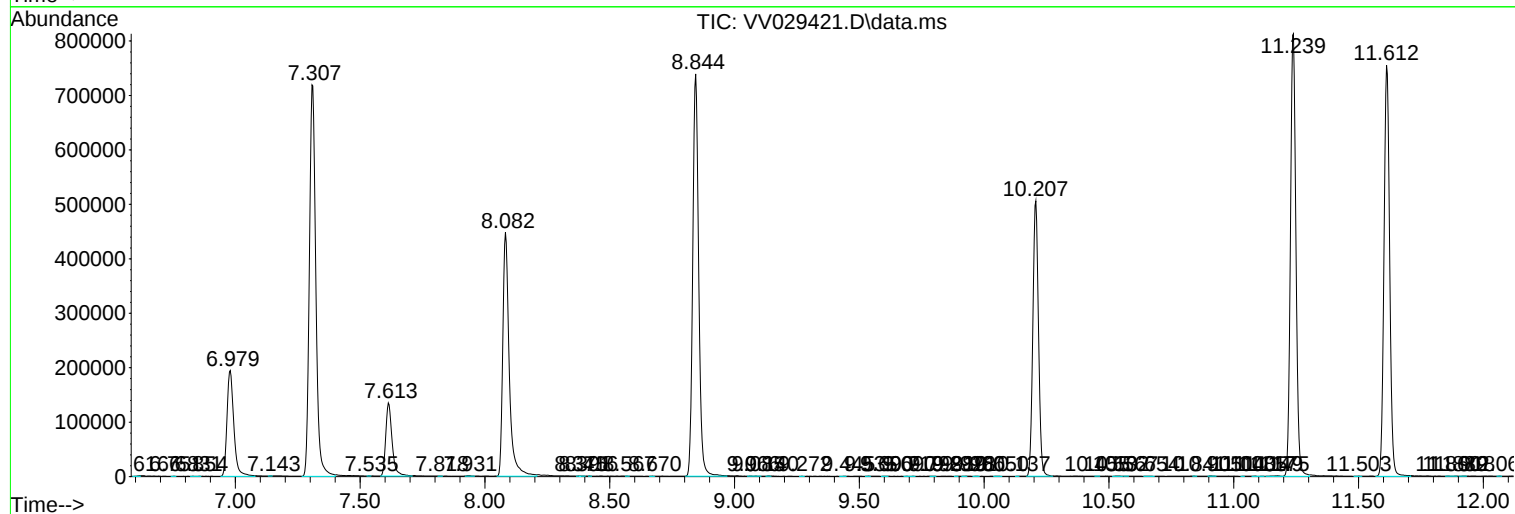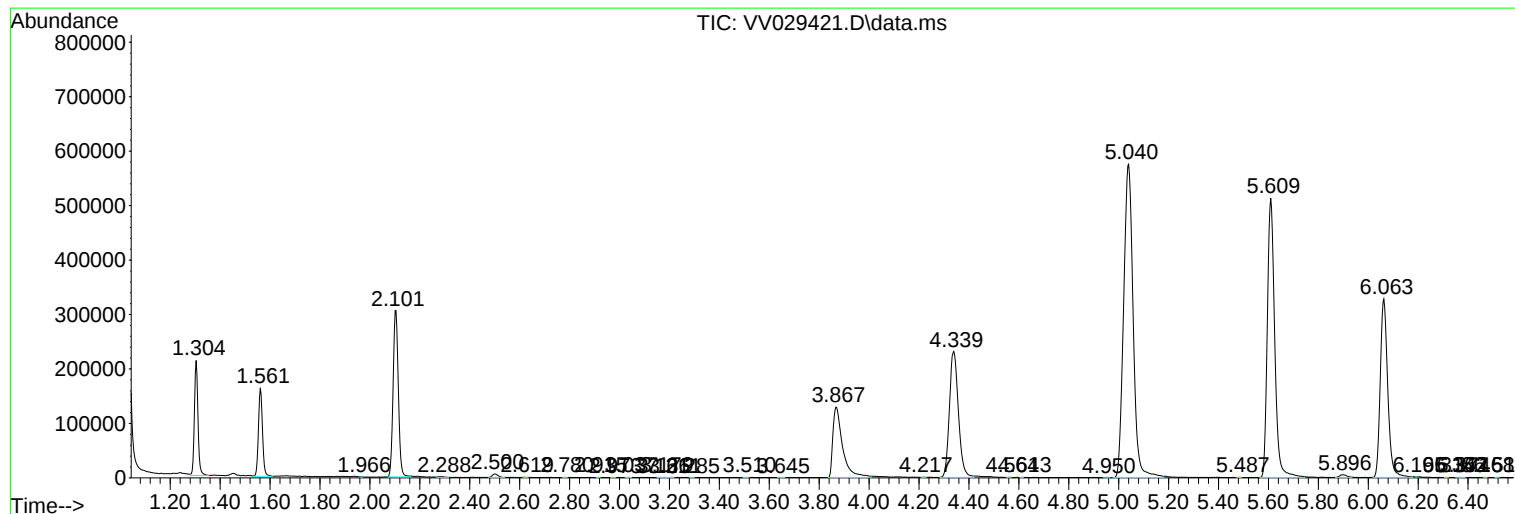

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029421.D
Acq On : 07 Dec 2022 16:47
Operator : SY/MD
Sample : VV1207MBL03
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK295

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029421.D
Acq On : 07 Dec 2022 16:47
Operator : SY/MD
Sample : VV1207MBL03
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK295

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc