

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029428.D
 Acq On : 07 Dec 2022 19:31
 Operator : SY/MD
 Sample : N5894-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029428.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	225708	219039	14.06%	1.714%
2	1.561	154	162	178	rVB	166422	189450	12.16%	1.483%
3	2.040	308	311	315	rBV3	310	239	0.02%	0.002%
4	2.105	319	331	344	rBV	323343	462793	29.70%	3.622%
5	2.288	381	388	395	rVB2	2683	3432	0.22%	0.027%
6	2.458	438	441	444	rVV2	439	351	0.02%	0.003%
7	2.503	448	455	465	rVB4	1228	1928	0.12%	0.015%
8	2.561	470	473	476	rBV2	370	223	0.01%	0.002%
9	2.616	485	490	494	rBV2	620	875	0.06%	0.007%
10	2.764	529	536	541	rBV6	715	939	0.06%	0.007%
11	2.995	606	608	613	rVB	377	251	0.02%	0.002%
12	3.249	684	687	695	rVB	384	446	0.03%	0.003%
13	3.597	793	795	801	rVB2	305	262	0.02%	0.002%
14	3.667	814	817	820	rBV2	315	213	0.01%	0.002%
15	3.870	869	880	920	rBV	126041	350227	22.48%	2.741%
16	4.339	1004	1026	1067	rBV	241536	601543	38.61%	4.708%
17	4.603	1104	1108	1112	rVB4	488	408	0.03%	0.003%
18	4.667	1123	1128	1133	rBV3	543	593	0.04%	0.005%
19	4.812	1166	1173	1174	rBV3	406	402	0.03%	0.003%
20	4.825	1174	1177	1184	rVB3	424	427	0.03%	0.003%
21	4.931	1206	1210	1218	rBV2	275	249	0.02%	0.002%
22	5.040	1224	1244	1283	rBV2	592255	1558089	100.00%	12.195%
23	5.262	1310	1313	1319	rBV3	290	242	0.02%	0.002%
24	5.394	1350	1354	1359	rBV3	335	333	0.02%	0.003%
25	5.474	1372	1379	1382	rBV4	448	446	0.03%	0.003%
26	5.552	1398	1403	1407	rBV3	414	379	0.02%	0.003%
27	5.609	1407	1421	1464	rBV	554906	1132958	72.71%	8.868%
28	5.899	1501	1511	1525	rVB8	4211	9266	0.59%	0.073%
29	5.963	1528	1531	1535	rBV	256	213	0.01%	0.002%
30	6.011	1541	1546	1548	rBV3	245	293	0.02%	0.002%
31	6.063	1548	1562	1590	rBV	337730	691394	44.37%	5.412%
32	6.410	1668	1670	1675	rBV3	284	242	0.02%	0.002%
33	6.513	1696	1702	1704	rBV2	317	273	0.02%	0.002%
34	6.580	1719	1723	1726	rBV2	248	263	0.02%	0.002%
35	6.629	1730	1738	1745	rVB5	886	1613	0.10%	0.013%
36	6.741	1771	1773	1777	rVB3	572	364	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029428.D
 Acq On : 07 Dec 2022 19:31
 Operator : SY/MD
 Sample : N5894-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.767	1777	1781	1784	rBV2	286	244	0.02%	0.002%
38	6.789	1784	1788	1790	rVB	330	226	0.01%	0.002%
39	6.979	1835	1847	1885	rVV	194588	367023	23.56%	2.873%
40	7.146	1893	1899	1903	rBV3	687	968	0.06%	0.008%
41	7.310	1937	1950	1979	rBV	739986	1309789	84.06%	10.252%
42	7.558	2025	2027	2032	rVB	319	264	0.02%	0.002%
43	7.613	2032	2044	2074	rBV	135089	239861	15.39%	1.877%
44	7.754	2086	2088	2093	rVB4	396	223	0.01%	0.002%
45	7.860	2117	2121	2124	rBV2	349	284	0.02%	0.002%
46	7.934	2131	2144	2154	rBV	15918	30545	1.96%	0.239%
47	8.082	2179	2190	2228	rBV	433424	781843	50.18%	6.120%
48	8.455	2303	2306	2310	rBV4	508	533	0.03%	0.004%
49	8.596	2345	2350	2351	rBV2	367	276	0.02%	0.002%
50	8.677	2372	2375	2381	rBV3	302	270	0.02%	0.002%
51	8.844	2415	2427	2464	rBV	802464	1313520	84.30%	10.281%
52	9.011	2474	2479	2484	rVB6	1264	1405	0.09%	0.011%
53	9.130	2513	2516	2527	rVB5	1440	2186	0.14%	0.017%
54	9.239	2547	2550	2555	rBV3	282	255	0.02%	0.002%
55	9.278	2559	2562	2567	rVB2	263	259	0.02%	0.002%
56	9.352	2582	2585	2589	rVB	343	297	0.02%	0.002%
57	9.384	2589	2595	2597	rBV	331	259	0.02%	0.002%
58	9.410	2599	2603	2605	rBV	353	285	0.02%	0.002%
59	9.445	2610	2614	2620	rVB3	493	462	0.03%	0.004%
60	9.535	2636	2642	2643	rBV2	1035	813	0.05%	0.006%
61	9.677	2682	2686	2694	rVB2	319	376	0.02%	0.003%
62	9.712	2694	2697	2703	rBV3	387	470	0.03%	0.004%
63	9.805	2723	2726	2730	rBV2	273	245	0.02%	0.002%
64	9.841	2734	2737	2742	rVV3	210	228	0.01%	0.002%
65	9.921	2756	2762	2771	rVB4	1252	2024	0.13%	0.016%
66	9.960	2771	2774	2777	rBV2	253	248	0.02%	0.002%
67	10.207	2835	2851	2871	rBV	505623	803628	51.58%	6.290%
68	10.313	2881	2884	2887	rBV3	408	250	0.02%	0.002%
69	10.374	2891	2903	2914	rVB	19431	32516	2.09%	0.255%
70	10.426	2914	2919	2922	rBV4	421	398	0.03%	0.003%
71	10.532	2945	2952	2960	rVB3	1259	1691	0.11%	0.013%
72	10.645	2981	2987	2991	rBV3	444	535	0.03%	0.004%
73	10.776	3023	3028	3035	rVB3	400	453	0.03%	0.004%
74	10.870	3055	3057	3061	rBV3	291	234	0.02%	0.002%
75	10.908	3062	3069	3077	rBV3	1315	1906	0.12%	0.015%
76	11.018	3097	3103	3107	rBV4	508	603	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029428.D
 Acq On : 07 Dec 2022 19:31
 Operator : SY/MD
 Sample : N5894-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.046	3109	3112	3116	rVV2	274	253	0.02%	0.002%
78	11.088	3116	3125	3135	rVV2	7681	11620	0.75%	0.091%
79	11.172	3144	3151	3152	rBV5	1605	1425	0.09%	0.011%
80	11.239	3153	3172	3191	rVV	883764	1358835	87.21%	10.636%
81	11.432	3227	3232	3233	rVB2	387	264	0.02%	0.002%
82	11.461	3238	3241	3248	rBV3	295	338	0.02%	0.003%
83	11.612	3275	3288	3314	rBV	782350	1239644	79.56%	9.703%
84	11.892	3372	3375	3379	rVB4	374	332	0.02%	0.003%
85	12.021	3412	3415	3418	rBV2	408	275	0.02%	0.002%
86	12.098	3435	3439	3442	rVB2	658	454	0.03%	0.004%
87	12.239	3472	3483	3495	rVV4	5304	8775	0.56%	0.069%
88	12.317	3505	3507	3509	rBV2	371	227	0.01%	0.002%
89	12.374	3521	3525	3527	rBV2	405	296	0.02%	0.002%
90	12.635	3597	3606	3616	rBV5	2430	3505	0.22%	0.027%
91	12.706	3624	3628	3638	rVB3	431	556	0.04%	0.004%
92	12.747	3638	3641	3644	rBV2	288	224	0.01%	0.002%
93	12.837	3665	3669	3670	rBV2	480	296	0.02%	0.002%
94	13.136	3759	3762	3763	rBV3	387	219	0.01%	0.002%
95	13.249	3790	3797	3809	rVB5	2564	4411	0.28%	0.035%
96	13.336	3821	3824	3828	rBV5	550	366	0.02%	0.003%
97	13.448	3854	3859	3860	rBV3	571	487	0.03%	0.004%
98	13.497	3866	3874	3887	rVB2	5747	9493	0.61%	0.074%
99	13.731	3941	3947	3957	rVB4	3237	4883	0.31%	0.038%
100	13.995	4027	4029	4033	rBV4	536	405	0.03%	0.003%




Sum of corrected areas: 12776136

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029428.D
Acq On : 07 Dec 2022 19:31
Operator : SY/MD
Sample : N5894-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

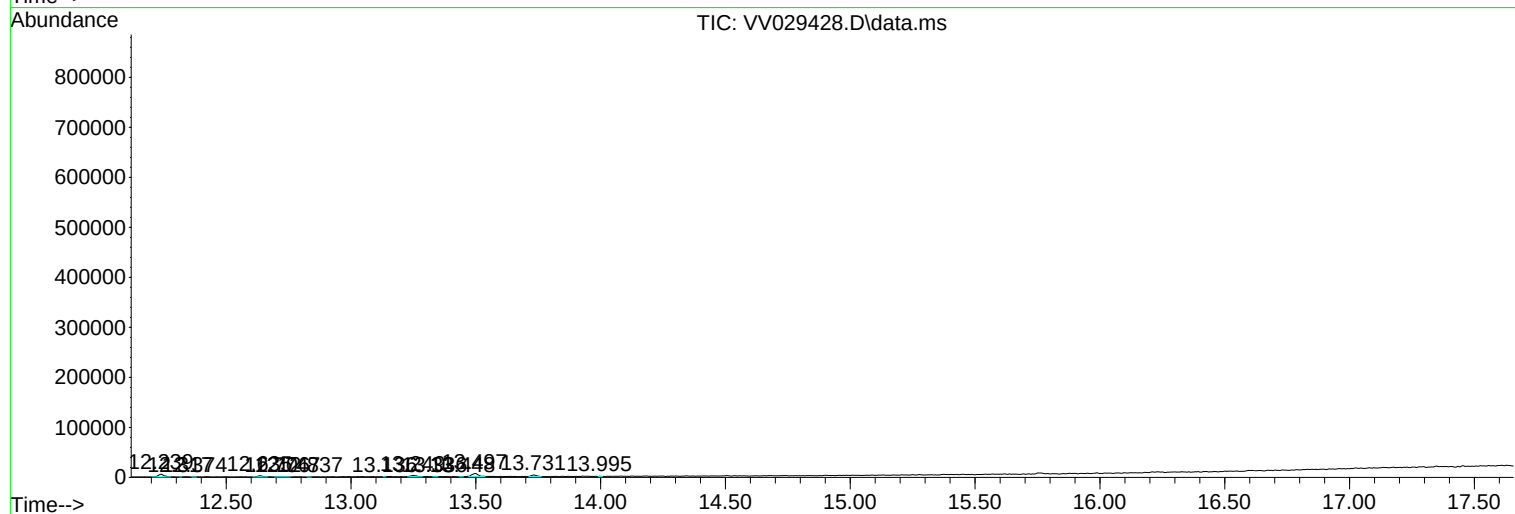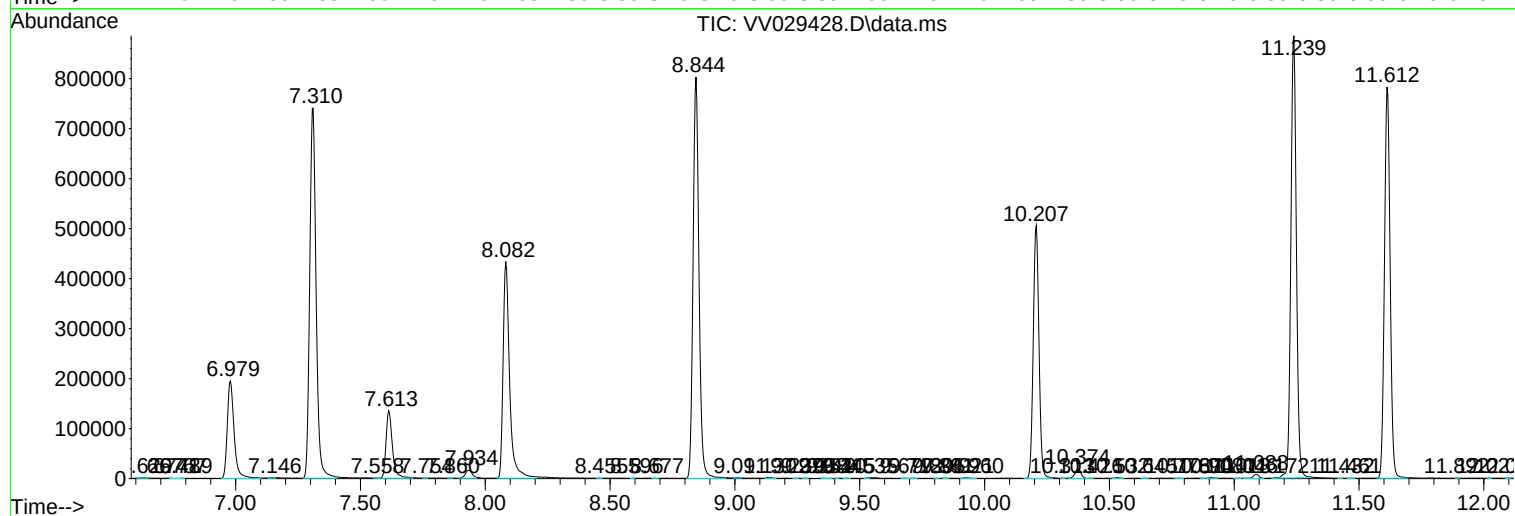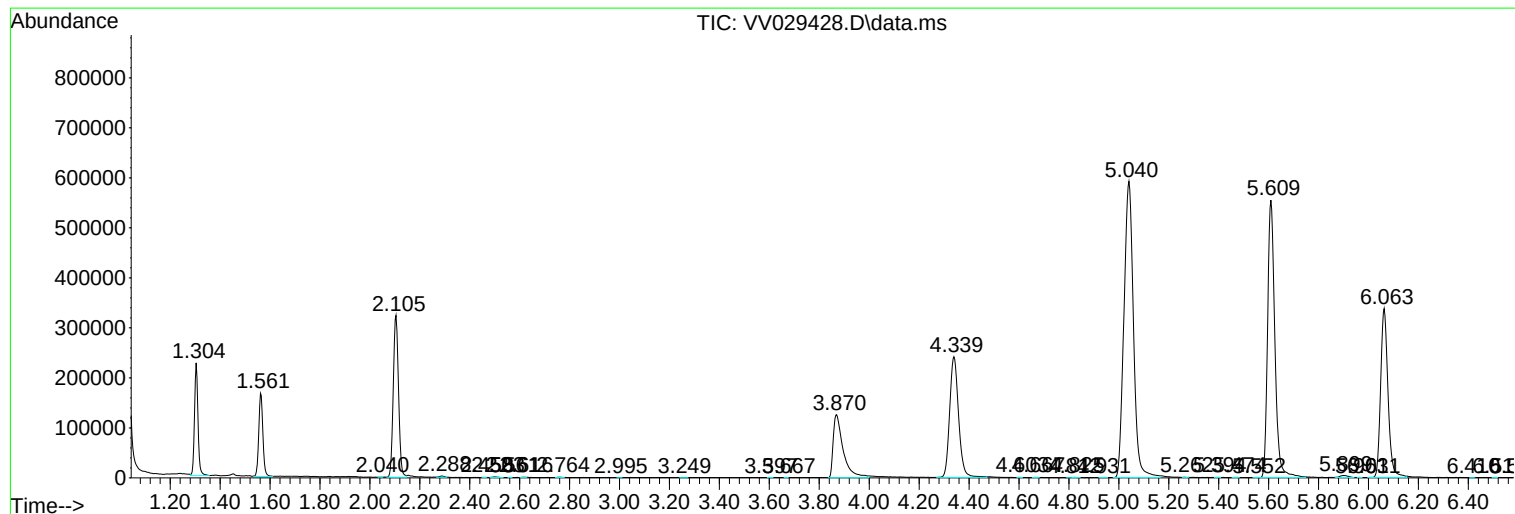

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029428.D
Acq On : 07 Dec 2022 19:31
Operator : SY/MD
Sample : N5894-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029428.D
Acq On : 07 Dec 2022 19:31
Operator : SY/MD
Sample : N5894-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------