

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029429.D
 Acq On : 07 Dec 2022 19:55
 Operator : SY/MD
 Sample : N5894-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029429.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	220750	214265	13.09%	1.635%
2	1.561	154	162	177	rBV	172970	196232	11.99%	1.497%
3	2.005	295	300	301	rBV	619	557	0.03%	0.004%
4	2.044	309	312	315	rBV2	464	334	0.02%	0.003%
5	2.105	320	331	343	rBV	334788	480819	29.37%	3.668%
6	2.291	379	389	398	rVB3	3448	5897	0.36%	0.045%
7	2.407	423	425	435	rVB2	351	363	0.02%	0.003%
8	2.474	438	446	448	rBV3	419	538	0.03%	0.004%
9	2.503	448	455	460	rBV5	1049	1689	0.10%	0.013%
10	2.626	486	493	494	rBV3	279	309	0.02%	0.002%
11	2.687	506	512	514	rBV	310	341	0.02%	0.003%
12	2.812	548	551	558	rVB2	328	299	0.02%	0.002%
13	2.912	575	582	584	rBV3	259	292	0.02%	0.002%
14	3.044	616	623	628	rBV2	340	344	0.02%	0.003%
15	3.101	636	641	647	rBV3	242	295	0.02%	0.002%
16	3.191	665	669	672	rVB2	337	218	0.01%	0.002%
17	3.391	729	731	736	rVB2	252	222	0.01%	0.002%
18	3.555	776	782	788	rVB2	233	253	0.02%	0.002%
19	3.867	869	879	929	rBV	127918	354489	21.66%	2.705%
20	4.224	987	990	994	rBV3	414	392	0.02%	0.003%
21	4.339	1008	1026	1055	rBV	249963	622769	38.05%	4.751%
22	4.587	1099	1103	1105	rVB2	325	265	0.02%	0.002%
23	4.629	1114	1116	1123	rVB3	283	320	0.02%	0.002%
24	4.683	1131	1133	1137	rVB2	532	332	0.02%	0.003%
25	4.921	1203	1207	1211	rVB3	339	244	0.01%	0.002%
26	5.040	1225	1244	1297	rBV2	613597	1636845	100.00%	12.488%
27	5.233	1302	1304	1307	rBV3	370	238	0.01%	0.002%
28	5.407	1353	1358	1360	rVV3	350	245	0.01%	0.002%
29	5.548	1397	1402	1407	rBV2	554	523	0.03%	0.004%
30	5.609	1408	1421	1448	rBV	552013	1119858	68.42%	8.544%
31	5.899	1502	1511	1525	rVV4	4324	8623	0.53%	0.066%
32	6.063	1548	1562	1597	rBV	349489	729250	44.55%	5.564%
33	6.236	1614	1616	1619	rBV4	429	243	0.01%	0.002%
34	6.391	1660	1664	1668	rVB2	245	234	0.01%	0.002%
35	6.413	1668	1671	1674	rVB2	334	245	0.01%	0.002%
36	6.471	1686	1689	1692	rBV2	236	208	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029429.D
 Acq On : 07 Dec 2022 19:55
 Operator : SY/MD
 Sample : N5894-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.558	1714	1716	1722	rVB2	214	208	0.01%	0.002%
38	6.619	1727	1735	1748	rBV5	1454	3346	0.20%	0.026%
39	6.674	1748	1752	1754	rVV3	337	371	0.02%	0.003%
40	6.850	1804	1807	1811	rVB2	247	228	0.01%	0.002%
41	6.912	1825	1826	1832	rVB	263	278	0.02%	0.002%
42	6.979	1835	1847	1878	rBV	208490	382388	23.36%	2.917%
43	7.146	1893	1899	1903	rBV8	836	1124	0.07%	0.009%
44	7.220	1919	1922	1924	rVB2	402	241	0.01%	0.002%
45	7.233	1924	1926	1930	rVB2	639	398	0.02%	0.003%
46	7.307	1933	1949	1989	rBV	776957	1384088	84.56%	10.560%
47	7.612	2033	2044	2071	rBV	141593	250755	15.32%	1.913%
48	7.838	2111	2114	2118	rVB2	463	293	0.02%	0.002%
49	7.937	2131	2145	2158	rBV2	8555	15813	0.97%	0.121%
50	8.082	2179	2190	2235	rBV	445080	812396	49.63%	6.198%
51	8.362	2274	2277	2281	rBV4	347	304	0.02%	0.002%
52	8.384	2282	2284	2287	rBV2	376	211	0.01%	0.002%
53	8.461	2306	2308	2311	rBV3	299	225	0.01%	0.002%
54	8.529	2326	2329	2332	rVB2	322	207	0.01%	0.002%
55	8.551	2332	2336	2337	rBV	287	219	0.01%	0.002%
56	8.612	2351	2355	2358	rBV2	478	483	0.03%	0.004%
57	8.844	2414	2427	2471	rBV	793189	1320587	80.68%	10.075%
58	8.998	2473	2475	2477	rBV3	494	270	0.02%	0.002%
59	9.059	2488	2494	2500	rVB4	691	780	0.05%	0.006%
60	9.133	2509	2517	2526	rVB4	1262	2321	0.14%	0.018%
61	9.182	2526	2532	2538	rBV4	480	632	0.04%	0.005%
62	9.217	2539	2543	2547	rVB3	399	353	0.02%	0.003%
63	9.416	2597	2605	2610	rBV4	531	753	0.05%	0.006%
64	9.455	2615	2617	2620	rBV2	348	219	0.01%	0.002%
65	9.529	2634	2640	2641	rBV2	360	317	0.02%	0.002%
66	9.709	2689	2696	2700	rBV3	600	814	0.05%	0.006%
67	9.767	2711	2714	2716	rBV2	399	236	0.01%	0.002%
68	9.927	2756	2764	2771	rVB3	552	924	0.06%	0.007%
69	10.053	2799	2803	2806	rBV3	207	220	0.01%	0.002%
70	10.207	2837	2851	2872	rBV	529256	836951	51.13%	6.385%
71	10.336	2888	2891	2893	rBV4	421	290	0.02%	0.002%
72	10.374	2894	2903	2918	rVB2	10368	17697	1.08%	0.135%
73	10.432	2918	2921	2923	rBV	376	232	0.01%	0.002%
74	10.509	2941	2945	2947	rBV2	511	388	0.02%	0.003%
75	10.718	3006	3010	3015	rVB3	339	303	0.02%	0.002%
76	10.741	3015	3017	3020	rBV2	282	237	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029429.D
 Acq On : 07 Dec 2022 19:55
 Operator : SY/MD
 Sample : N5894-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.841	3044	3048	3053	rBV3	547	618	0.04%	0.005%
78	10.985	3087	3093	3094	rBV2	330	323	0.02%	0.002%
79	11.008	3096	3100	3105	rVB2	214	243	0.01%	0.002%
80	11.088	3115	3125	3136	rVB2	9590	13899	0.85%	0.106%
81	11.239	3147	3172	3195	rBV	871687	1361353	83.17%	10.386%
82	11.384	3214	3217	3219	rBV3	333	222	0.01%	0.002%
83	11.435	3228	3233	3236	rVB2	750	742	0.05%	0.006%
84	11.551	3262	3269	3273	rBV4	821	1228	0.08%	0.009%
85	11.612	3275	3288	3314	rBV	823125	1292674	78.97%	9.862%
86	11.808	3345	3349	3352	rBV4	309	250	0.02%	0.002%
87	12.124	3444	3447	3453	rBV4	305	340	0.02%	0.003%
88	12.178	3461	3464	3469	rBV3	353	347	0.02%	0.003%
89	12.239	3476	3483	3493	rVB5	3187	5943	0.36%	0.045%
90	12.336	3511	3513	3518	rVB5	602	338	0.02%	0.003%
91	12.635	3600	3606	3612	rVB4	1352	1523	0.09%	0.012%
92	12.834	3665	3668	3675	rBV4	416	404	0.02%	0.003%
93	13.252	3791	3798	3804	rBV6	1987	2880	0.18%	0.022%
94	13.387	3836	3840	3841	rBV3	529	331	0.02%	0.003%
95	13.423	3848	3851	3856	rVB6	1062	876	0.05%	0.007%
96	13.477	3865	3868	3870	rBV2	1134	773	0.05%	0.006%
97	13.500	3870	3875	3881	rVV4	2448	3347	0.20%	0.026%
98	13.725	3941	3945	3946	rBV3	1134	750	0.05%	0.006%
99	14.017	4033	4036	4042	rBV7	827	940	0.06%	0.007%
100	14.111	4063	4065	4066	rBV	609	210	0.01%	0.002%




Sum of corrected areas: 13107244

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029429.D
Acq On : 07 Dec 2022 19:55
Operator : SY/MD
Sample : N5894-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

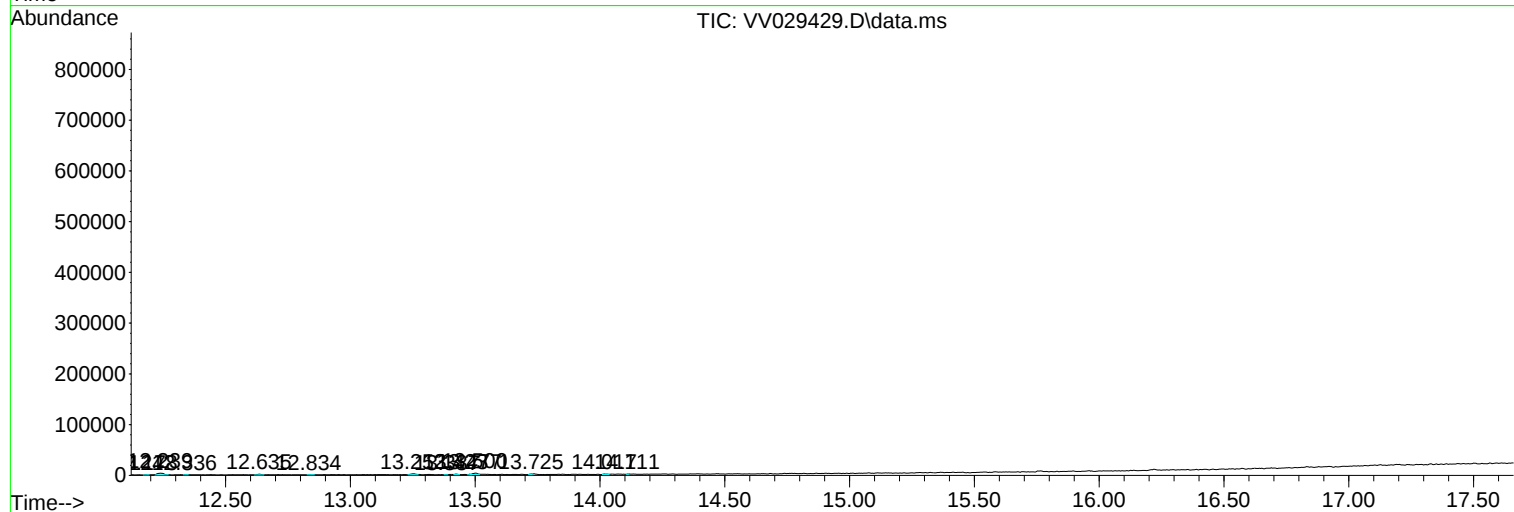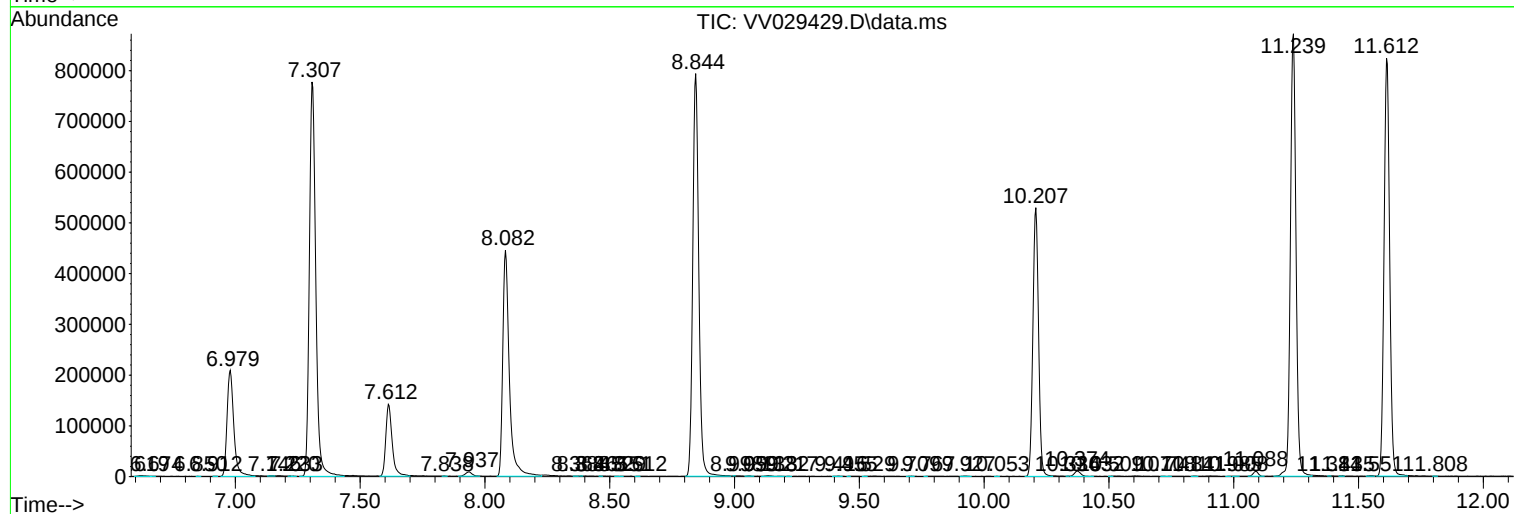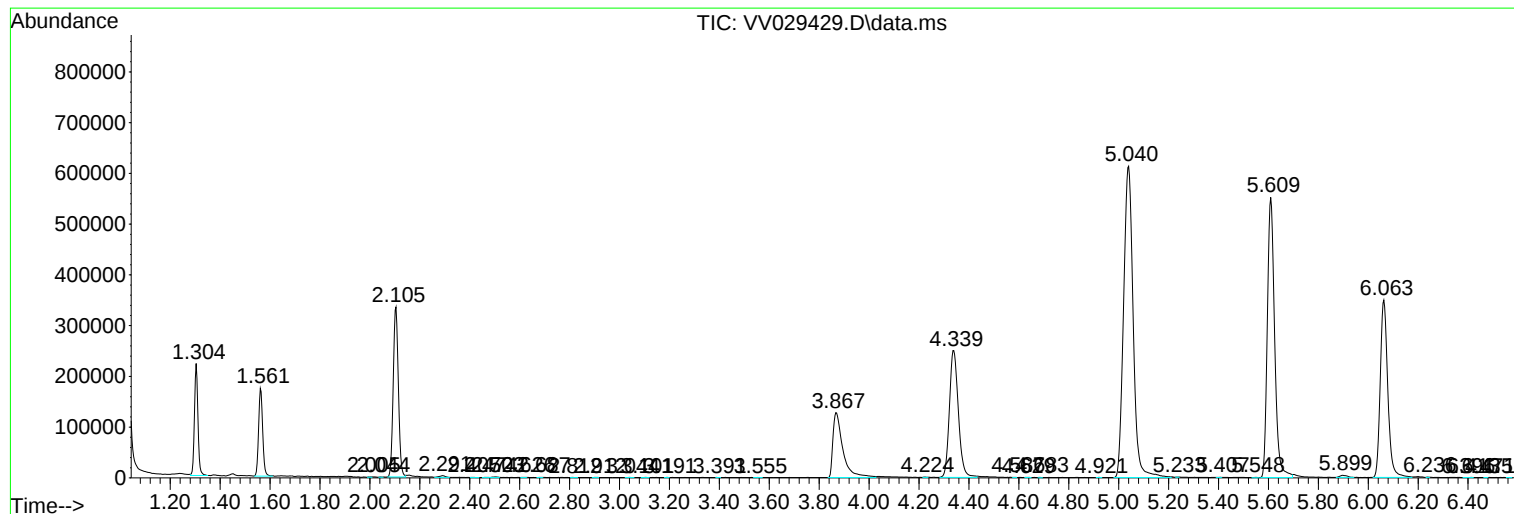

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029429.D
Acq On : 07 Dec 2022 19:55
Operator : SY/MD
Sample : N5894-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029429.D
Acq On : 07 Dec 2022 19:55
Operator : SY/MD
Sample : N5894-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------