

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029430.D
 Acq On : 07 Dec 2022 20:18
 Operator : SY/MD
 Sample : N5894-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029430.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	221526	213376	0.34%	0.135%
2	1.452	122	128	139	rVB6	4440	5995	0.01%	0.004%
3	1.561	154	162	178	rVB	174090	196457	0.32%	0.124%
4	2.105	319	331	345	rBV	333648	486138	0.78%	0.308%
5	2.265	378	381	383	rBV2	479	381	0.00%	0.000%
6	2.288	384	388	396	rVB2	2503	3119	0.01%	0.002%
7	2.355	405	409	412	rBV2	426	352	0.00%	0.000%
8	2.375	412	415	420	rBV3	369	330	0.00%	0.000%
9	2.503	448	455	464	rVV6	1632	2596	0.00%	0.002%
10	2.571	468	476	486	rVB5	2202	3389	0.01%	0.002%
11	2.638	494	497	502	rVV2	245	277	0.00%	0.000%
12	2.661	502	504	507	rVB3	399	217	0.00%	0.000%
13	2.687	507	512	515	rVB2	263	247	0.00%	0.000%
14	2.761	533	535	539	rVB2	373	256	0.00%	0.000%
15	2.931	583	588	593	rVB2	204	217	0.00%	0.000%
16	3.072	628	632	636	rBV2	187	218	0.00%	0.000%
17	3.111	641	644	650	rBV3	243	226	0.00%	0.000%
18	3.204	667	673	679	rBV2	247	332	0.00%	0.000%
19	3.304	702	704	711	rVV3	247	260	0.00%	0.000%
20	3.548	777	780	784	rVB	369	239	0.00%	0.000%
21	3.696	823	826	831	rBV	284	230	0.00%	0.000%
22	3.754	831	844	846	rBV5	3413	5504	0.01%	0.003%
23	3.867	869	879	920	rBV	131655	356235	0.57%	0.226%
24	4.278	1001	1007	1008	rBV3	309	282	0.00%	0.000%
25	4.339	1009	1026	1065	rVV	261286	643143	1.04%	0.407%
26	4.609	1107	1110	1115	rVV3	474	443	0.00%	0.000%
27	4.638	1115	1119	1120	rVV2	524	368	0.00%	0.000%
28	4.670	1120	1129	1141	rVV6	2842	6334	0.01%	0.004%
29	4.773	1157	1161	1166	rVB2	297	240	0.00%	0.000%
30	4.908	1198	1203	1209	rBV3	206	273	0.00%	0.000%
31	5.098	1226	1262	1333	rBV2	25878854	62016150	100.00%	39.270%
32	5.609	1409	1421	1461	rVB	555796	1100896	1.78%	0.697%
33	5.905	1503	1513	1523	rBV10	6142	12386	0.02%	0.008%
34	6.063	1547	1562	1598	rBV	344005	718235	1.16%	0.455%
35	6.268	1624	1626	1629	rBV4	382	215	0.00%	0.000%
36	6.381	1659	1661	1667	rVB3	373	277	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029430.D
 Acq On : 07 Dec 2022 20:18
 Operator : SY/MD
 Sample : N5894-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.619	1727	1735	1739	rBV3	1298	1880	0.00%	0.001%
38	6.780	1782	1785	1788	rBV3	387	339	0.00%	0.000%
39	6.860	1806	1810	1815	rVB5	435	503	0.00%	0.000%
40	6.899	1818	1822	1826	rBV4	271	278	0.00%	0.000%
41	6.921	1826	1829	1831	rBV	312	219	0.00%	0.000%
42	6.979	1835	1847	1880	rBV	209622	383012	0.62%	0.243%
43	7.124	1889	1892	1894	rBV3	680	448	0.00%	0.000%
44	7.307	1935	1949	1971	rBV	785384	1377675	2.22%	0.872%
45	7.612	2033	2044	2070	rBV	142480	252008	0.41%	0.160%
46	7.735	2080	2082	2085	rBV3	436	236	0.00%	0.000%
47	7.783	2094	2097	2100	rBV3	630	473	0.00%	0.000%
48	7.799	2100	2102	2105	rVB3	493	215	0.00%	0.000%
49	7.934	2135	2144	2149	rBV4	5033	8399	0.01%	0.005%
50	8.082	2179	2190	2231	rBV	454092	814333	1.31%	0.516%
51	8.571	2339	2342	2347	rBV3	474	444	0.00%	0.000%
52	8.638	2359	2363	2368	rBV4	265	294	0.00%	0.000%
53	8.792	2407	2411	2415	rBV4	375	361	0.00%	0.000%
54	8.879	2415	2438	2489	rBV2	34087764	60223702	97.11%	38.135%
55	9.664	2678	2682	2684	rBV4	461	349	0.00%	0.000%
56	9.924	2757	2763	2767	rVB4	672	666	0.00%	0.000%
57	10.050	2799	2802	2805	rVB2	500	320	0.00%	0.000%
58	10.082	2805	2812	2816	rBV3	449	549	0.00%	0.000%
59	10.104	2816	2819	2824	rVB2	349	328	0.00%	0.000%
60	10.136	2824	2829	2835	rBV3	544	540	0.00%	0.000%
61	10.207	2835	2851	2877	rBV	493103	784294	1.26%	0.497%
62	10.374	2893	2903	2912	rBV2	5955	10142	0.02%	0.006%
63	10.416	2912	2916	2930	rVV5	1735	2629	0.00%	0.002%
64	10.535	2944	2953	2960	rBV3	1638	2134	0.00%	0.001%
65	10.661	2981	2992	2995	rBV4	389	628	0.00%	0.000%
66	10.802	3032	3036	3041	rVB3	250	286	0.00%	0.000%
67	10.863	3052	3055	3057	rBV2	313	227	0.00%	0.000%
68	10.905	3062	3068	3069	rBV3	621	628	0.00%	0.000%
69	10.995	3093	3096	3099	rVB2	345	226	0.00%	0.000%
70	11.043	3109	3111	3115	rVB2	489	346	0.00%	0.000%
71	11.088	3115	3125	3134	rBV2	7617	11400	0.02%	0.007%
72	11.172	3138	3151	3161	rBV	269930	436324	0.70%	0.276%
73	11.262	3162	3179	3218	rVB	8708532	14357095	23.15%	9.091%
74	11.551	3266	3269	3276	rVB4	1384	1275	0.00%	0.001%
75	11.632	3276	3294	3329	rBV2	8126288	13394332	21.60%	8.482%
76	11.886	3371	3373	3378	rBV4	348	355	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029430.D
 Acq On : 07 Dec 2022 20:18
 Operator : SY/MD
 Sample : N5894-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	12.033	3415	3419	3421	rVB3	358	278	0.00%	0.000%
78	12.050	3421	3424	3425	rBV2	374	223	0.00%	0.000%
79	12.130	3445	3449	3453	rBV4	290	299	0.00%	0.000%
80	12.230	3474	3480	3481	rBV3	1468	1169	0.00%	0.001%
81	12.278	3492	3495	3498	rVB3	420	216	0.00%	0.000%
82	12.445	3542	3547	3548	rBV3	313	253	0.00%	0.000%
83	12.580	3588	3589	3592	rVV3	482	238	0.00%	0.000%
84	12.603	3592	3596	3599	rVV2	461	435	0.00%	0.000%
85	12.619	3599	3601	3602	rVV	727	353	0.00%	0.000%
86	12.635	3602	3606	3613	rVB4	1357	1678	0.00%	0.001%
87	12.686	3618	3622	3627	rBV4	584	730	0.00%	0.000%
88	12.731	3634	3636	3642	rBV4	455	414	0.00%	0.000%
89	12.882	3681	3683	3688	rVB3	391	262	0.00%	0.000%
90	12.911	3690	3692	3696	rVB3	528	350	0.00%	0.000%
91	12.956	3696	3706	3708	rBV4	662	1028	0.00%	0.001%
92	12.982	3709	3714	3720	rVV4	478	648	0.00%	0.000%
93	13.082	3742	3745	3746	rBV2	454	229	0.00%	0.000%
94	13.156	3765	3768	3770	rBV2	437	282	0.00%	0.000%
95	13.249	3787	3797	3809	rBV	40473	61172	0.10%	0.039%
96	13.500	3870	3875	3880	rVB3	1587	1710	0.00%	0.001%
97	13.648	3919	3921	3929	rBV4	518	567	0.00%	0.000%
98	13.731	3942	3947	3955	rVV6	2444	3496	0.01%	0.002%
99	13.773	3958	3960	3963	rVB3	769	422	0.00%	0.000%
100	14.014	4032	4035	4040	rBV4	731	592	0.00%	0.000%




Sum of corrected areas: 157922769

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029430.D
Acq On : 07 Dec 2022 20:18
Operator : SY/MD
Sample : N5894-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

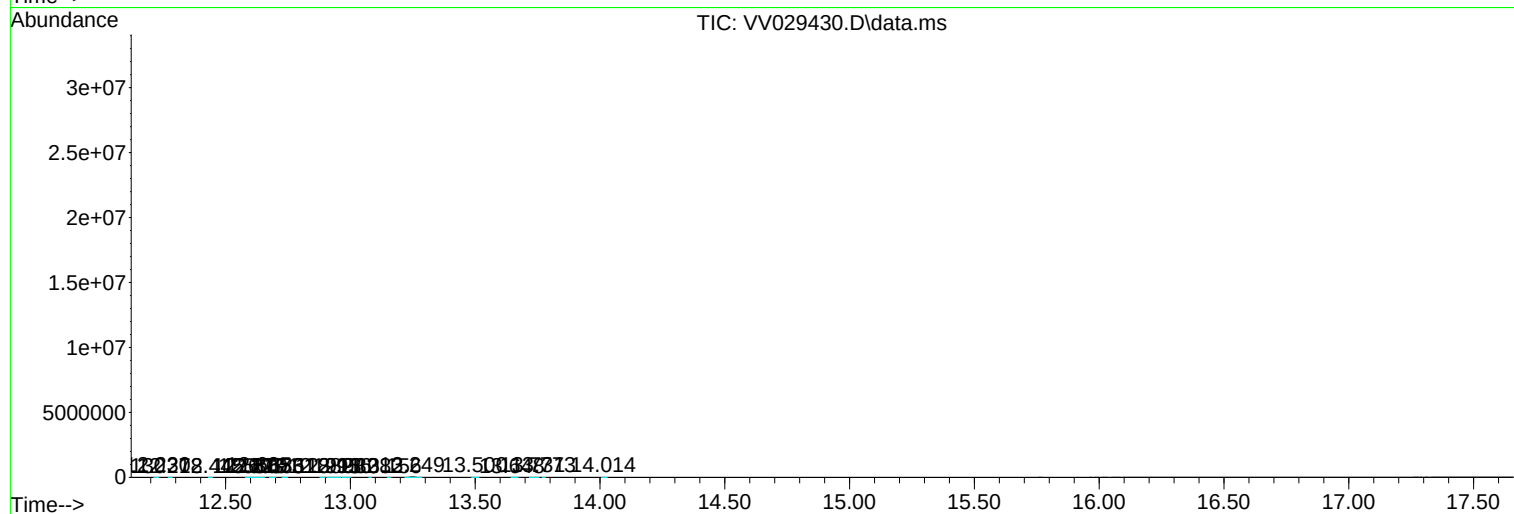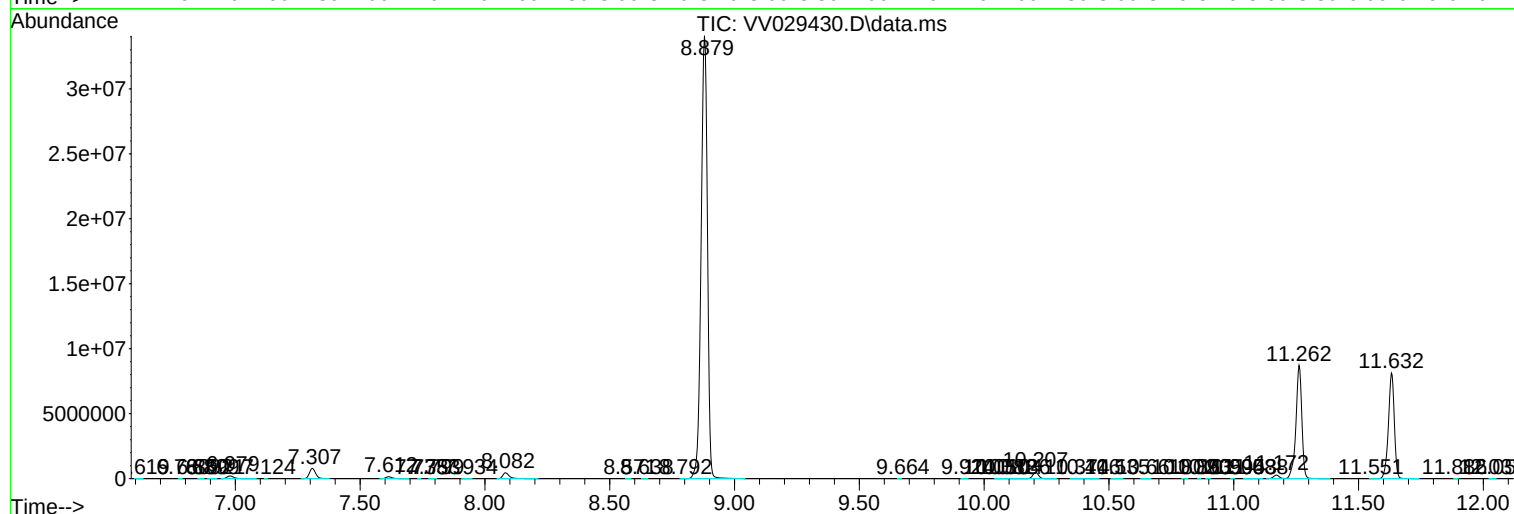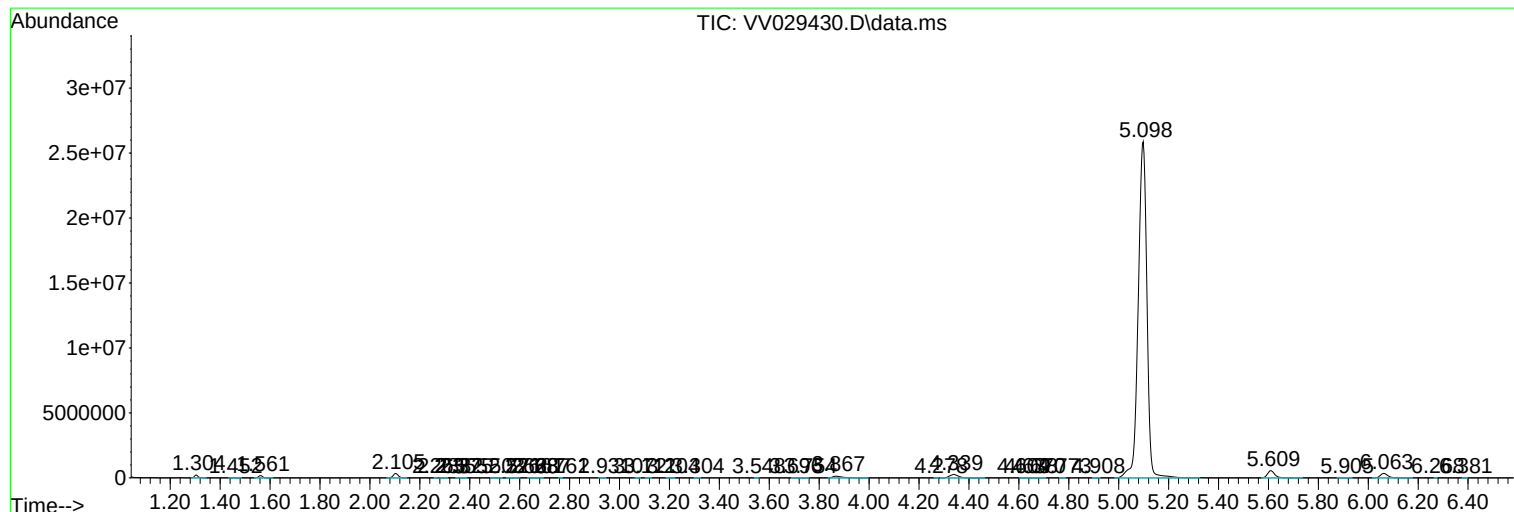

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029430.D
Acq On : 07 Dec 2022 20:18
Operator : SY/MD
Sample : N5894-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029430.D
Acq On : 07 Dec 2022 20:18
Operator : SY/MD
Sample : N5894-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc