

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029435.D
 Acq On : 07 Dec 2022 22:39
 Operator : SY/MD
 Sample : VV1207WBL04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK296

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	97	rVB	220202	217773	13.12%	1.654%
2	1.561	154	162	175	rBV	177069	195216	11.76%	1.482%
3	2.101	319	330	346	rBV	338703	486534	29.31%	3.694%
4	2.413	422	427	429	rBV	310	263	0.02%	0.002%
5	2.442	434	436	440	rVB2	445	215	0.01%	0.002%
6	2.500	446	454	463	rBV3	4849	7486	0.45%	0.057%
7	2.568	471	475	480	rBV2	358	338	0.02%	0.003%
8	2.619	485	491	494	rBV2	437	360	0.02%	0.003%
9	2.757	527	534	536	rBV4	503	600	0.04%	0.005%
10	2.844	559	561	565	rVB2	303	188	0.01%	0.001%
11	2.944	590	592	597	rVB2	325	223	0.01%	0.002%
12	3.140	650	653	657	rBV3	247	198	0.01%	0.002%
13	3.484	757	760	763	rVB2	315	224	0.01%	0.002%
14	3.519	768	771	775	rVB2	294	198	0.01%	0.002%
15	3.600	794	796	804	rVB2	248	188	0.01%	0.001%
16	3.867	867	879	929	rBV	124187	343374	20.68%	2.607%
17	4.336	1008	1025	1061	rBV	249486	625752	37.69%	4.751%
18	4.561	1091	1095	1098	rBV3	526	459	0.03%	0.003%
19	4.577	1098	1100	1103	rVV2	337	205	0.01%	0.002%
20	4.606	1107	1109	1114	rBV4	455	387	0.02%	0.003%
21	4.641	1117	1120	1124	rVV3	368	293	0.02%	0.002%
22	4.667	1124	1128	1132	rVB5	714	708	0.04%	0.005%
23	4.953	1213	1217	1220	rBV2	351	240	0.01%	0.002%
24	5.037	1224	1243	1295	rBV2	628791	1660091	100.00%	12.605%
25	5.310	1326	1328	1333	rVB2	388	252	0.02%	0.002%
26	5.339	1333	1337	1339	rBV3	417	345	0.02%	0.003%
27	5.391	1350	1353	1356	rBV3	544	506	0.03%	0.004%
28	5.461	1371	1375	1378	rBV3	272	211	0.01%	0.002%
29	5.490	1378	1384	1387	rVB4	396	396	0.02%	0.003%
30	5.609	1408	1421	1446	rBV	559185	1127623	67.93%	8.562%
31	5.815	1483	1485	1490	rVB3	516	404	0.02%	0.003%
32	5.899	1500	1511	1526	rVB6	5465	12174	0.73%	0.092%
33	6.063	1546	1562	1598	rBV	351221	733978	44.21%	5.573%
34	6.249	1618	1620	1623	rVB2	461	253	0.02%	0.002%
35	6.304	1632	1637	1639	rBV3	375	300	0.02%	0.002%
36	6.387	1658	1663	1664	rBV2	249	189	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029435.D
 Acq On : 07 Dec 2022 22:39
 Operator : SY/MD
 Sample : VV1207WBL04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK296

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.519	1698	1704	1707	rVB3	337	256	0.02%	0.002%
38	6.554	1707	1715	1719	rVB3	341	393	0.02%	0.003%
39	6.580	1719	1723	1728	rBV3	463	411	0.02%	0.003%
40	6.625	1728	1737	1739	rBV4	1351	1822	0.11%	0.014%
41	6.722	1764	1767	1770	rBV3	360	316	0.02%	0.002%
42	6.895	1816	1821	1823	rBV2	238	235	0.01%	0.002%
43	6.979	1834	1847	1877	rBV	207357	379131	22.84%	2.879%
44	7.307	1936	1949	1994	rVV	775455	1396543	84.12%	10.604%
45	7.612	2033	2044	2073	rBV	141496	249958	15.06%	1.898%
46	7.857	2114	2120	2125	rBV6	391	482	0.03%	0.004%
47	7.969	2150	2155	2156	rBV3	486	367	0.02%	0.003%
48	8.082	2180	2190	2225	rBV	443483	795110	47.90%	6.037%
49	8.358	2272	2276	2281	rBV4	495	662	0.04%	0.005%
50	8.493	2315	2318	2323	rBV2	382	421	0.03%	0.003%
51	8.616	2352	2356	2360	rVB3	403	297	0.02%	0.002%
52	8.667	2369	2372	2375	rBV3	362	334	0.02%	0.003%
53	8.741	2392	2395	2398	rVB2	253	182	0.01%	0.001%
54	8.773	2403	2405	2413	rVB4	373	470	0.03%	0.004%
55	8.844	2413	2427	2468	rBV	808224	1342152	80.85%	10.191%
56	9.053	2490	2492	2497	rBV5	390	366	0.02%	0.003%
57	9.124	2510	2514	2515	rBV3	837	469	0.03%	0.004%
58	9.262	2556	2557	2565	rVB2	214	223	0.01%	0.002%
59	9.387	2593	2596	2599	rVB3	336	236	0.01%	0.002%
60	9.416	2600	2605	2607	rBV	418	280	0.02%	0.002%
61	9.474	2620	2623	2626	rBV	287	184	0.01%	0.001%
62	9.535	2638	2642	2644	rBV2	678	519	0.03%	0.004%
63	9.561	2644	2650	2658	rVV3	1531	2170	0.13%	0.016%
64	9.599	2659	2662	2664	rVV2	301	186	0.01%	0.001%
65	9.622	2666	2669	2675	rVB2	509	490	0.03%	0.004%
66	9.657	2675	2680	2683	rBV3	394	402	0.02%	0.003%
67	9.702	2690	2694	2697	rBV4	378	273	0.02%	0.002%
68	9.924	2757	2763	2769	rVB3	865	1184	0.07%	0.009%
69	9.976	2775	2779	2784	rBV3	186	184	0.01%	0.001%
70	10.075	2801	2810	2818	rBV5	1782	3503	0.21%	0.027%
71	10.207	2838	2851	2879	rBV	530500	834783	50.29%	6.339%
72	10.326	2885	2888	2892	rBV4	411	224	0.01%	0.002%
73	10.345	2892	2894	2896	rVV2	379	251	0.02%	0.002%
74	10.374	2900	2903	2913	rVB2	1105	1238	0.07%	0.009%
75	10.468	2929	2932	2936	rVV3	323	247	0.01%	0.002%
76	10.532	2945	2952	2956	rVB4	784	927	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029435.D
 Acq On : 07 Dec 2022 22:39
 Operator : SY/MD
 Sample : VV1207WBL04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK296

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.837	3043	3047	3048	rBV3	393	264	0.02%	0.002%
78	10.873	3054	3058	3061	rBV3	386	366	0.02%	0.003%
79	10.908	3064	3069	3077	rVB2	940	1372	0.08%	0.010%
80	11.172	3143	3151	3160	rBV5	2250	4062	0.24%	0.031%
81	11.239	3160	3172	3201	rBV	879619	1370226	82.54%	10.404%
82	11.561	3269	3272	3274	rVB2	590	330	0.02%	0.003%
83	11.612	3275	3288	3316	rBV	823209	1305941	78.67%	9.916%
84	11.799	3344	3346	3350	rVB3	394	258	0.02%	0.002%
85	12.017	3412	3414	3417	rBV2	341	218	0.01%	0.002%
86	12.078	3430	3433	3436	rBV3	303	204	0.01%	0.002%
87	12.201	3465	3471	3475	rBV2	402	489	0.03%	0.004%
88	12.416	3536	3538	3542	rVB4	615	441	0.03%	0.003%
89	12.506	3564	3566	3568	rBV	335	183	0.01%	0.001%
90	12.638	3599	3607	3614	rBV4	2804	4224	0.25%	0.032%
91	12.847	3669	3672	3673	rBV2	519	298	0.02%	0.002%
92	12.921	3692	3695	3696	rBV	443	220	0.01%	0.002%
93	12.998	3717	3719	3723	rVB4	595	360	0.02%	0.003%
94	13.178	3772	3775	3777	rBV3	413	260	0.02%	0.002%
95	13.207	3781	3784	3786	rVV3	514	372	0.02%	0.003%
96	13.252	3789	3798	3809	rVB4	5683	9115	0.55%	0.069%
97	13.496	3865	3874	3888	rVB	16738	26710	1.61%	0.203%
98	13.731	3941	3947	3955	rVB4	4625	6826	0.41%	0.052%
99	13.995	4025	4029	4031	rBV3	774	598	0.04%	0.005%
100	14.358	4140	4142	4143	rBV2	701	291	0.02%	0.002%




Sum of corrected areas: 13169653

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029435.D
Acq On : 07 Dec 2022 22:39
Operator : SY/MD
Sample : VV1207WBL04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK296

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

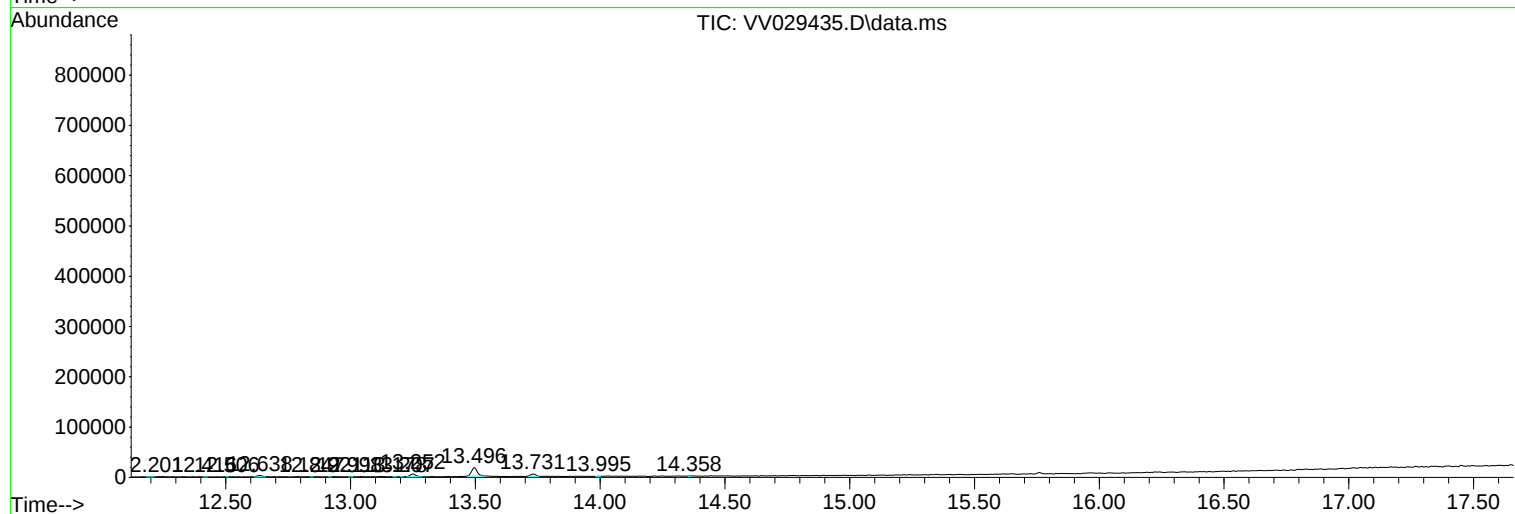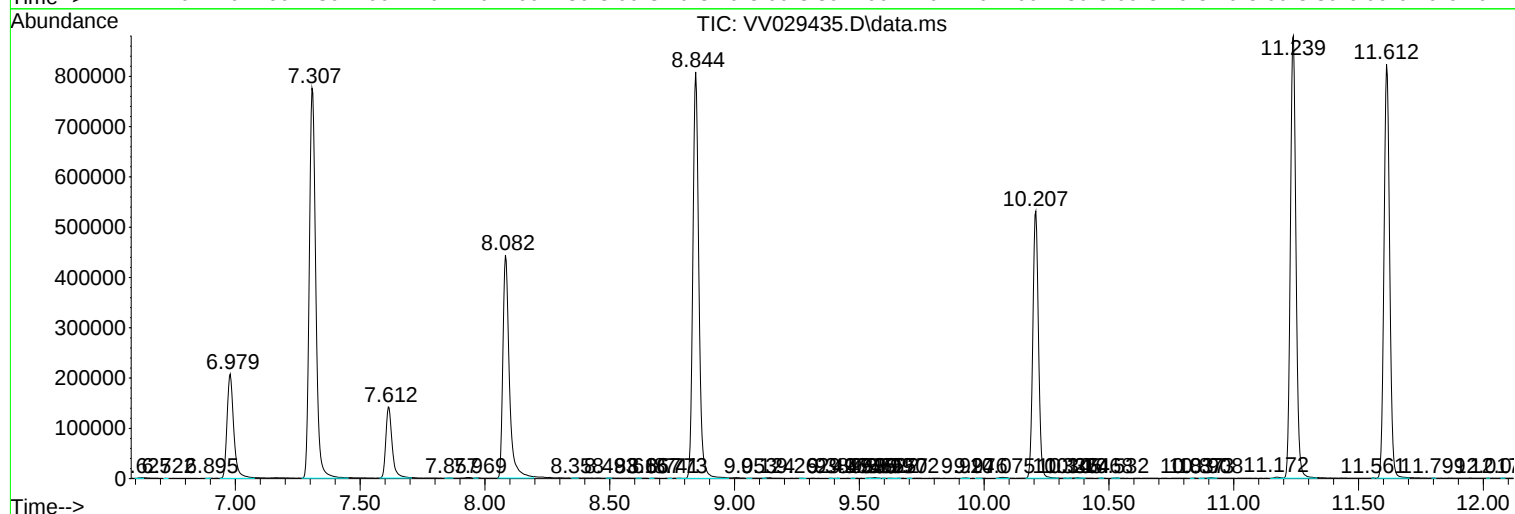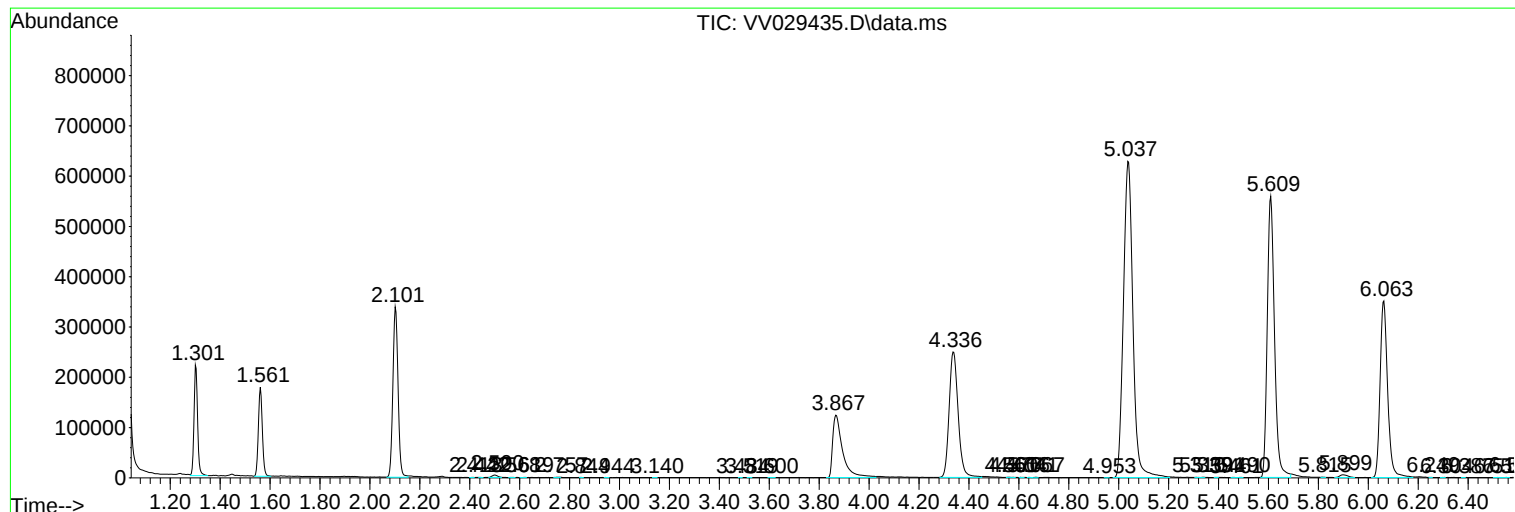

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029435.D
Acq On : 07 Dec 2022 22:39
Operator : SY/MD
Sample : VV1207WBL04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK296

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029435.D
Acq On : 07 Dec 2022 22:39
Operator : SY/MD
Sample : VV1207WBL04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK296

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc