

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029436.D
 Acq On : 07 Dec 2022 23:03
 Operator : SY/MD
 Sample : N5894-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VV029436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	226273	220350	13.89%	1.744%
2	1.446	122	126	132	rBV5	3330	3613	0.23%	0.029%
3	1.561	155	162	178	rVB	167164	188303	11.87%	1.490%
4	1.979	289	292	295	rBV5	443	356	0.02%	0.003%
5	2.105	319	331	344	rBV	324814	466874	29.42%	3.695%
6	2.288	384	388	398	rVB2	2245	3313	0.21%	0.026%
7	2.436	430	434	437	rBV	288	267	0.02%	0.002%
8	2.503	447	455	463	rBV	3716	5587	0.35%	0.044%
9	2.754	530	533	537	rVB3	574	441	0.03%	0.003%
10	3.150	654	656	662	rVB2	334	219	0.01%	0.002%
11	3.288	695	699	701	rBV	372	266	0.02%	0.002%
12	3.564	782	785	792	rVB2	291	289	0.02%	0.002%
13	3.796	853	857	863	rVB3	305	297	0.02%	0.002%
14	3.867	870	879	917	rBV	116422	318782	20.09%	2.523%
15	4.089	945	948	949	rBV2	621	301	0.02%	0.002%
16	4.191	978	980	987	rBV3	424	352	0.02%	0.003%
17	4.278	1002	1007	1010	rBV3	429	491	0.03%	0.004%
18	4.339	1010	1026	1055	rVV	241589	601145	37.88%	4.758%
19	4.558	1092	1094	1099	rVB2	471	279	0.02%	0.002%
20	4.590	1099	1104	1106	rBV3	352	295	0.02%	0.002%
21	4.670	1127	1129	1132	rBV2	336	219	0.01%	0.002%
22	4.683	1132	1133	1137	rVB2	472	250	0.02%	0.002%
23	4.754	1148	1155	1158	rBV2	405	355	0.02%	0.003%
24	4.799	1165	1169	1170	rBV	306	202	0.01%	0.002%
25	4.831	1175	1179	1182	rBV3	232	208	0.01%	0.002%
26	4.973	1219	1223	1225	rBV2	403	282	0.02%	0.002%
27	5.040	1225	1244	1297	rBV2	595052	1586821	100.00%	12.560%
28	5.301	1322	1325	1329	rBV2	345	223	0.01%	0.002%
29	5.445	1363	1370	1375	rBV3	423	614	0.04%	0.005%
30	5.474	1375	1379	1380	rBV2	444	322	0.02%	0.003%
31	5.519	1388	1393	1396	rBV2	304	304	0.02%	0.002%
32	5.609	1406	1421	1462	rBV	537947	1090506	68.72%	8.632%
33	5.899	1501	1511	1526	rVB8	3893	9158	0.58%	0.072%
34	5.989	1536	1539	1543	rVB3	240	219	0.01%	0.002%
35	6.063	1546	1562	1593	rBV	339556	702444	44.27%	5.560%
36	6.188	1598	1601	1604	rBV4	638	499	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029436.D
 Acq On : 07 Dec 2022 23:03
 Operator : SY/MD
 Sample : N5894-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.252	1618	1621	1623	rBV4	416	280	0.02%	0.002%
38	6.285	1626	1631	1634	rVB3	310	252	0.02%	0.002%
39	6.326	1641	1644	1649	rVB3	632	407	0.03%	0.003%
40	6.497	1694	1697	1704	rVV2	258	211	0.01%	0.002%
41	6.587	1719	1725	1729	rBV4	362	375	0.02%	0.003%
42	6.629	1729	1738	1740	rBV4	1131	1660	0.10%	0.013%
43	6.838	1797	1803	1807	rBV4	383	384	0.02%	0.003%
44	6.883	1814	1817	1820	rVB	420	224	0.01%	0.002%
45	6.937	1830	1834	1835	rBV2	335	202	0.01%	0.002%
46	6.979	1835	1847	1879	rBV	197062	362410	22.84%	2.869%
47	7.149	1897	1900	1901	rBV2	493	312	0.02%	0.002%
48	7.307	1936	1949	1985	rBV	751801	1335593	84.17%	10.572%
49	7.613	2034	2044	2069	rBV	137678	241123	15.20%	1.909%
50	7.809	2102	2105	2108	rBV2	312	210	0.01%	0.002%
51	7.937	2135	2145	2154	rBV4	3942	7378	0.46%	0.058%
52	7.973	2154	2156	2159	rVB2	677	311	0.02%	0.002%
53	8.082	2178	2190	2225	rBV	417514	761771	48.01%	6.030%
54	8.468	2307	2310	2315	rVB3	404	352	0.02%	0.003%
55	8.545	2330	2334	2341	rVB4	421	324	0.02%	0.003%
56	8.606	2346	2353	2358	rBV3	472	665	0.04%	0.005%
57	8.709	2381	2385	2386	rBV2	453	257	0.02%	0.002%
58	8.754	2396	2399	2401	rBV	360	258	0.02%	0.002%
59	8.844	2414	2427	2454	rBV	779361	1278147	80.55%	10.117%
60	9.088	2499	2503	2506	rBV4	289	251	0.02%	0.002%
61	9.108	2506	2509	2512	rVV3	346	237	0.01%	0.002%
62	9.140	2512	2519	2528	rVB6	1174	1957	0.12%	0.015%
63	9.175	2528	2530	2535	rVB2	352	282	0.02%	0.002%
64	9.281	2559	2563	2567	rBV2	220	256	0.02%	0.002%
65	9.542	2639	2644	2645	rBV3	653	504	0.03%	0.004%
66	9.600	2658	2662	2669	rVB3	325	368	0.02%	0.003%
67	9.661	2679	2681	2684	rBV2	343	217	0.01%	0.002%
68	9.728	2698	2702	2705	rBV2	379	327	0.02%	0.003%
69	9.915	2756	2760	2763	rBV3	800	722	0.05%	0.006%
70	10.030	2791	2796	2800	rBV2	309	345	0.02%	0.003%
71	10.075	2806	2810	2811	rBV2	775	619	0.04%	0.005%
72	10.207	2838	2851	2871	rBV	515609	805585	50.77%	6.376%
73	10.374	2892	2903	2912	rVB	5189	8730	0.55%	0.069%
74	10.535	2949	2953	2957	rVB3	795	798	0.05%	0.006%
75	10.587	2965	2969	2972	rBV2	317	241	0.02%	0.002%
76	10.690	2998	3001	3007	rVB3	248	258	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029436.D
 Acq On : 07 Dec 2022 23:03
 Operator : SY/MD
 Sample : N5894-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.844	3046	3049	3053	rVB2	658	517	0.03%	0.004%
78	10.911	3061	3070	3075	rBV4	1065	1678	0.11%	0.013%
79	11.001	3095	3098	3102	rBV2	294	227	0.01%	0.002%
80	11.079	3119	3122	3124	rBV2	609	405	0.03%	0.003%
81	11.143	3138	3142	3145	rBV3	495	494	0.03%	0.004%
82	11.172	3145	3151	3156	rBV2	1712	1914	0.12%	0.015%
83	11.239	3159	3172	3192	rBV	847819	1311417	82.64%	10.380%
84	11.455	3237	3239	3243	rVB2	545	234	0.01%	0.002%
85	11.548	3256	3268	3276	rBV3	6358	11525	0.73%	0.091%
86	11.612	3276	3288	3311	rVV	804759	1257677	79.26%	9.955%
87	11.799	3343	3346	3349	rBV3	715	520	0.03%	0.004%
88	11.921	3380	3384	3391	rVV5	387	390	0.02%	0.003%
89	11.963	3395	3397	3401	rVB3	410	245	0.02%	0.002%
90	12.236	3477	3482	3490	rBV6	1500	2201	0.14%	0.017%
91	12.336	3511	3513	3517	rVB3	740	447	0.03%	0.004%
92	12.384	3524	3528	3530	rBV2	286	225	0.01%	0.002%
93	12.632	3600	3605	3616	rBV5	1722	2830	0.18%	0.022%
94	12.898	3686	3688	3691	rBV2	299	229	0.01%	0.002%
95	12.998	3714	3719	3721	rBV2	653	475	0.03%	0.004%
96	13.252	3791	3798	3803	rBV6	2969	4355	0.27%	0.034%
97	13.300	3811	3813	3815	rVB3	590	273	0.02%	0.002%
98	13.320	3815	3819	3823	rBV3	747	777	0.05%	0.006%
99	13.497	3863	3874	3882	rBV2	6468	11489	0.72%	0.091%
100	13.734	3943	3948	3956	rVB5	3065	3981	0.25%	0.032%




Sum of corrected areas: 12633774

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029436.D
Acq On : 07 Dec 2022 23:03
Operator : SY/MD
Sample : N5894-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

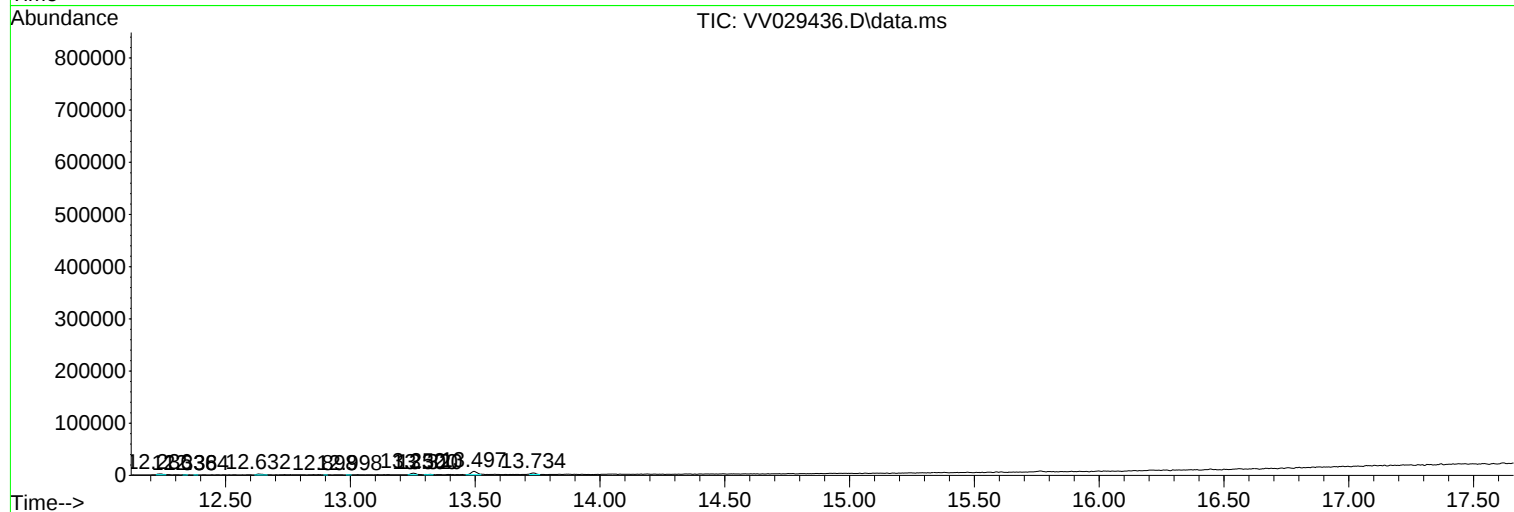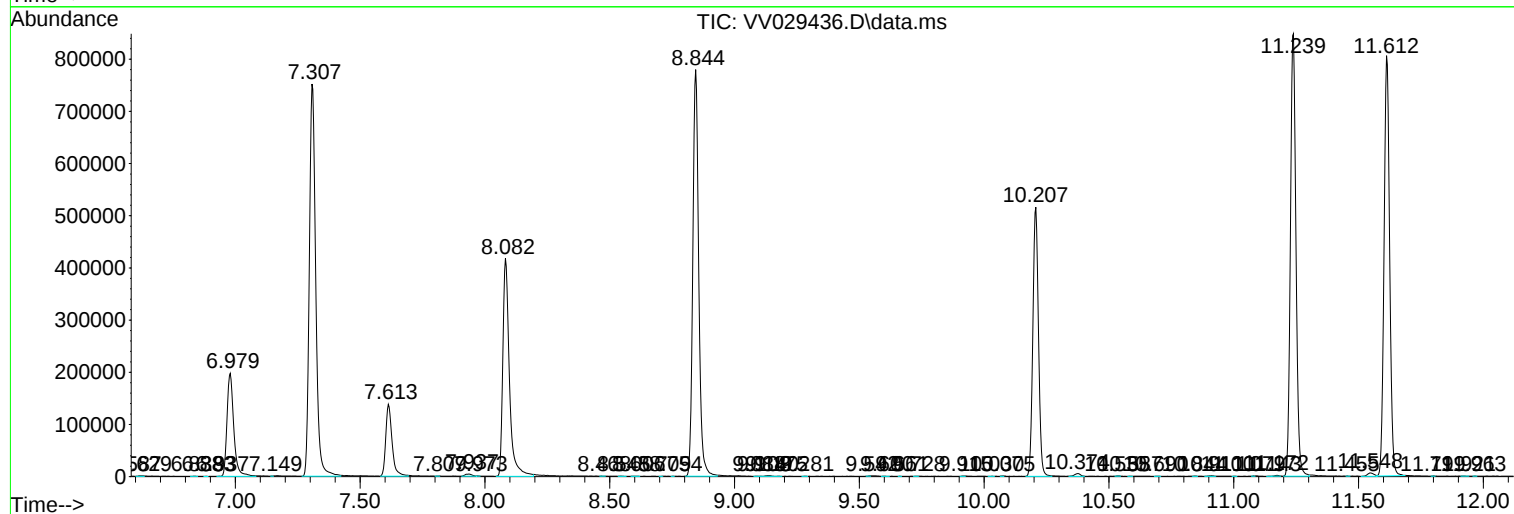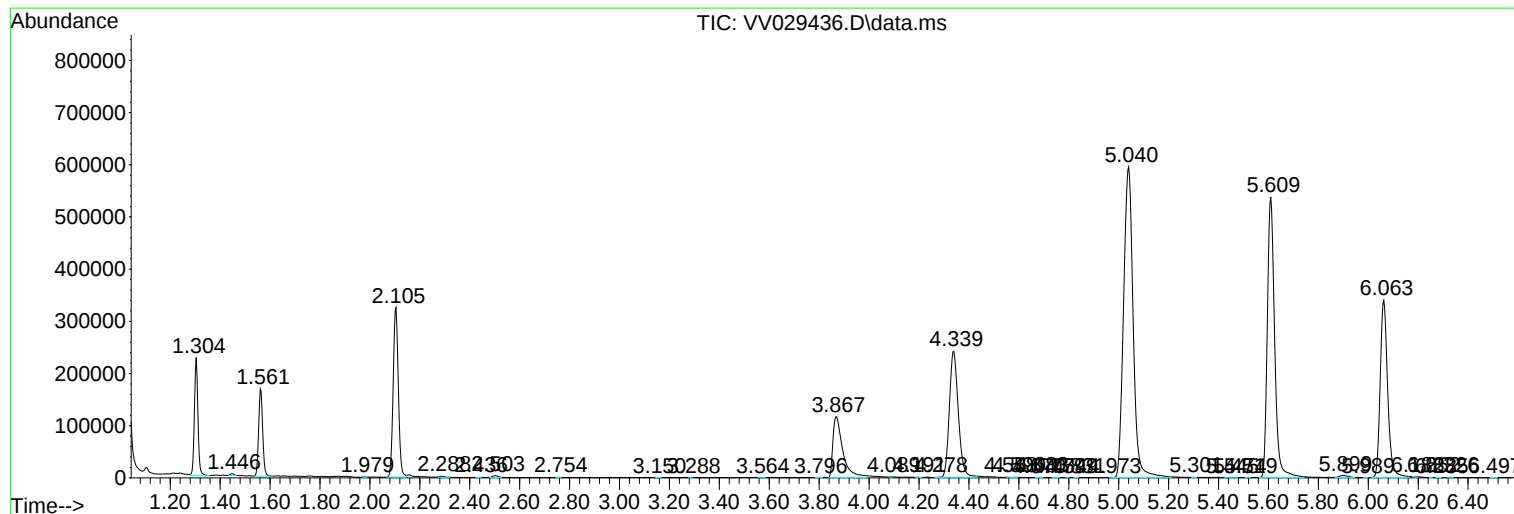

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029436.D
Acq On : 07 Dec 2022 23:03
Operator : SY/MD
Sample : N5894-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029436.D
Acq On : 07 Dec 2022 23:03
Operator : SY/MD
Sample : N5894-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc