

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029437.D
 Acq On : 07 Dec 2022 23:26
 Operator : SY/MD
 Sample : N5894-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029437.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	226519	224216	0.36%	0.140%
2	1.561	154	162	175	rBV	178054	201665	0.32%	0.126%
3	2.027	304	307	308	rBV4	443	278	0.00%	0.000%
4	2.105	320	331	344	rBV	351263	504777	0.81%	0.315%
5	2.342	402	405	409	rBV2	273	217	0.00%	0.000%
6	2.362	409	411	416	rVB3	395	357	0.00%	0.000%
7	2.394	416	421	423	rBV2	332	268	0.00%	0.000%
8	2.423	428	430	435	rVB	434	267	0.00%	0.000%
9	2.494	447	452	453	rBV	1218	762	0.00%	0.000%
10	2.574	466	477	489	rVB5	2273	4014	0.01%	0.003%
11	2.625	489	493	497	rBV4	300	307	0.00%	0.000%
12	2.658	500	503	504	rBV2	387	226	0.00%	0.000%
13	2.764	530	536	541	rVV4	316	439	0.00%	0.000%
14	2.889	570	575	578	rBV2	335	342	0.00%	0.000%
15	2.963	594	598	601	rVB4	279	215	0.00%	0.000%
16	2.989	601	606	609	rBV3	289	269	0.00%	0.000%
17	3.137	649	652	658	rBV2	235	277	0.00%	0.000%
18	3.381	721	728	733	rBV3	285	355	0.00%	0.000%
19	3.471	751	756	758	rVV3	408	230	0.00%	0.000%
20	3.568	781	786	790	rBV2	314	239	0.00%	0.000%
21	3.751	832	843	862	rVB5	3959	9880	0.02%	0.006%
22	3.867	869	879	918	rBV	128048	349905	0.56%	0.219%
23	4.143	962	965	968	rVB3	577	388	0.00%	0.000%
24	4.339	1009	1026	1052	rBV	260947	659174	1.05%	0.412%
25	4.593	1101	1105	1109	rVB3	660	660	0.00%	0.000%
26	4.667	1119	1128	1130	rBV5	2779	3145	0.01%	0.002%
27	5.098	1226	1262	1338	rBV2	26083084	62553357	100.00%	39.097%
28	5.609	1408	1421	1452	rBV	550665	1109509	1.77%	0.693%
29	5.905	1503	1513	1529	rVB9	7391	16571	0.03%	0.010%
30	5.992	1537	1540	1545	rVB4	417	280	0.00%	0.000%
31	6.063	1545	1562	1592	rBV	356613	736471	1.18%	0.460%
32	6.288	1630	1632	1636	rVB2	725	328	0.00%	0.000%
33	6.577	1718	1722	1725	rBV3	355	356	0.00%	0.000%
34	6.625	1728	1737	1740	rBV5	1164	1686	0.00%	0.001%
35	6.677	1751	1753	1756	rBV3	390	246	0.00%	0.000%
36	6.860	1807	1810	1813	rVV2	353	249	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029437.D
 Acq On : 07 Dec 2022 23:26
 Operator : SY/MD
 Sample : N5894-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.902	1820	1823	1827	rBV5	476	377	0.00%	0.000%
38	6.979	1834	1847	1877	rBV	208221	385378	0.62%	0.241%
39	7.191	1910	1913	1918	rVB2	499	371	0.00%	0.000%
40	7.307	1936	1949	1969	rBV	803668	1405641	2.25%	0.879%
41	7.554	2023	2026	2027	rBV3	381	242	0.00%	0.000%
42	7.612	2034	2044	2071	rBV	145002	252069	0.40%	0.158%
43	7.789	2094	2099	2105	rBV4	518	613	0.00%	0.000%
44	7.934	2136	2144	2149	rBV4	2747	4441	0.01%	0.003%
45	8.082	2179	2190	2226	rBV	447263	810098	1.30%	0.506%
46	8.362	2274	2277	2280	rBV3	375	261	0.00%	0.000%
47	8.435	2295	2300	2302	rBV3	524	484	0.00%	0.000%
48	8.519	2321	2326	2329	rBV2	394	331	0.00%	0.000%
49	8.667	2370	2372	2378	rBV3	283	213	0.00%	0.000%
50	8.712	2383	2386	2390	rBV2	363	336	0.00%	0.000%
51	8.792	2410	2411	2414	rBV2	362	214	0.00%	0.000%
52	8.879	2415	2438	2489	rBV2	34397332	60992060	97.50%	38.122%
53	9.545	2638	2645	2646	rBV4	698	794	0.00%	0.000%
54	9.632	2669	2672	2675	rBV2	261	216	0.00%	0.000%
55	9.696	2689	2692	2697	rVB3	602	504	0.00%	0.000%
56	9.950	2770	2771	2777	rVB2	335	261	0.00%	0.000%
57	10.075	2805	2810	2811	rBV3	656	472	0.00%	0.000%
58	10.130	2824	2827	2833	rVB3	507	487	0.00%	0.000%
59	10.159	2833	2836	2837	rBV2	426	263	0.00%	0.000%
60	10.207	2839	2851	2866	rBV	499020	789622	1.26%	0.494%
61	10.374	2893	2903	2910	rBV3	3564	5787	0.01%	0.004%
62	10.416	2910	2916	2921	rVB2	1602	1820	0.00%	0.001%
63	10.532	2945	2952	2962	rVB4	2020	2785	0.00%	0.002%
64	10.596	2969	2972	2975	rBV3	379	322	0.00%	0.000%
65	10.734	3012	3015	3017	rBV2	272	226	0.00%	0.000%
66	10.773	3023	3027	3030	rBV2	370	418	0.00%	0.000%
67	10.789	3030	3032	3037	rVB4	520	349	0.00%	0.000%
68	10.837	3044	3047	3051	rBV2	258	221	0.00%	0.000%
69	10.902	3057	3067	3068	rBV3	914	961	0.00%	0.001%
70	11.017	3100	3103	3108	rBV3	181	216	0.00%	0.000%
71	11.088	3115	3125	3136	rVB2	7248	10530	0.02%	0.007%
72	11.168	3138	3150	3162	rBV	274382	448422	0.72%	0.280%
73	11.262	3162	3179	3213	rVB	8921794	14669631	23.45%	9.169%
74	11.509	3252	3256	3259	rVB4	623	552	0.00%	0.000%
75	11.551	3260	3269	3276	rBV5	3646	6291	0.01%	0.004%
76	11.631	3276	3294	3330	rVV2	8259794	13728643	21.95%	8.581%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029437.D
 Acq On : 07 Dec 2022 23:26
 Operator : SY/MD
 Sample : N5894-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	12.027	3414	3417	3423	rVB3	766	702	0.00%	0.000%
78	12.066	3426	3429	3431	rVV3	403	237	0.00%	0.000%
79	12.127	3444	3448	3454	rBV6	616	838	0.00%	0.001%
80	12.236	3476	3482	3483	rBV4	1101	1256	0.00%	0.001%
81	12.326	3506	3510	3513	rBV2	560	522	0.00%	0.000%
82	12.390	3524	3530	3537	rVB6	1266	1573	0.00%	0.001%
83	12.603	3594	3596	3599	rVV2	484	231	0.00%	0.000%
84	12.635	3599	3606	3614	rVV5	1848	2636	0.00%	0.002%
85	12.734	3633	3637	3640	rBV4	675	429	0.00%	0.000%
86	12.770	3646	3648	3652	rVV2	395	240	0.00%	0.000%
87	12.914	3689	3693	3695	rBV2	452	338	0.00%	0.000%
88	12.966	3706	3709	3713	rBV3	460	499	0.00%	0.000%
89	12.995	3716	3718	3724	rVB2	492	410	0.00%	0.000%
90	13.024	3725	3727	3730	rBV3	555	333	0.00%	0.000%
91	13.072	3739	3742	3744	rVB2	509	248	0.00%	0.000%
92	13.249	3787	3797	3807	rBV2	42047	63780	0.10%	0.040%
93	13.313	3815	3817	3819	rVB3	469	234	0.00%	0.000%
94	13.332	3820	3823	3828	rVB3	516	329	0.00%	0.000%
95	13.493	3867	3873	3881	rBV3	3872	5810	0.01%	0.004%
96	13.734	3939	3948	3959	rBV6	3651	5935	0.01%	0.004%
97	13.889	3994	3996	4000	rVB4	606	384	0.00%	0.000%
98	13.911	4000	4003	4005	rBV4	646	489	0.00%	0.000%
99	14.027	4037	4039	4041	rVB3	900	406	0.00%	0.000%
100	14.075	4050	4054	4056	rBV3	1020	766	0.00%	0.000%




Sum of corrected areas: 159993472

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029437.D
Acq On : 07 Dec 2022 23:26
Operator : SY/MD
Sample : N5894-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

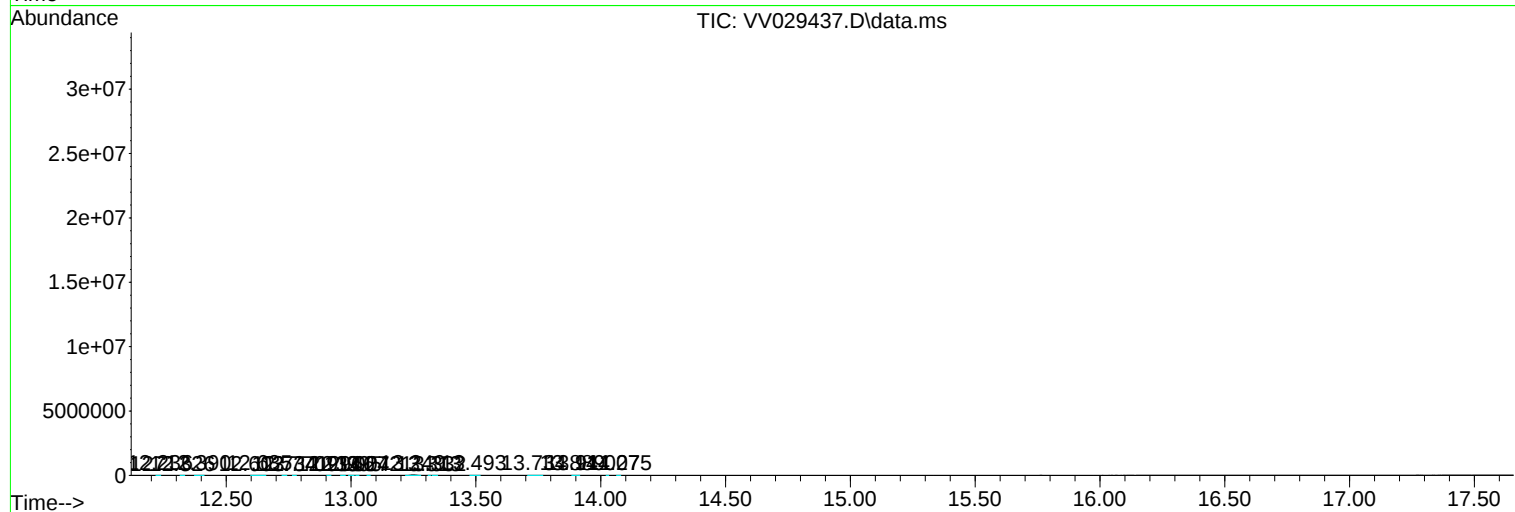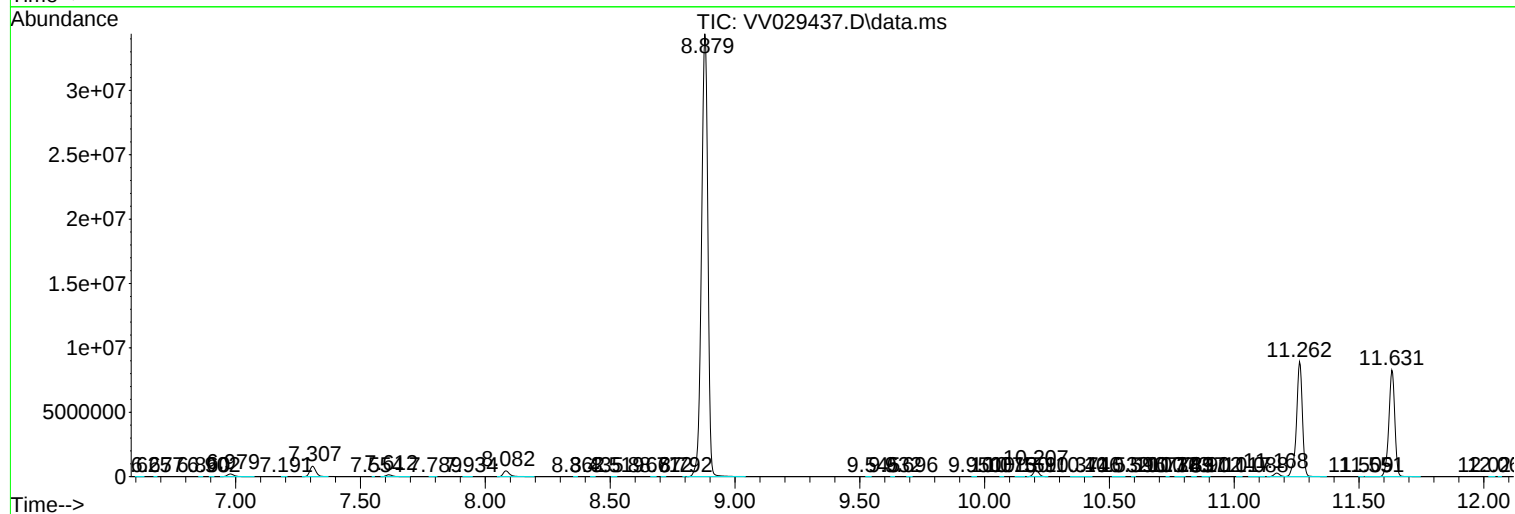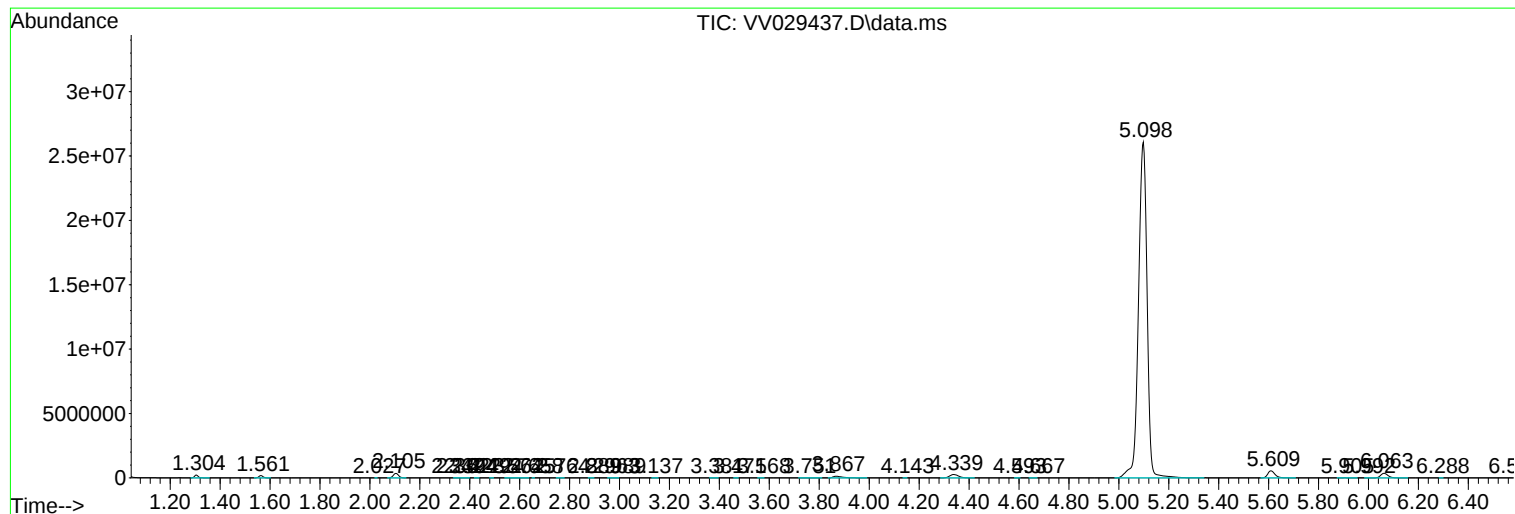

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029437.D
Acq On : 07 Dec 2022 23:26
Operator : SY/MD
Sample : N5894-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029437.D
Acq On : 07 Dec 2022 23:26
Operator : SY/MD
Sample : N5894-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc