

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029438.D
 Acq On : 07 Dec 2022 23:50
 Operator : SY/MD
 Sample : N5919-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rVB	210181	208656	13.02%	1.630%
2	1.561	155	162	174	rVB	161294	180697	11.28%	1.412%
3	1.870	253	258	261	rBV4	2328	2400	0.15%	0.019%
4	2.011	298	302	304	rBV3	379	306	0.02%	0.002%
5	2.105	319	331	344	rBV	322030	453785	28.32%	3.546%
6	2.272	377	383	397	rVB2	4382	8371	0.52%	0.065%
7	2.500	447	454	466	rVB5	1486	2045	0.13%	0.016%
8	2.610	479	488	493	rBV5	939	1324	0.08%	0.010%
9	2.912	579	582	585	rBV2	345	232	0.01%	0.002%
10	3.060	622	628	631	rBV	324	348	0.02%	0.003%
11	3.127	646	649	651	rVV2	292	217	0.01%	0.002%
12	3.166	658	661	666	rBV3	297	236	0.01%	0.002%
13	3.240	680	684	686	rBV2	365	243	0.02%	0.002%
14	3.349	713	718	723	rVB3	311	328	0.02%	0.003%
15	3.622	799	803	806	rVV2	391	272	0.02%	0.002%
16	3.867	869	879	919	rBV	118147	317548	19.82%	2.481%
17	4.339	1009	1026	1049	rBV	237408	582668	36.36%	4.553%
18	4.574	1096	1099	1104	rVB4	467	379	0.02%	0.003%
19	4.712	1138	1142	1147	rVB2	213	231	0.01%	0.002%
20	4.851	1180	1185	1189	rBV3	297	353	0.02%	0.003%
21	4.953	1210	1217	1220	rBV3	397	445	0.03%	0.003%
22	5.040	1225	1244	1290	rBV2	579004	1602363	100.00%	12.520%
23	5.352	1338	1341	1345	rVB2	344	278	0.02%	0.002%
24	5.394	1351	1354	1357	rVB4	521	378	0.02%	0.003%
25	5.458	1369	1374	1375	rBV2	347	209	0.01%	0.002%
26	5.526	1392	1395	1400	rVB2	429	294	0.02%	0.002%
27	5.609	1408	1421	1460	rBV	531841	1072591	66.94%	8.381%
28	5.822	1485	1487	1493	rVB4	397	289	0.02%	0.002%
29	5.902	1501	1512	1527	rVB6	3900	8540	0.53%	0.067%
30	6.063	1547	1562	1597	rBV	324024	677459	42.28%	5.293%
31	6.291	1630	1633	1639	rBV4	359	367	0.02%	0.003%
32	6.500	1693	1698	1701	rBV2	304	245	0.02%	0.002%
33	6.551	1710	1714	1718	rBV3	218	220	0.01%	0.002%
34	6.622	1726	1736	1744	rBV5	1203	2313	0.14%	0.018%
35	6.722	1762	1767	1770	rBV2	333	213	0.01%	0.002%
36	6.783	1783	1786	1790	rVB2	359	277	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029438.D
 Acq On : 07 Dec 2022 23:50
 Operator : SY/MD
 Sample : N5919-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.857	1805	1809	1816	rBV2	427	458	0.03%	0.004%
38	6.924	1828	1830	1835	rBV3	284	206	0.01%	0.002%
39	6.979	1835	1847	1878	rBV	190680	356407	22.24%	2.785%
40	7.236	1924	1927	1931	rVB3	543	430	0.03%	0.003%
41	7.307	1936	1949	1983	rBV	723661	1297347	80.96%	10.137%
42	7.613	2034	2044	2070	rBV	132917	233077	14.55%	1.821%
43	7.934	2134	2144	2156	rBV	2677	4970	0.31%	0.039%
44	7.979	2156	2158	2162	rVB3	333	216	0.01%	0.002%
45	8.021	2167	2171	2175	rBV4	236	254	0.02%	0.002%
46	8.082	2179	2190	2235	rBV	421616	769155	48.00%	6.010%
47	8.326	2263	2266	2269	rBV4	493	301	0.02%	0.002%
48	8.461	2304	2308	2313	rBV5	383	470	0.03%	0.004%
49	8.638	2358	2363	2366	rBV3	314	357	0.02%	0.003%
50	8.709	2379	2385	2388	rBV3	403	435	0.03%	0.003%
51	8.844	2410	2427	2455	rBV	781549	1436607	89.66%	11.225%
52	9.079	2495	2500	2501	rBV2	243	213	0.01%	0.002%
53	9.378	2587	2593	2594	rBV2	273	294	0.02%	0.002%
54	9.526	2633	2639	2643	rBV3	404	521	0.03%	0.004%
55	9.567	2650	2652	2655	rBV	328	241	0.02%	0.002%
56	9.632	2669	2672	2675	rBV2	303	286	0.02%	0.002%
57	9.722	2694	2700	2704	rBV	432	441	0.03%	0.003%
58	9.760	2708	2712	2715	rBV3	278	231	0.01%	0.002%
59	9.866	2741	2745	2749	rBV3	461	495	0.03%	0.004%
60	9.915	2758	2760	2763	rBV2	524	444	0.03%	0.003%
61	9.956	2769	2773	2777	rVB3	371	360	0.02%	0.003%
62	10.085	2810	2813	2817	rVB	382	268	0.02%	0.002%
63	10.124	2821	2825	2829	rBV2	267	320	0.02%	0.003%
64	10.207	2837	2851	2874	rVV	498583	793433	49.52%	6.199%
65	10.374	2896	2903	2916	rVB4	2862	4404	0.27%	0.034%
66	10.497	2937	2941	2944	rVB3	422	342	0.02%	0.003%
67	10.619	2973	2979	2983	rBV2	331	246	0.02%	0.002%
68	10.725	3010	3012	3015	rVB	471	220	0.01%	0.002%
69	10.760	3019	3023	3030	rBV3	250	317	0.02%	0.002%
70	10.796	3030	3034	3040	rVB2	265	280	0.02%	0.002%
71	10.841	3045	3048	3053	rVB4	569	392	0.02%	0.003%
72	10.908	3062	3069	3072	rBV3	558	635	0.04%	0.005%
73	10.937	3075	3078	3080	rBV2	452	338	0.02%	0.003%
74	10.969	3085	3088	3093	rVB4	336	307	0.02%	0.002%
75	11.037	3106	3109	3113	rVB4	354	287	0.02%	0.002%
76	11.172	3144	3151	3160	rBV6	2915	4268	0.27%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029438.D
 Acq On : 07 Dec 2022 23:50
 Operator : SY/MD
 Sample : N5919-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.239	3160	3172	3197	rBV	839616	1410246	88.01%	11.019%
78	11.461	3239	3241	3244	rBV2	460	282	0.02%	0.002%
79	11.548	3261	3268	3276	rBV4	2643	4353	0.27%	0.034%
80	11.612	3276	3288	3323	rVV	787597	1329292	82.96%	10.386%
81	11.821	3350	3353	3355	rBV2	355	206	0.01%	0.002%
82	11.902	3374	3378	3379	rBV2	339	229	0.01%	0.002%
83	12.149	3452	3455	3457	rBV2	334	263	0.02%	0.002%
84	12.236	3474	3482	3483	rBV3	950	928	0.06%	0.007%
85	12.345	3512	3516	3519	rVB3	399	305	0.02%	0.002%
86	12.381	3523	3527	3530	rVB3	284	212	0.01%	0.002%
87	12.435	3542	3544	3548	rBV3	393	278	0.02%	0.002%
88	12.583	3582	3590	3592	rBV3	528	584	0.04%	0.005%
89	12.603	3592	3596	3600	rVB3	394	329	0.02%	0.003%
90	12.635	3600	3606	3614	rBV3	965	1519	0.09%	0.012%
91	12.670	3614	3617	3620	rBV3	404	269	0.02%	0.002%
92	12.780	3648	3651	3654	rBV3	500	300	0.02%	0.002%
93	12.805	3656	3659	3666	rVB5	819	954	0.06%	0.007%
94	12.844	3667	3671	3673	rBV4	500	327	0.02%	0.003%
95	12.905	3686	3690	3692	rBV2	372	293	0.02%	0.002%
96	12.963	3706	3708	3712	rBV3	283	231	0.01%	0.002%
97	13.169	3770	3772	3777	rBV3	440	389	0.02%	0.003%
98	13.252	3791	3798	3807	rVV7	2518	4012	0.25%	0.031%
99	13.497	3868	3874	3884	rVB2	2425	3477	0.22%	0.027%
100	13.734	3942	3948	3954	rVB5	1343	1698	0.11%	0.013%




Sum of corrected areas: 12798369

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029438.D
Acq On : 07 Dec 2022 23:50
Operator : SY/MD
Sample : N5919-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

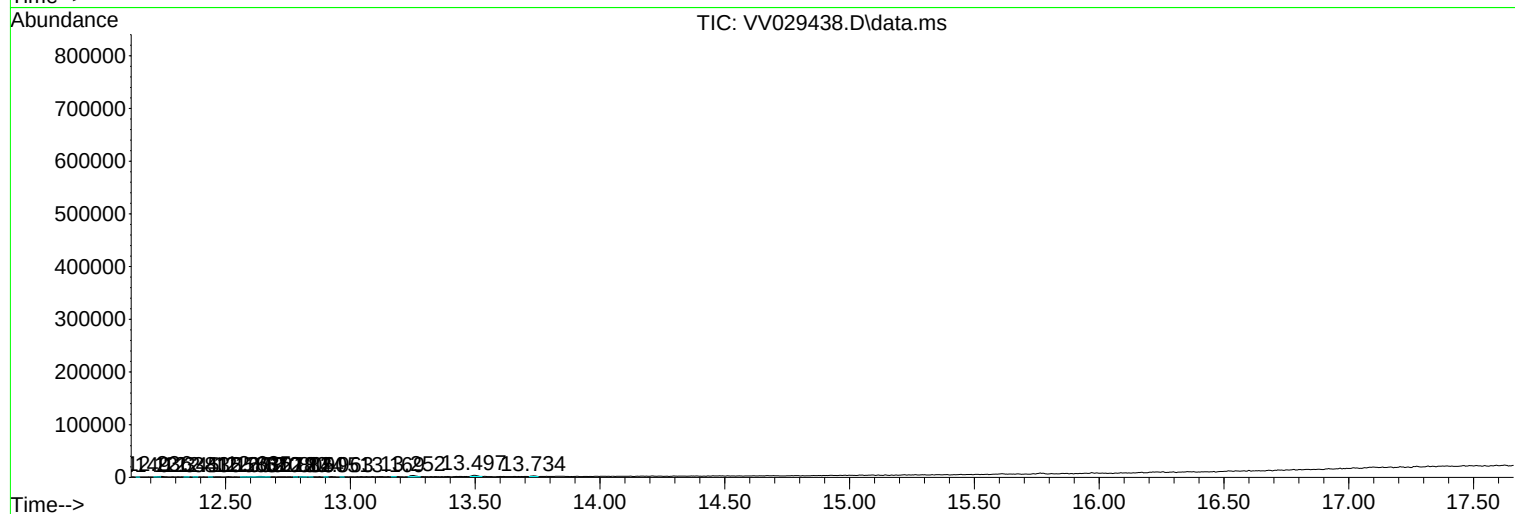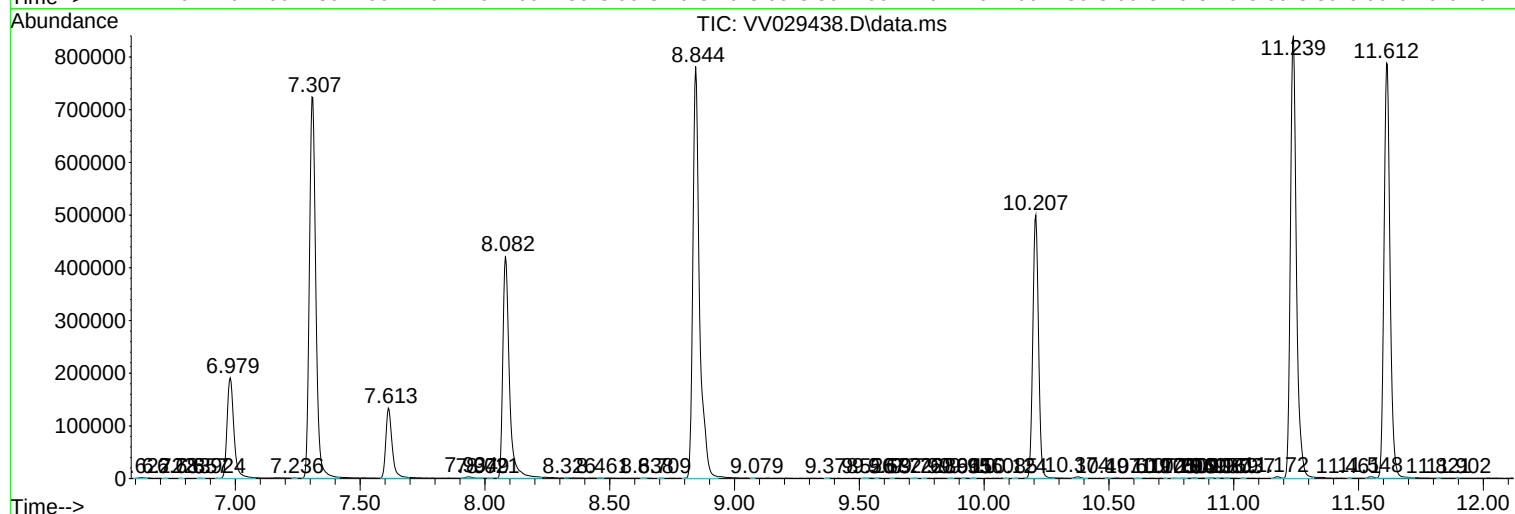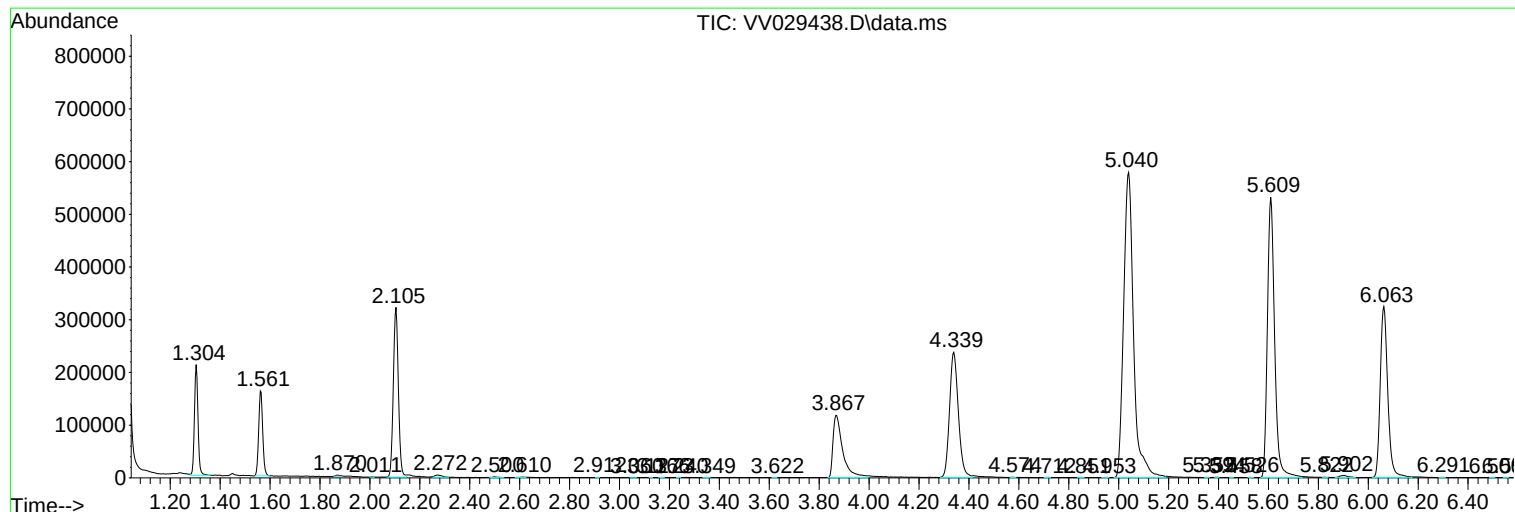

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029438.D
Acq On : 07 Dec 2022 23:50
Operator : SY/MD
Sample : N5919-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029438.D
Acq On : 07 Dec 2022 23:50
Operator : SY/MD
Sample : N5919-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc