

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029439.D
 Acq On : 08 Dec 2022 00:13
 Operator : SY/MD
 Sample : N5919-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029439.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	45	50	59	rVB	34256	30551	0.43%	0.144%
2	1.304	75	82	96	rVB	210133	205949	2.90%	0.972%
3	1.561	155	162	181	rVB	165624	191723	2.70%	0.905%
4	1.873	253	259	266	rBV3	5194	6524	0.09%	0.031%
5	2.108	319	332	361	rBV3	455811	777072	10.94%	3.667%
6	2.269	373	382	398	rVB2	10747	21073	0.30%	0.099%
7	2.506	449	456	461	rBV3	1453	1825	0.03%	0.009%
8	2.532	461	464	468	rVB2	368	244	0.00%	0.001%
9	2.558	470	472	477	rVB3	438	257	0.00%	0.001%
10	2.616	485	490	493	rBV2	478	522	0.01%	0.002%
11	2.632	493	495	498	rVB2	596	336	0.00%	0.002%
12	2.648	498	500	505	rVB	438	344	0.00%	0.002%
13	2.751	527	532	534	rBV2	910	763	0.01%	0.004%
14	2.767	534	537	541	rVB4	1214	1016	0.01%	0.005%
15	3.069	623	631	634	rBV2	309	388	0.01%	0.002%
16	3.182	656	666	687	rVB	6490	13165	0.19%	0.062%
17	3.442	744	747	752	rVB2	265	248	0.00%	0.001%
18	3.683	819	822	829	rVB2	349	336	0.00%	0.002%
19	3.722	829	834	842	rBV3	342	401	0.01%	0.002%
20	3.767	842	848	852	rBV2	192	262	0.00%	0.001%
21	3.899	870	889	933	rBV2	268642	920340	12.95%	4.343%
22	4.339	1009	1026	1056	rBV2	246784	612617	8.62%	2.891%
23	4.600	1089	1107	1129	rBV2	125547	315242	4.44%	1.488%
24	5.040	1220	1244	1284	rBV2	604209	1615264	22.73%	7.622%
25	5.490	1380	1384	1388	rVB2	463	396	0.01%	0.002%
26	5.609	1406	1421	1463	rBV	539596	1109947	15.62%	5.238%
27	5.905	1498	1513	1548	rBV	3661585	7105053	100.00%	33.528%
28	6.063	1550	1562	1592	rVB	349494	721447	10.15%	3.404%
29	6.281	1627	1630	1633	rVB4	577	361	0.01%	0.002%
30	6.397	1662	1666	1669	rVB3	441	267	0.00%	0.001%
31	6.413	1669	1671	1676	rBV3	363	278	0.00%	0.001%
32	6.603	1727	1730	1731	rBV	825	392	0.01%	0.002%
33	6.709	1757	1763	1765	rVB3	338	330	0.00%	0.002%
34	6.792	1787	1789	1797	rVB3	369	353	0.00%	0.002%
35	6.931	1828	1832	1835	rBV3	475	353	0.00%	0.002%
36	6.979	1835	1847	1871	rBV	201773	366755	5.16%	1.731%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029439.D
 Acq On : 08 Dec 2022 00:13
 Operator : SY/MD
 Sample : N5919-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.233	1923	1926	1930	rVB3	400	282	0.00%	0.001%
38	7.310	1934	1950	1978	rBV	751657	1335813	18.80%	6.304%
39	7.612	2034	2044	2070	rBV	134445	241452	3.40%	1.139%
40	7.831	2105	2112	2113	rBV4	3281	2708	0.04%	0.013%
41	7.911	2133	2137	2138	rBV2	565	376	0.01%	0.002%
42	7.937	2138	2145	2152	rVB4	2020	3255	0.05%	0.015%
43	7.969	2152	2155	2158	rBV4	704	522	0.01%	0.002%
44	8.082	2179	2190	2222	rBV	433515	786638	11.07%	3.712%
45	8.268	2244	2248	2253	rVB4	1137	966	0.01%	0.005%
46	8.423	2295	2296	2302	rVB2	661	485	0.01%	0.002%
47	8.461	2302	2308	2311	rBV4	481	573	0.01%	0.003%
48	8.554	2331	2337	2341	rVB2	606	582	0.01%	0.003%
49	8.583	2341	2346	2349	rBV3	347	362	0.01%	0.002%
50	8.699	2379	2382	2386	rVB2	284	249	0.00%	0.001%
51	8.844	2414	2427	2459	rBV	787020	1357189	19.10%	6.405%
52	9.252	2549	2554	2556	rBV	337	327	0.00%	0.002%
53	9.426	2604	2608	2611	rVB3	358	315	0.00%	0.001%
54	9.452	2611	2616	2618	rBV2	386	260	0.00%	0.001%
55	9.480	2623	2625	2631	rVB2	483	428	0.01%	0.002%
56	9.516	2631	2636	2639	rBV2	438	422	0.01%	0.002%
57	9.538	2639	2643	2645	rBV2	372	281	0.00%	0.001%
58	9.886	2748	2751	2756	rVB3	379	320	0.00%	0.002%
59	9.921	2758	2762	2764	rBV3	407	333	0.00%	0.002%
60	10.050	2799	2802	2808	rVB2	400	327	0.00%	0.002%
61	10.085	2808	2813	2815	rBV2	327	273	0.00%	0.001%
62	10.207	2839	2851	2871	rBV	522380	821285	11.56%	3.876%
63	10.307	2880	2882	2887	rVB3	667	513	0.01%	0.002%
64	10.374	2893	2903	2910	rBV6	2926	4919	0.07%	0.023%
65	10.525	2946	2950	2951	rBV2	399	282	0.00%	0.001%
66	10.567	2957	2963	2967	rBV4	348	390	0.01%	0.002%
67	10.632	2979	2983	2986	rBV	431	364	0.01%	0.002%
68	10.738	3013	3016	3019	rBV2	383	253	0.00%	0.001%
69	10.837	3045	3047	3052	rVB4	763	679	0.01%	0.003%
70	10.915	3065	3071	3075	rVB4	587	735	0.01%	0.003%
71	10.950	3075	3082	3085	rBV2	819	1065	0.01%	0.005%
72	10.979	3088	3091	3097	rBV2	318	325	0.00%	0.002%
73	11.095	3125	3127	3133	rVB2	336	265	0.00%	0.001%
74	11.172	3146	3151	3156	rVV4	1104	1262	0.02%	0.006%
75	11.239	3159	3172	3201	rBV	849316	1332986	18.76%	6.290%
76	11.416	3225	3227	3232	rVB2	363	252	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029439.D
 Acq On : 08 Dec 2022 00:13
 Operator : SY/MD
 Sample : N5919-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.471	3242	3244	3251	rVB3	411	392	0.01%	0.002%
78	11.525	3255	3261	3263	rBV2	446	396	0.01%	0.002%
79	11.551	3263	3269	3276	rBV6	2122	3378	0.05%	0.016%
80	11.612	3276	3288	3314	rBV	787140	1253024	17.64%	5.913%
81	12.062	3425	3428	3432	rBV3	348	344	0.00%	0.002%
82	12.082	3432	3434	3439	rVB2	347	285	0.00%	0.001%
83	12.246	3481	3485	3493	rVB4	1075	1222	0.02%	0.006%
84	12.400	3531	3533	3537	rVV4	450	355	0.00%	0.002%
85	12.439	3542	3545	3548	rVB	441	340	0.00%	0.002%
86	12.480	3555	3558	3561	rBV3	333	277	0.00%	0.001%
87	12.564	3582	3584	3588	rBV3	463	399	0.01%	0.002%
88	12.638	3602	3607	3616	rVB6	805	1026	0.01%	0.005%
89	12.908	3690	3691	3695	rBV2	383	285	0.00%	0.001%
90	13.130	3757	3760	3761	rBV	505	251	0.00%	0.001%
91	13.226	3787	3790	3792	rBV2	483	296	0.00%	0.001%
92	13.249	3792	3797	3799	rBV3	1181	1087	0.02%	0.005%
93	13.342	3821	3826	3830	rBV5	599	639	0.01%	0.003%
94	13.500	3869	3875	3879	rBV3	1569	1563	0.02%	0.007%
95	13.731	3943	3947	3949	rBV3	1008	886	0.01%	0.004%
96	13.860	3985	3987	3988	rBV2	484	261	0.00%	0.001%
97	13.911	4001	4003	4007	rBV4	618	506	0.01%	0.002%
98	14.024	4036	4038	4041	rBV3	653	321	0.00%	0.002%
99	14.130	4068	4071	4073	rBV3	534	295	0.00%	0.001%
100	14.258	4108	4111	4113	rBV3	690	551	0.01%	0.003%




Sum of corrected areas: 21191086

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029439.D
Acq On : 08 Dec 2022 00:13
Operator : SY/MD
Sample : N5919-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

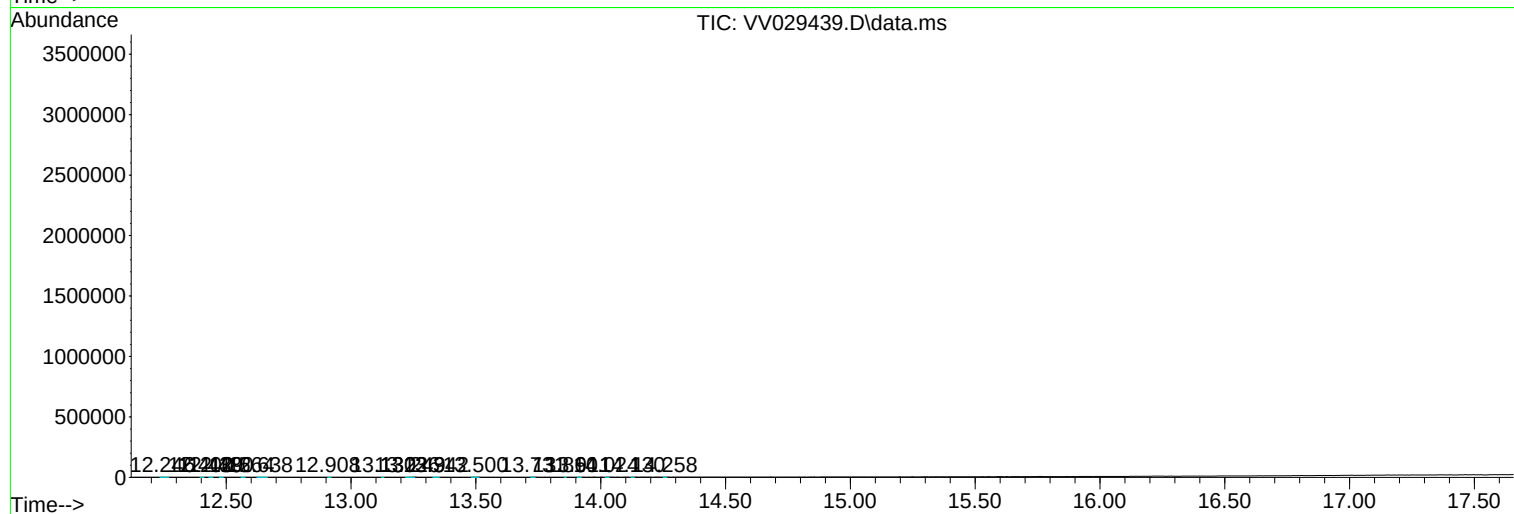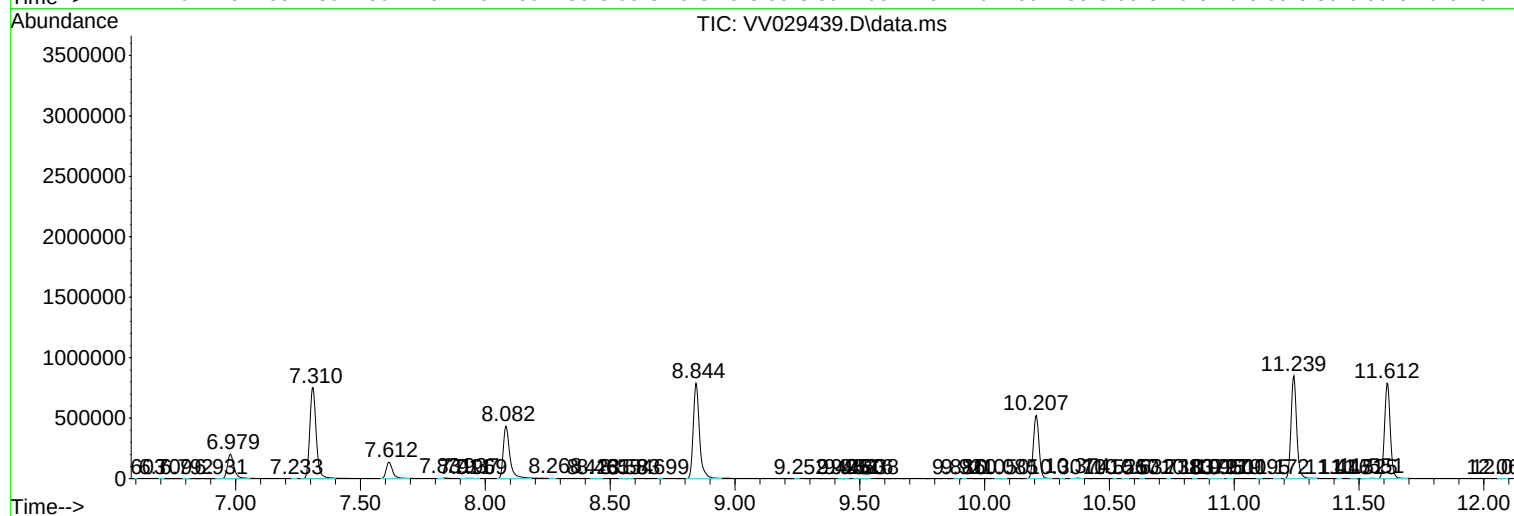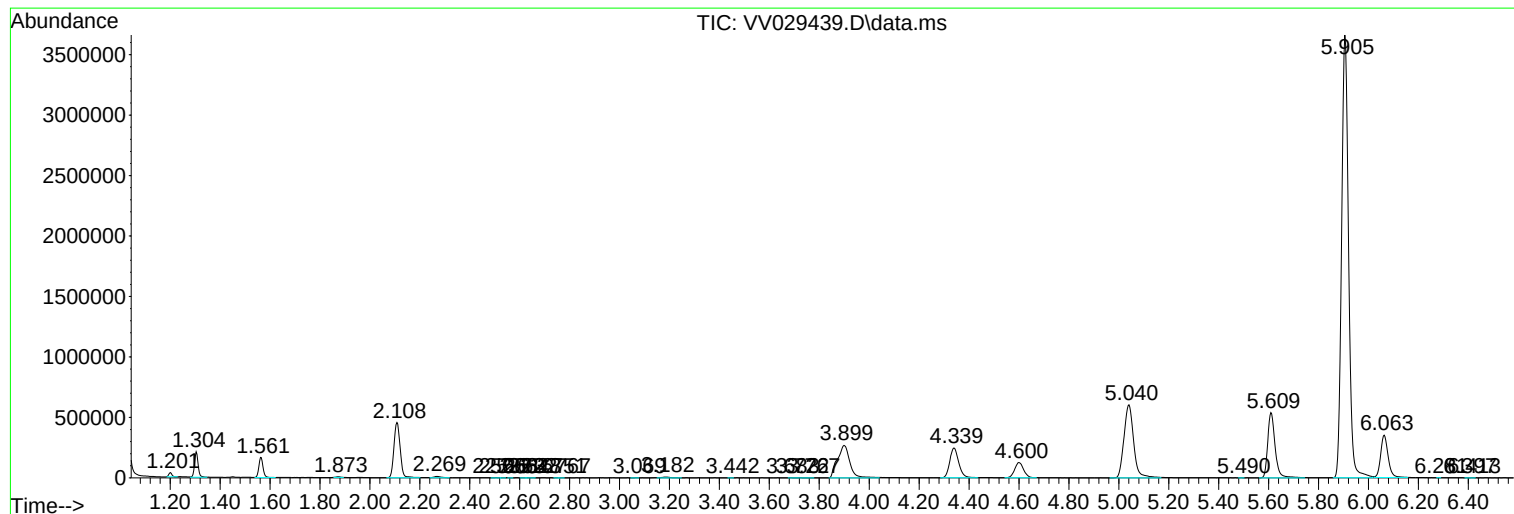

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029439.D
Acq On : 08 Dec 2022 00:13
Operator : SY/MD
Sample : N5919-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029439.D
Acq On : 08 Dec 2022 00:13
Operator : SY/MD
Sample : N5919-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------