

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029440.D
 Acq On : 08 Dec 2022 00:37
 Operator : SY/MD
 Sample : N5919-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029440.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	45	50	58	rVB	28284	25083	1.63%	0.202%
2	1.304	75	82	103	rVB	209300	208493	13.58%	1.676%
3	1.561	154	162	182	rVB	160754	180930	11.79%	1.454%
4	2.105	319	331	345	rBV	311503	448837	29.24%	3.608%
5	2.433	429	433	436	rBV2	321	287	0.02%	0.002%
6	2.503	449	455	461	rVB3	874	1254	0.08%	0.010%
7	2.626	482	493	495	rBV3	1022	1464	0.10%	0.012%
8	2.696	511	515	519	rBV	286	274	0.02%	0.002%
9	2.812	547	551	553	rBV2	398	258	0.02%	0.002%
10	2.957	588	596	599	rBV5	661	827	0.05%	0.007%
11	2.992	604	607	609	rBV2	258	209	0.01%	0.002%
12	3.073	625	632	635	rBV2	255	203	0.01%	0.002%
13	3.150	651	656	662	rBV3	306	294	0.02%	0.002%
14	3.355	717	720	723	rBV2	326	222	0.01%	0.002%
15	3.526	768	773	777	rBV2	247	226	0.01%	0.002%
16	3.626	800	804	807	rBV2	304	192	0.01%	0.002%
17	3.870	870	880	918	rBV	117366	315979	20.58%	2.540%
18	4.339	1008	1026	1065	rBV	234284	584241	38.06%	4.696%
19	4.699	1136	1138	1144	rVB2	257	204	0.01%	0.002%
20	5.040	1225	1244	1281	rBV2	577118	1535036	100.00%	12.338%
21	5.320	1327	1331	1334	rBV2	313	287	0.02%	0.002%
22	5.391	1348	1353	1355	rBV3	478	395	0.03%	0.003%
23	5.468	1374	1377	1382	rBV4	516	447	0.03%	0.004%
24	5.609	1407	1421	1458	rBV	529738	1084282	70.64%	8.715%
25	5.806	1479	1482	1484	rBV3	425	260	0.02%	0.002%
26	5.912	1502	1515	1533	rBV7	12147	27890	1.82%	0.224%
27	6.005	1540	1544	1548	rBV2	182	208	0.01%	0.002%
28	6.063	1548	1562	1595	rBV	328968	681138	44.37%	5.475%
29	6.191	1600	1602	1606	rBV3	480	431	0.03%	0.003%
30	6.236	1614	1616	1620	rVB3	566	467	0.03%	0.004%
31	6.378	1657	1660	1664	rVB2	349	274	0.02%	0.002%
32	6.433	1672	1677	1681	rBV2	249	260	0.02%	0.002%
33	6.468	1681	1688	1690	rBV3	359	305	0.02%	0.002%
34	6.490	1690	1695	1698	rVB2	270	250	0.02%	0.002%
35	6.513	1698	1702	1705	rBV	275	218	0.01%	0.002%
36	6.625	1727	1737	1744	rBV5	1379	2590	0.17%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029440.D
 Acq On : 08 Dec 2022 00:37
 Operator : SY/MD
 Sample : N5919-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.886	1810	1818	1820	rBV2	403	447	0.03%	0.004%
38	6.979	1835	1847	1881	rBV	189767	352945	22.99%	2.837%
39	7.146	1896	1899	1902	rBV2	472	336	0.02%	0.003%
40	7.307	1934	1949	1991	rBV	720720	1286356	83.80%	10.339%
41	7.613	2033	2044	2072	rBV	131886	232340	15.14%	1.867%
42	7.899	2129	2133	2135	rBV2	404	314	0.02%	0.003%
43	7.934	2135	2144	2155	rVB3	1981	3635	0.24%	0.029%
44	8.018	2167	2170	2173	rBV4	334	294	0.02%	0.002%
45	8.082	2176	2190	2232	rBV	425716	763845	49.76%	6.139%
46	8.522	2324	2327	2328	rBV2	339	197	0.01%	0.002%
47	8.648	2363	2366	2369	rVB3	302	222	0.01%	0.002%
48	8.693	2378	2380	2384	rBV2	371	263	0.02%	0.002%
49	8.844	2415	2427	2457	rBV	777769	1297921	84.55%	10.432%
50	9.201	2534	2538	2542	rBV3	473	430	0.03%	0.003%
51	9.307	2564	2571	2574	rBV2	470	526	0.03%	0.004%
52	9.330	2574	2578	2581	rVV2	344	291	0.02%	0.002%
53	9.358	2584	2587	2591	rBV	297	212	0.01%	0.002%
54	9.474	2617	2623	2626	rBV2	236	313	0.02%	0.003%
55	9.494	2626	2629	2634	rVB3	424	340	0.02%	0.003%
56	9.529	2637	2640	2644	rBV3	324	285	0.02%	0.002%
57	9.645	2673	2676	2679	rVV	268	244	0.02%	0.002%
58	9.735	2700	2704	2706	rBV2	244	190	0.01%	0.002%
59	9.776	2712	2717	2721	rBV4	359	436	0.03%	0.004%
60	9.802	2721	2725	2730	rVB3	418	449	0.03%	0.004%
61	9.915	2757	2760	2764	rBV3	439	381	0.02%	0.003%
62	10.159	2833	2836	2838	rBV3	360	271	0.02%	0.002%
63	10.207	2838	2851	2877	rVV	502749	793408	51.69%	6.377%
64	10.326	2886	2888	2893	rVB3	560	340	0.02%	0.003%
65	10.371	2893	2902	2910	rBV6	2103	3572	0.23%	0.029%
66	10.490	2935	2939	2943	rBV3	313	308	0.02%	0.002%
67	10.519	2943	2948	2949	rVV3	310	236	0.02%	0.002%
68	10.532	2949	2952	2958	rVB3	570	457	0.03%	0.004%
69	10.577	2960	2966	2968	rBV2	223	263	0.02%	0.002%
70	10.812	3035	3039	3043	rVB3	629	456	0.03%	0.004%
71	10.841	3044	3048	3057	rVB4	629	932	0.06%	0.007%
72	10.883	3057	3061	3063	rBV2	264	208	0.01%	0.002%
73	10.908	3063	3069	3072	rBV3	455	536	0.03%	0.004%
74	11.178	3146	3153	3159	rVB4	1353	1728	0.11%	0.014%
75	11.236	3159	3171	3198	rBV	845018	1334019	86.90%	10.722%
76	11.394	3217	3220	3226	rVV3	347	334	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029440.D
 Acq On : 08 Dec 2022 00:37
 Operator : SY/MD
 Sample : N5919-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.442	3230	3235	3238	rBV3	360	364	0.02%	0.003%
78	11.471	3242	3244	3247	rVB3	338	215	0.01%	0.002%
79	11.548	3260	3268	3276	rBV4	4185	6845	0.45%	0.055%
80	11.612	3276	3288	3314	rVV	779604	1242822	80.96%	9.989%
81	11.757	3331	3333	3336	rBV2	344	196	0.01%	0.002%
82	11.802	3345	3347	3351	rVB3	348	193	0.01%	0.002%
83	11.850	3360	3362	3366	rVB3	433	247	0.02%	0.002%
84	11.927	3384	3386	3389	rBV2	374	225	0.01%	0.002%
85	12.075	3429	3432	3436	rBV3	404	342	0.02%	0.003%
86	12.159	3453	3458	3460	rVB2	537	342	0.02%	0.003%
87	12.214	3471	3475	3477	rBV2	514	324	0.02%	0.003%
88	12.297	3498	3501	3505	rBV4	333	315	0.02%	0.003%
89	12.400	3531	3533	3536	rBV2	386	268	0.02%	0.002%
90	12.468	3550	3554	3556	rVV	293	212	0.01%	0.002%
91	12.500	3561	3564	3567	rBV3	280	202	0.01%	0.002%
92	12.558	3580	3582	3585	rBV3	384	218	0.01%	0.002%
93	12.596	3592	3594	3599	rVB2	475	300	0.02%	0.002%
94	12.625	3601	3603	3604	rBV	388	198	0.01%	0.002%
95	12.728	3632	3635	3637	rBV2	288	196	0.01%	0.002%
96	12.783	3647	3652	3656	rBV3	590	670	0.04%	0.005%
97	13.027	3726	3728	3731	rVB2	420	243	0.02%	0.002%
98	13.371	3830	3835	3841	rBV5	623	843	0.05%	0.007%
99	13.423	3848	3851	3853	rBV4	449	246	0.02%	0.002%
100	13.497	3869	3874	3875	rBV5	1263	971	0.06%	0.008%




Sum of corrected areas: 12441492

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029440.D
Acq On : 08 Dec 2022 00:37
Operator : SY/MD
Sample : N5919-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

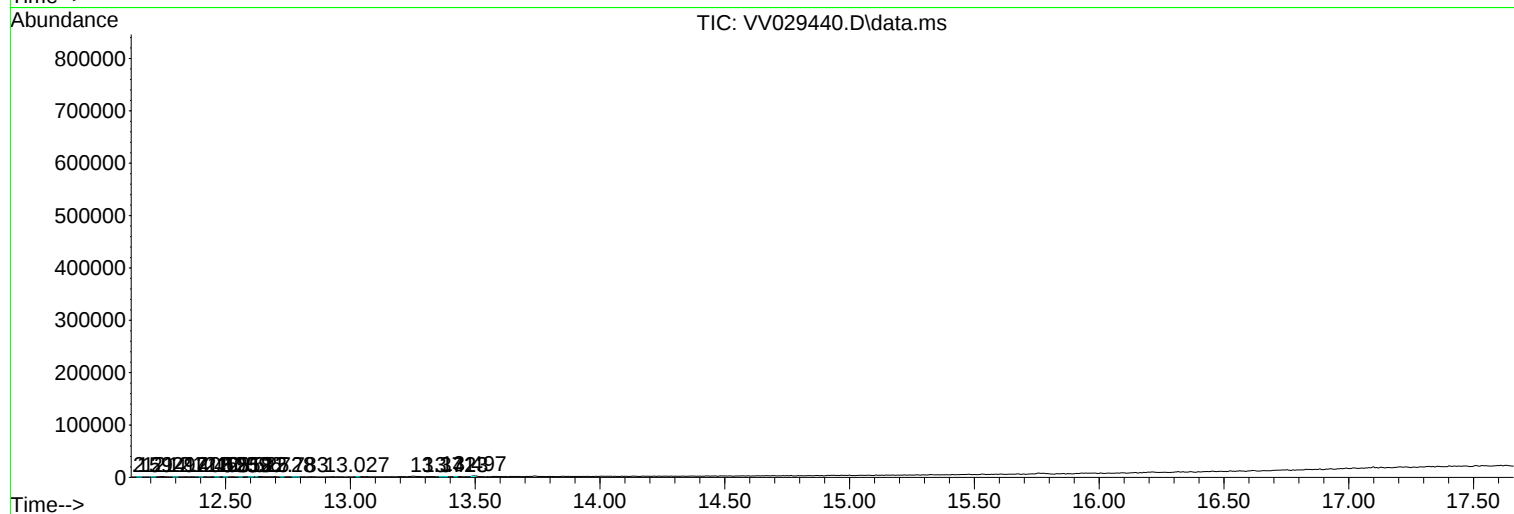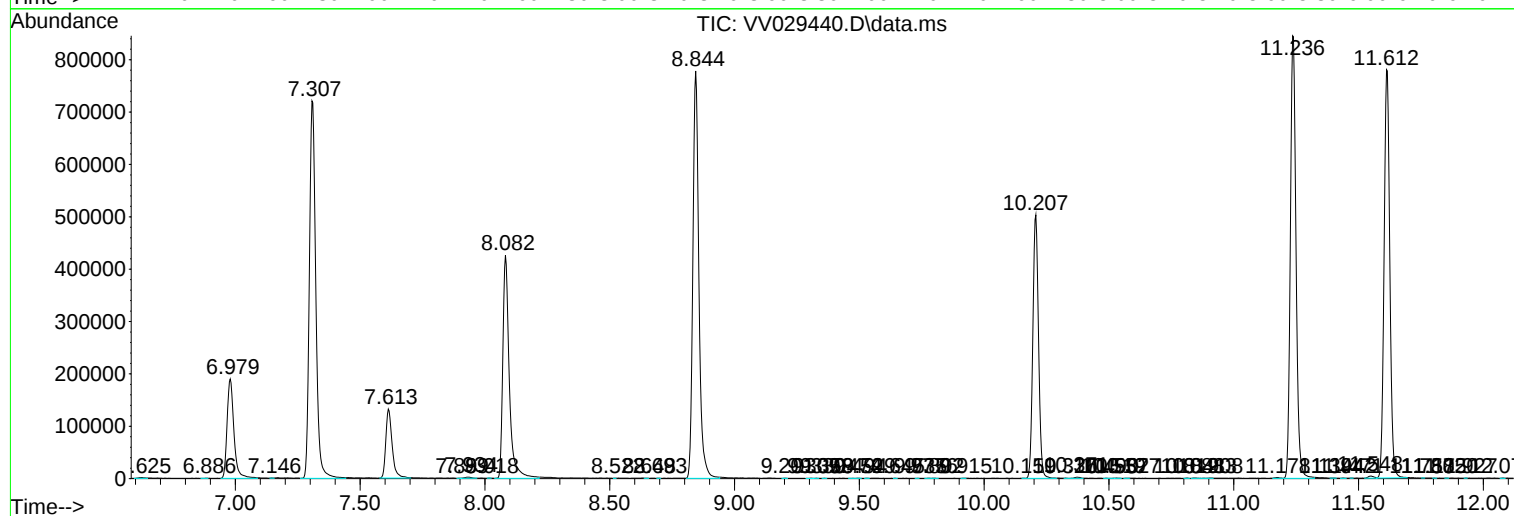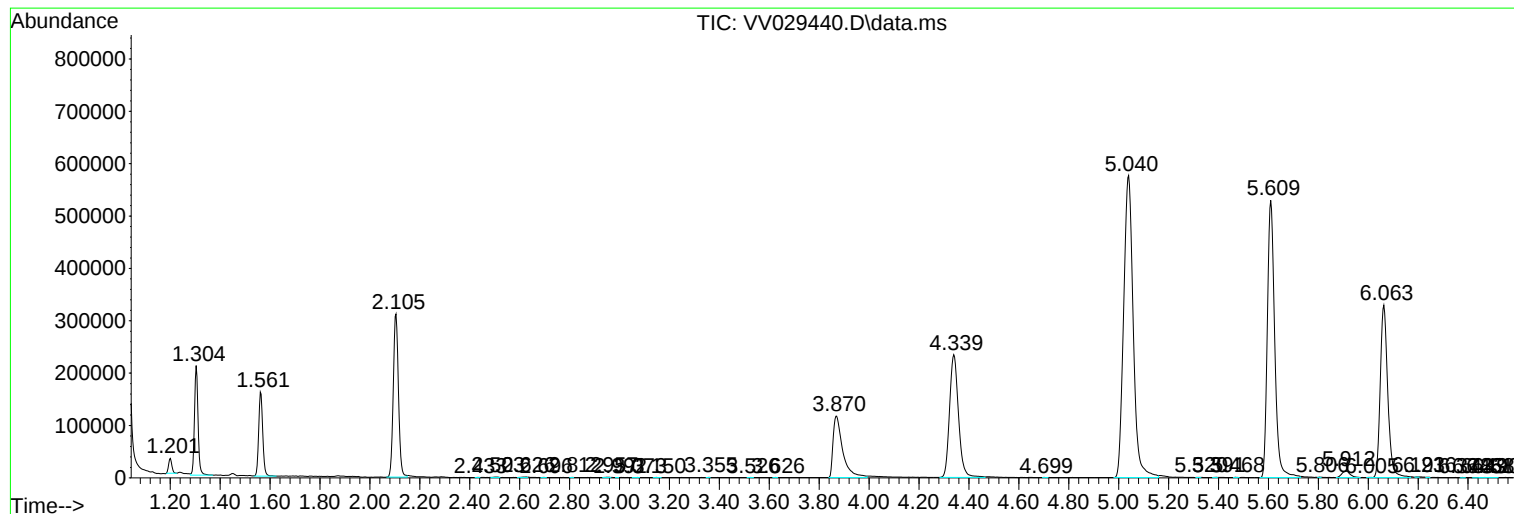

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029440.D
Acq On : 08 Dec 2022 00:37
Operator : SY/MD
Sample : N5919-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029440.D
Acq On : 08 Dec 2022 00:37
Operator : SY/MD
Sample : N5919-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc