

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029441.D
 Acq On : 08 Dec 2022 01:01
 Operator : SY/MD
 Sample : N5919-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rVB	206862	206808	12.81%	1.590%
2	1.561	155	162	181	rVB	166428	190180	11.78%	1.462%
3	2.047	311	313	316	rBV4	463	273	0.02%	0.002%
4	2.105	319	331	344	rBV	324066	468125	28.99%	3.599%
5	2.503	448	455	461	rVV5	939	1303	0.08%	0.010%
6	2.619	481	491	492	rBV3	1119	1294	0.08%	0.010%
7	2.690	511	513	518	rVB	419	217	0.01%	0.002%
8	2.757	529	534	537	rVB3	443	371	0.02%	0.003%
9	2.783	541	542	549	rVB2	307	205	0.01%	0.002%
10	2.844	552	561	565	rVB3	381	453	0.03%	0.003%
11	2.870	565	569	577	rBV2	336	381	0.02%	0.003%
12	2.954	586	595	596	rBV3	961	981	0.06%	0.008%
13	3.323	704	710	713	rBV3	229	286	0.02%	0.002%
14	3.513	765	769	773	rVB2	256	243	0.02%	0.002%
15	3.719	830	833	836	rBV3	309	257	0.02%	0.002%
16	3.793	853	856	859	rVV2	278	217	0.01%	0.002%
17	3.870	870	880	919	rBV	120774	324892	20.12%	2.498%
18	4.339	1009	1026	1050	rBV2	246790	610390	37.80%	4.692%
19	4.568	1093	1097	1100	rBV5	309	344	0.02%	0.003%
20	4.606	1107	1109	1116	rVB3	333	280	0.02%	0.002%
21	5.040	1226	1244	1284	rBV2	606612	1614921	100.00%	12.414%
22	5.387	1348	1352	1354	rBV2	343	224	0.01%	0.002%
23	5.455	1366	1373	1376	rBV4	267	283	0.02%	0.002%
24	5.609	1408	1421	1449	rBV	547098	1113981	68.98%	8.563%
25	5.908	1501	1514	1533	rBV2	72788	152176	9.42%	1.170%
26	6.063	1547	1562	1597	rBV	347761	712597	44.13%	5.478%
27	6.301	1632	1636	1640	rVB4	374	299	0.02%	0.002%
28	6.542	1704	1711	1715	rBV3	493	424	0.03%	0.003%
29	6.619	1726	1735	1737	rBV5	1016	1240	0.08%	0.010%
30	6.802	1789	1792	1793	rBV2	375	251	0.02%	0.002%
31	6.867	1807	1812	1815	rVB3	385	312	0.02%	0.002%
32	6.918	1824	1828	1829	rBV	536	282	0.02%	0.002%
33	6.979	1836	1847	1883	rBV	201549	370721	22.96%	2.850%
34	7.149	1896	1900	1902	rBV2	683	526	0.03%	0.004%
35	7.310	1937	1950	1986	rVV	746306	1337570	82.83%	10.282%
36	7.612	2033	2044	2065	rBV	136911	240557	14.90%	1.849%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029441.D
 Acq On : 08 Dec 2022 01:01
 Operator : SY/MD
 Sample : N5919-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.741	2081	2084	2086	rVB2	522	230	0.01%	0.002%
38	7.850	2115	2118	2121	rBV3	580	387	0.02%	0.003%
39	7.934	2136	2144	2154	rVB3	2315	4052	0.25%	0.031%
40	8.082	2180	2190	2230	rBV	429973	789285	48.87%	6.067%
41	8.336	2265	2269	2273	rBV4	557	448	0.03%	0.003%
42	8.423	2290	2296	2298	rBV4	527	599	0.04%	0.005%
43	8.674	2369	2374	2379	rVB5	418	509	0.03%	0.004%
44	8.709	2379	2385	2387	rBV2	347	375	0.02%	0.003%
45	8.754	2397	2399	2401	rBV2	358	225	0.01%	0.002%
46	8.844	2415	2427	2461	rBV	792538	1337444	82.82%	10.281%
47	8.995	2472	2474	2478	rBV4	437	246	0.02%	0.002%
48	9.085	2499	2502	2505	rBV4	413	314	0.02%	0.002%
49	9.130	2513	2516	2518	rBV4	446	278	0.02%	0.002%
50	9.207	2538	2540	2546	rVB4	600	453	0.03%	0.003%
51	9.233	2546	2548	2552	rBV2	247	219	0.01%	0.002%
52	9.384	2592	2595	2599	rBV2	276	252	0.02%	0.002%
53	9.432	2607	2610	2613	rBV	315	281	0.02%	0.002%
54	9.513	2631	2635	2640	rBV2	307	290	0.02%	0.002%
55	9.542	2640	2644	2647	rVV2	388	281	0.02%	0.002%
56	9.564	2647	2651	2656	rVV3	573	558	0.03%	0.004%
57	9.590	2656	2659	2663	rVB3	298	268	0.02%	0.002%
58	9.677	2682	2686	2687	rBV2	366	244	0.02%	0.002%
59	9.699	2690	2693	2695	rBV3	390	298	0.02%	0.002%
60	9.760	2709	2712	2716	rBV4	345	261	0.02%	0.002%
61	9.802	2722	2725	2728	rVB3	294	227	0.01%	0.002%
62	9.825	2728	2732	2737	rVB3	220	230	0.01%	0.002%
63	9.870	2742	2746	2749	rBV3	264	238	0.01%	0.002%
64	9.921	2759	2762	2765	rBV3	456	361	0.02%	0.003%
65	9.960	2769	2774	2778	rBV2	402	362	0.02%	0.003%
66	10.008	2785	2789	2793	rBV3	322	295	0.02%	0.002%
67	10.207	2838	2851	2873	rBV	517323	831364	51.48%	6.391%
68	10.371	2897	2902	2915	rVB5	1771	2975	0.18%	0.023%
69	10.535	2945	2953	2954	rBV2	384	386	0.02%	0.003%
70	10.593	2968	2971	2974	rVB2	302	234	0.01%	0.002%
71	10.667	2990	2994	2998	rVB2	388	339	0.02%	0.003%
72	10.728	3008	3013	3019	rVB2	472	534	0.03%	0.004%
73	10.821	3037	3042	3046	rBV3	435	402	0.02%	0.003%
74	10.847	3046	3050	3053	rBV3	479	386	0.02%	0.003%
75	10.969	3084	3088	3091	rBV3	350	263	0.02%	0.002%
76	11.172	3144	3151	3154	rBV5	999	977	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029441.D
 Acq On : 08 Dec 2022 01:01
 Operator : SY/MD
 Sample : N5919-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.239	3160	3172	3199	rBV	866044	1374274	85.10%	10.564%
78	11.400	3219	3222	3223	rBV3	424	213	0.01%	0.002%
79	11.545	3259	3267	3276	rBV4	5221	9442	0.58%	0.073%
80	11.612	3276	3288	3315	rVB	812357	1286036	79.63%	9.886%
81	11.886	3370	3373	3376	rBV	330	222	0.01%	0.002%
82	11.979	3399	3402	3404	rVB2	419	250	0.02%	0.002%
83	11.998	3404	3408	3411	rBV	327	287	0.02%	0.002%
84	12.037	3417	3420	3423	rBV	398	214	0.01%	0.002%
85	12.114	3439	3444	3445	rBV2	312	262	0.02%	0.002%
86	12.172	3460	3462	3465	rVB3	365	208	0.01%	0.002%
87	12.191	3465	3468	3471	rBV2	315	215	0.01%	0.002%
88	12.210	3471	3474	3477	rBV2	233	217	0.01%	0.002%
89	12.239	3481	3483	3490	rVB5	688	644	0.04%	0.005%
90	12.320	3506	3508	3511	rVB	419	216	0.01%	0.002%
91	12.342	3511	3515	3518	rBV4	539	415	0.03%	0.003%
92	12.387	3526	3529	3535	rVB4	455	345	0.02%	0.003%
93	12.416	3535	3538	3541	rVB3	377	249	0.02%	0.002%
94	12.709	3626	3629	3631	rBV	367	271	0.02%	0.002%
95	12.744	3637	3640	3643	rBV3	325	250	0.02%	0.002%
96	13.072	3739	3742	3746	rBV2	322	231	0.01%	0.002%
97	13.178	3771	3775	3777	rBV2	304	228	0.01%	0.002%
98	13.249	3793	3797	3805	rVB6	1153	1350	0.08%	0.010%
99	13.480	3862	3869	3870	rBV3	901	917	0.06%	0.007%
100	13.689	3932	3934	3941	rBV4	395	311	0.02%	0.002%




Sum of corrected areas: 13008501

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029441.D
Acq On : 08 Dec 2022 01:01
Operator : SY/MD
Sample : N5919-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

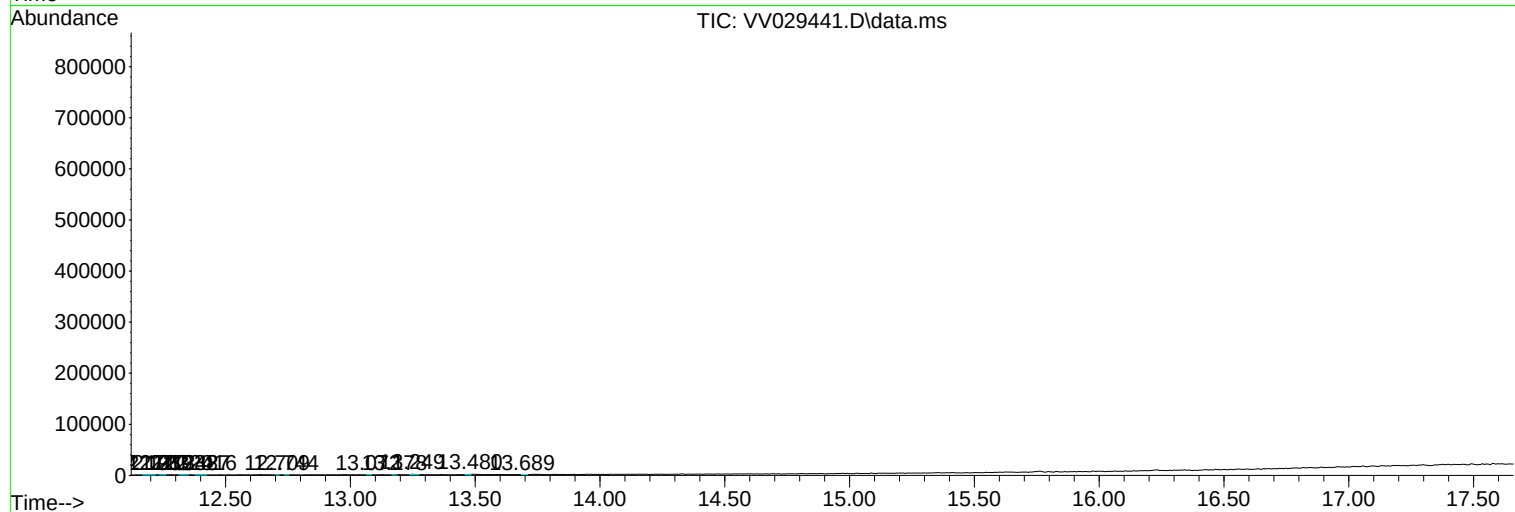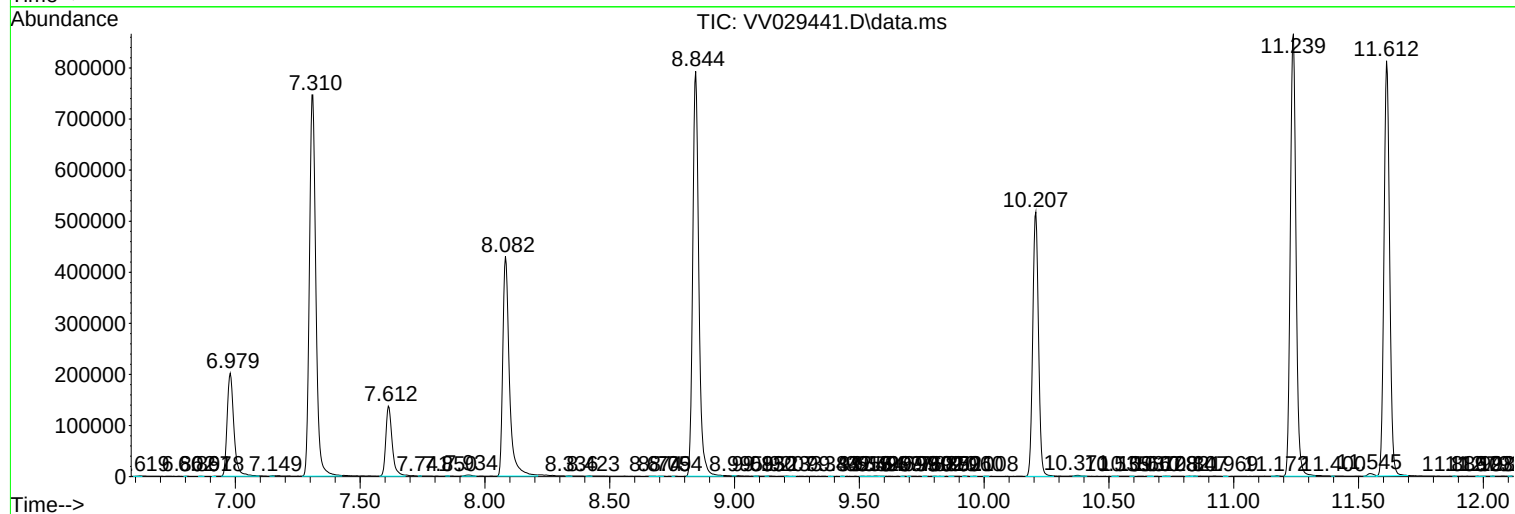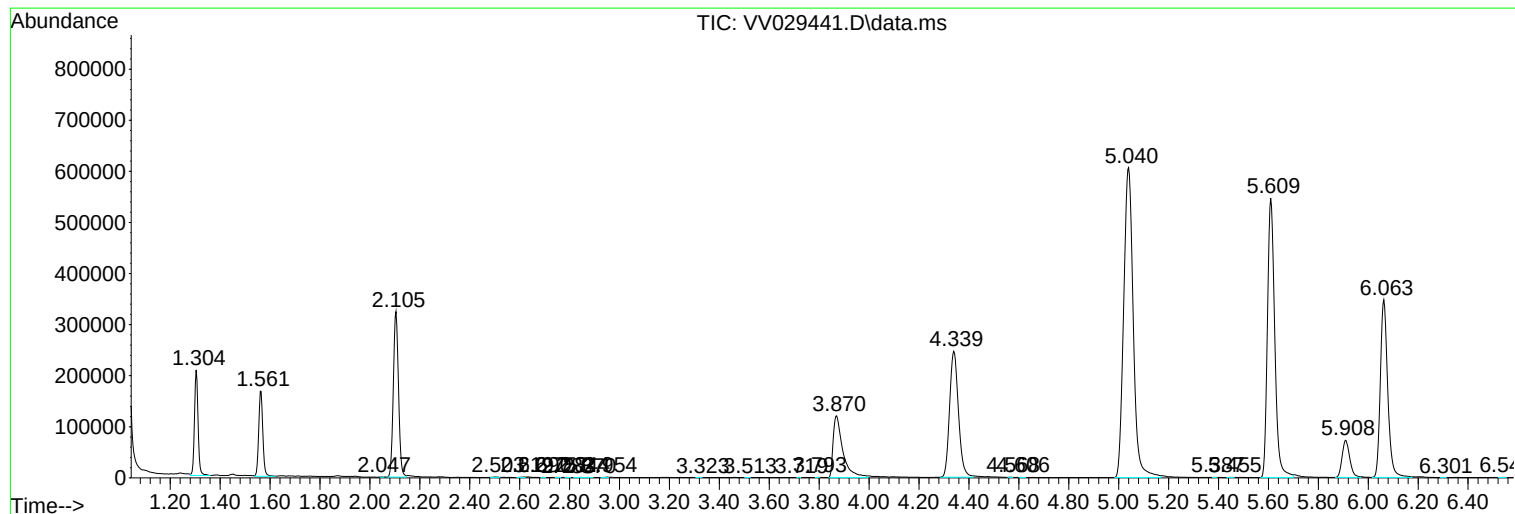

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029441.D
Acq On : 08 Dec 2022 01:01
Operator : SY/MD
Sample : N5919-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029441.D
Acq On : 08 Dec 2022 01:01
Operator : SY/MD
Sample : N5919-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------