

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029442.D
 Acq On : 08 Dec 2022 01:24
 Operator : SY/MD
 Sample : N5919-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029442.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	211717	205402	13.31%	1.648%
2	1.561	155	162	179	rVB	160857	183301	11.88%	1.471%
3	2.105	319	331	343	rBV	314270	450998	29.23%	3.618%
4	2.407	422	425	431	rVB3	219	180	0.01%	0.001%
5	2.481	444	448	449	rBV2	333	211	0.01%	0.002%
6	2.507	449	456	463	rVB6	1335	1957	0.13%	0.016%
7	2.619	483	491	500	rBV3	1409	2324	0.15%	0.019%
8	2.709	516	519	523	rBV2	295	212	0.01%	0.002%
9	2.928	584	587	590	rBV3	328	204	0.01%	0.002%
10	3.056	624	627	631	rVB2	229	185	0.01%	0.001%
11	3.082	631	635	639	rBV2	325	283	0.02%	0.002%
12	3.172	660	663	667	rVB2	238	196	0.01%	0.002%
13	3.298	698	702	705	rVV2	191	190	0.01%	0.002%
14	3.535	772	776	781	rVB	211	193	0.01%	0.002%
15	3.616	796	801	804	rBV	208	202	0.01%	0.002%
16	3.870	869	880	917	rBV	116869	314087	20.36%	2.520%
17	4.339	1008	1026	1063	rBV	238329	593626	38.47%	4.763%
18	4.597	1099	1106	1113	rBV5	797	1127	0.07%	0.009%
19	4.699	1136	1138	1142	rVB2	434	262	0.02%	0.002%
20	5.040	1225	1244	1297	rVV2	577396	1543017	100.00%	12.380%
21	5.352	1338	1341	1348	rBV3	286	348	0.02%	0.003%
22	5.555	1398	1404	1406	rBV2	193	246	0.02%	0.002%
23	5.609	1408	1421	1461	rBV	532737	1089905	70.63%	8.745%
24	5.908	1502	1514	1526	rVB8	5891	13578	0.88%	0.109%
25	5.986	1534	1538	1541	rVB2	261	186	0.01%	0.001%
26	6.063	1547	1562	1601	rBV	330664	688396	44.61%	5.523%
27	6.236	1614	1616	1619	rVB2	442	181	0.01%	0.001%
28	6.304	1635	1637	1640	rVB2	529	308	0.02%	0.002%
29	6.397	1664	1666	1669	rVB2	427	179	0.01%	0.001%
30	6.429	1672	1676	1679	rVB2	428	229	0.01%	0.002%
31	6.481	1685	1692	1695	rBV2	322	361	0.02%	0.003%
32	6.506	1698	1700	1705	rBV2	246	238	0.02%	0.002%
33	6.622	1729	1736	1739	rBV5	1426	1558	0.10%	0.013%
34	6.667	1748	1750	1756	rBV2	435	420	0.03%	0.003%
35	6.731	1769	1770	1774	rVB2	318	191	0.01%	0.002%
36	6.760	1774	1779	1782	rBV2	380	429	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120722\
 Data File : VW029442.D
 Acq On : 08 Dec 2022 01:24
 Operator : SY/MD
 Sample : N5919-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.776	1782	1784	1787	rVB2	357	191	0.01%	0.002%
38	6.799	1787	1791	1795	rBV2	298	253	0.02%	0.002%
39	6.838	1800	1803	1807	rBV2	404	357	0.02%	0.003%
40	6.873	1812	1814	1819	rVB4	420	277	0.02%	0.002%
41	6.908	1819	1825	1827	rBV2	243	295	0.02%	0.002%
42	6.979	1835	1847	1880	rBV	191100	351723	22.79%	2.822%
43	7.169	1893	1906	1910	rBV4	785	1775	0.12%	0.014%
44	7.214	1918	1920	1923	rVB3	532	264	0.02%	0.002%
45	7.230	1923	1925	1930	rBV	383	255	0.02%	0.002%
46	7.307	1936	1949	1989	rBV	731560	1292588	83.77%	10.371%
47	7.612	2034	2044	2071	rBV	129154	229539	14.88%	1.842%
48	7.937	2137	2145	2155	rVB3	1658	2833	0.18%	0.023%
49	8.082	2175	2190	2227	rBV	428903	775377	50.25%	6.221%
50	8.381	2279	2283	2286	rBV3	243	262	0.02%	0.002%
51	8.510	2319	2323	2325	rBV3	343	268	0.02%	0.002%
52	8.529	2326	2329	2332	rVB2	451	244	0.02%	0.002%
53	8.548	2333	2335	2340	rVB3	438	315	0.02%	0.003%
54	8.664	2365	2371	2372	rBV3	314	311	0.02%	0.002%
55	8.751	2392	2398	2401	rBV2	525	588	0.04%	0.005%
56	8.773	2402	2405	2407	rVV2	257	177	0.01%	0.001%
57	8.844	2412	2427	2456	rBV	770512	1296311	84.01%	10.401%
58	9.018	2478	2481	2485	rBV4	595	490	0.03%	0.004%
59	9.140	2517	2519	2525	rVB4	330	222	0.01%	0.002%
60	9.201	2534	2538	2542	rVB2	275	238	0.02%	0.002%
61	9.259	2552	2556	2560	rBV2	294	238	0.02%	0.002%
62	9.349	2578	2584	2586	rBV2	266	253	0.02%	0.002%
63	9.403	2597	2601	2605	rBV2	336	286	0.02%	0.002%
64	9.513	2631	2635	2640	rBV2	199	211	0.01%	0.002%
65	9.538	2640	2643	2648	rVB2	517	434	0.03%	0.003%
66	9.574	2648	2654	2661	rBV3	486	777	0.05%	0.006%
67	9.603	2661	2663	2669	rVB3	292	246	0.02%	0.002%
68	9.690	2687	2690	2694	rBV2	228	183	0.01%	0.001%
69	9.828	2730	2733	2737	rVB2	360	306	0.02%	0.002%
70	9.927	2761	2764	2766	rVB3	316	196	0.01%	0.002%
71	9.998	2782	2786	2787	rBV2	292	177	0.01%	0.001%
72	10.069	2805	2808	2811	rVB3	346	183	0.01%	0.001%
73	10.207	2837	2851	2872	rBV	505600	800898	51.90%	6.426%
74	10.378	2897	2904	2910	rVB5	1646	2228	0.14%	0.018%
75	10.445	2923	2925	2931	rVB2	405	345	0.02%	0.003%
76	10.487	2934	2938	2940	rBV	325	295	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029442.D
 Acq On : 08 Dec 2022 01:24
 Operator : SY/MD
 Sample : N5919-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.847	3047	3050	3052	rVB3	420	189	0.01%	0.002%
78	10.908	3065	3069	3071	rVV3	449	355	0.02%	0.003%
79	10.927	3071	3075	3080	rVB3	361	300	0.02%	0.002%
80	10.989	3091	3094	3096	rBV2	264	182	0.01%	0.001%
81	11.239	3160	3172	3194	rBV	856629	1343004	87.04%	10.775%
82	11.426	3228	3230	3233	rBV3	316	187	0.01%	0.002%
83	11.548	3259	3268	3276	rBV3	7639	12719	0.82%	0.102%
84	11.612	3276	3288	3306	rVV	787648	1242331	80.51%	9.968%
85	11.808	3346	3349	3351	rBV	414	323	0.02%	0.003%
86	11.992	3401	3406	3409	rBV2	428	485	0.03%	0.004%
87	12.239	3479	3483	3489	rVB3	502	456	0.03%	0.004%
88	12.320	3505	3508	3511	rBV3	401	274	0.02%	0.002%
89	12.339	3511	3514	3519	rVB3	385	343	0.02%	0.003%
90	12.609	3596	3598	3601	rBV3	305	205	0.01%	0.002%
91	12.915	3691	3693	3697	rBV4	405	287	0.02%	0.002%
92	13.078	3742	3744	3747	rBV2	382	252	0.02%	0.002%
93	13.149	3761	3766	3771	rBV3	591	770	0.05%	0.006%
94	13.194	3777	3780	3781	rBV	380	241	0.02%	0.002%
95	13.246	3791	3796	3797	rBV2	704	602	0.04%	0.005%
96	13.329	3819	3822	3827	rBV2	618	640	0.04%	0.005%
97	13.406	3844	3846	3851	rVB2	776	519	0.03%	0.004%
98	13.435	3852	3855	3856	rBV3	636	278	0.02%	0.002%
99	13.799	3965	3968	3974	rBV4	1021	905	0.06%	0.007%
100	13.873	3987	3991	3992	rBV2	664	508	0.03%	0.004%




Sum of corrected areas: 12463674

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029442.D
Acq On : 08 Dec 2022 01:24
Operator : SY/MD
Sample : N5919-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

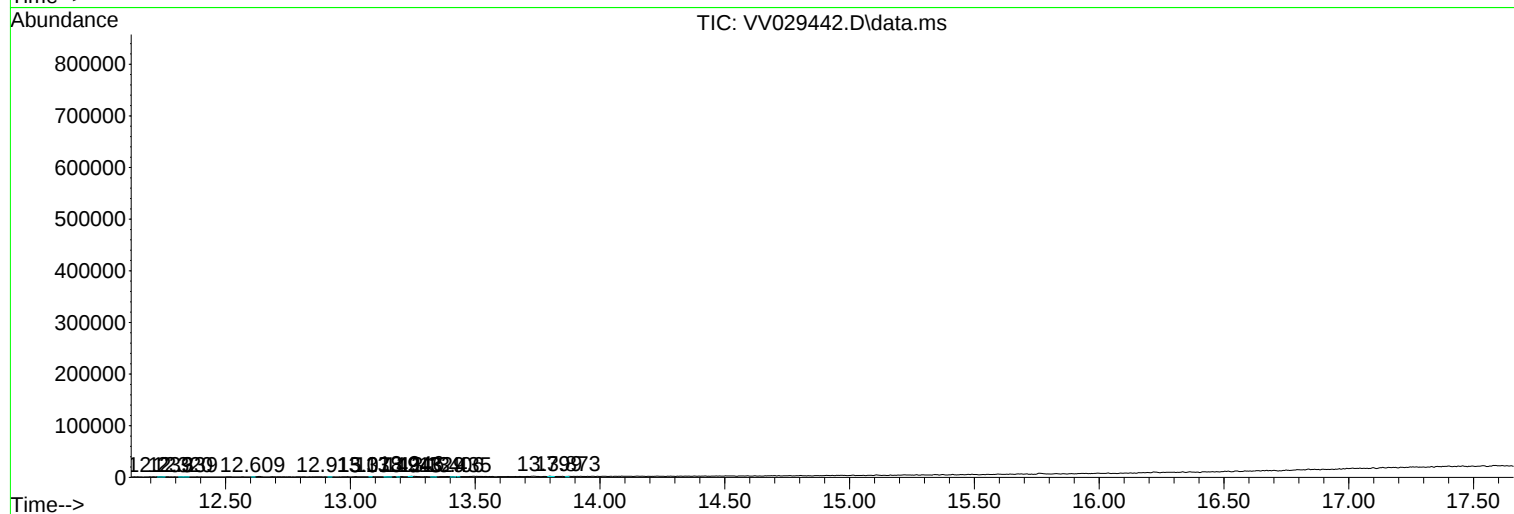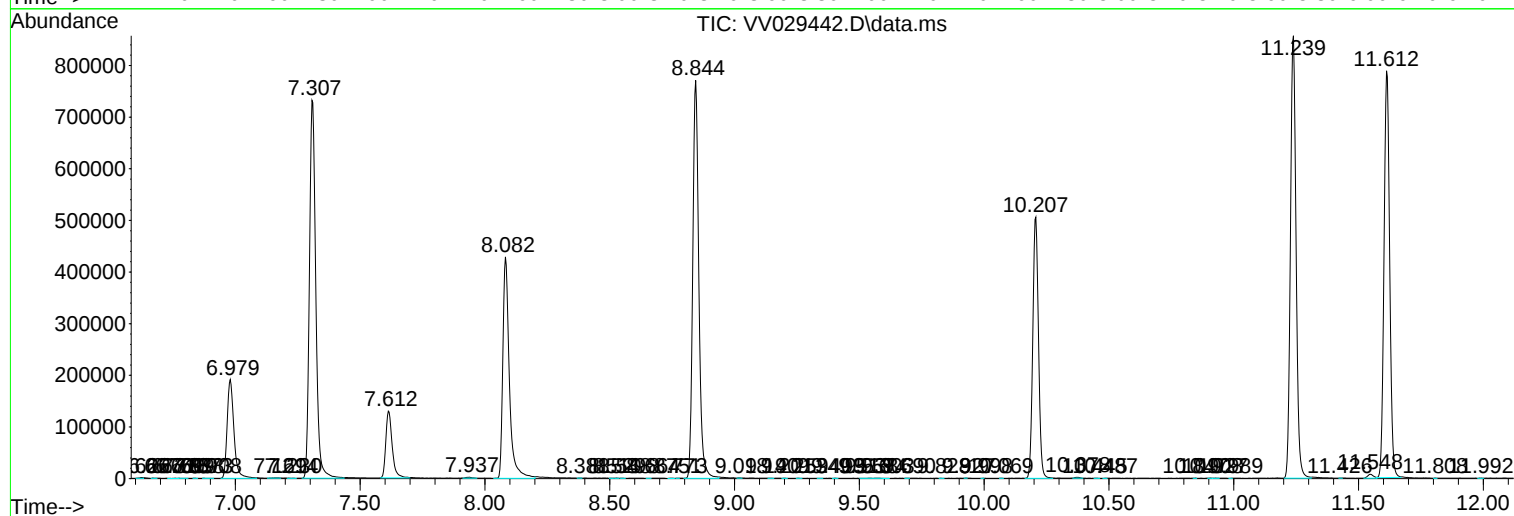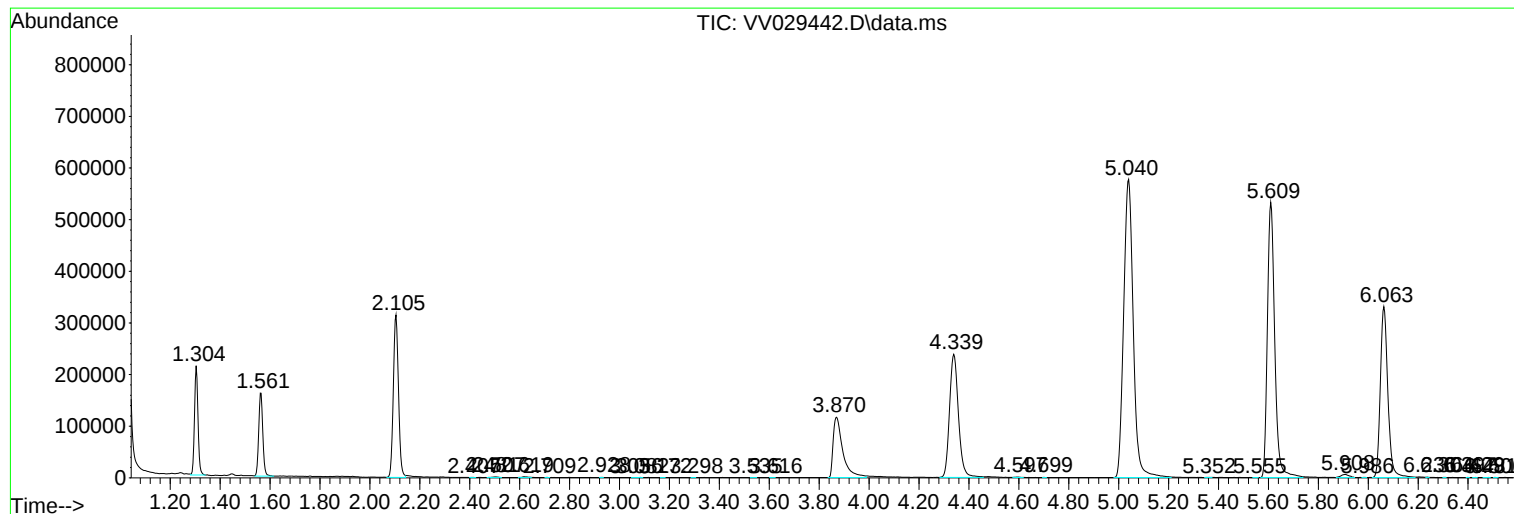

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029442.D
Acq On : 08 Dec 2022 01:24
Operator : SY/MD
Sample : N5919-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029442.D
Acq On : 08 Dec 2022 01:24
Operator : SY/MD
Sample : N5919-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------