

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029443.D
 Acq On : 08 Dec 2022 01:48
 Operator : SY/MD
 Sample : N5919-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rVB	201416	198325	12.65%	1.413%
2	1.561	155	162	176	rVB	164580	184510	11.77%	1.315%
3	2.105	320	331	345	rBV2	335721	510980	32.59%	3.641%
4	2.410	424	426	431	rVB2	316	212	0.01%	0.002%
5	2.432	431	433	436	rBV2	412	285	0.02%	0.002%
6	2.474	443	446	449	rBV2	476	357	0.02%	0.003%
7	2.506	449	456	461	rBV3	1574	2084	0.13%	0.015%
8	2.532	461	464	466	rVV	267	203	0.01%	0.001%
9	2.805	542	549	552	rBV2	327	339	0.02%	0.002%
10	2.831	552	557	560	rBV3	291	247	0.02%	0.002%
11	2.876	567	571	574	rBV3	218	208	0.01%	0.001%
12	3.066	625	630	637	rVB3	294	332	0.02%	0.002%
13	3.121	642	647	649	rBV2	337	276	0.02%	0.002%
14	3.178	658	665	666	rBV2	1099	1035	0.07%	0.007%
15	3.349	712	718	722	rBV3	316	309	0.02%	0.002%
16	3.432	740	744	748	rBV3	224	232	0.01%	0.002%
17	3.458	748	752	755	rVV	281	203	0.01%	0.001%
18	3.596	789	795	800	rVB2	420	397	0.03%	0.003%
19	3.789	851	855	859	rBV2	230	259	0.02%	0.002%
20	3.873	870	881	918	rBV3	123712	438697	27.98%	3.126%
21	4.265	1000	1003	1008	rVB3	327	223	0.01%	0.002%
22	4.339	1008	1026	1055	rBV	241356	599802	38.26%	4.273%
23	4.600	1092	1107	1124	rVB2	18183	43142	2.75%	0.307%
24	4.780	1159	1163	1168	rBV2	248	236	0.02%	0.002%
25	4.937	1207	1212	1216	rBV2	400	489	0.03%	0.003%
26	5.040	1220	1244	1278	rBV2	595251	1567799	100.00%	11.170%
27	5.243	1303	1307	1312	rVB4	569	549	0.04%	0.004%
28	5.397	1350	1355	1359	rBV3	463	472	0.03%	0.003%
29	5.481	1379	1381	1385	rVV3	303	265	0.02%	0.002%
30	5.609	1408	1421	1457	rBV	546139	1108015	70.67%	7.894%
31	5.805	1480	1482	1485	rVB2	520	260	0.02%	0.002%
32	5.905	1499	1513	1546	rBV	605331	1207088	76.99%	8.600%
33	6.063	1549	1562	1590	rVV	335007	684161	43.64%	4.874%
34	6.191	1600	1602	1603	rBV2	457	211	0.01%	0.002%
35	6.352	1648	1652	1655	rBV	412	386	0.02%	0.003%
36	6.400	1663	1667	1670	rBV2	424	355	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029443.D
 Acq On : 08 Dec 2022 01:48
 Operator : SY/MD
 Sample : N5919-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.452	1680	1683	1688	rVB2	321	241	0.02%	0.002%
38	6.593	1725	1727	1729	rBV2	353	204	0.01%	0.001%
39	6.616	1730	1734	1736	rBV3	807	706	0.05%	0.005%
40	6.725	1763	1768	1769	rBV	342	256	0.02%	0.002%
41	6.754	1775	1777	1781	rVB2	387	240	0.02%	0.002%
42	6.873	1809	1814	1821	rVB2	275	373	0.02%	0.003%
43	6.908	1821	1825	1826	rBV2	351	220	0.01%	0.002%
44	6.979	1834	1847	1877	rBV	192849	358128	22.84%	2.552%
45	7.146	1895	1899	1902	rBV3	700	629	0.04%	0.004%
46	7.246	1926	1930	1931	rBV	446	320	0.02%	0.002%
47	7.307	1937	1949	1983	rBV	729907	1298219	82.81%	9.249%
48	7.612	2034	2044	2078	rBV	131302	234902	14.98%	1.674%
49	7.937	2134	2145	2154	rBV3	2194	3536	0.23%	0.025%
50	8.082	2180	2190	2223	rBV	433587	779993	49.75%	5.557%
51	8.455	2303	2306	2309	rBV3	406	240	0.02%	0.002%
52	8.535	2327	2331	2334	rVV4	417	236	0.02%	0.002%
53	8.632	2359	2361	2366	rVB	362	263	0.02%	0.002%
54	8.712	2384	2386	2391	rVB	520	416	0.03%	0.003%
55	8.744	2391	2396	2401	rBV2	371	408	0.03%	0.003%
56	8.792	2406	2411	2412	rBV3	430	304	0.02%	0.002%
57	8.844	2415	2427	2460	rBV	793198	1316508	83.97%	9.380%
58	9.098	2502	2506	2510	rBV2	541	496	0.03%	0.004%
59	9.133	2515	2517	2518	rVV	422	200	0.01%	0.001%
60	9.188	2530	2534	2536	rVB3	359	266	0.02%	0.002%
61	9.214	2540	2542	2547	rBV2	525	370	0.02%	0.003%
62	9.493	2622	2629	2630	rBV2	489	481	0.03%	0.003%
63	9.641	2672	2675	2678	rBV2	309	232	0.01%	0.002%
64	9.664	2680	2682	2687	rVB3	395	253	0.02%	0.002%
65	9.706	2688	2695	2699	rBV3	389	450	0.03%	0.003%
66	9.741	2703	2706	2708	rBV2	310	237	0.02%	0.002%
67	9.805	2721	2726	2728	rVB2	315	275	0.02%	0.002%
68	9.847	2733	2739	2743	rBV3	371	449	0.03%	0.003%
69	9.911	2754	2759	2760	rBV2	280	217	0.01%	0.002%
70	9.963	2771	2775	2779	rVV2	297	315	0.02%	0.002%
71	10.017	2784	2792	2794	rBV	368	477	0.03%	0.003%
72	10.117	2818	2823	2826	rVB2	199	230	0.01%	0.002%
73	10.207	2838	2851	2871	rBV	518409	812777	51.84%	5.791%
74	10.371	2896	2902	2907	rBV5	1529	1817	0.12%	0.013%
75	10.525	2947	2950	2953	rVB2	381	286	0.02%	0.002%
76	10.606	2972	2975	2980	rBV4	278	276	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029443.D
 Acq On : 08 Dec 2022 01:48
 Operator : SY/MD
 Sample : N5919-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.689	2996	3001	3003	rBV2	246	209	0.01%	0.001%
78	10.744	3014	3018	3022	rVB4	408	268	0.02%	0.002%
79	10.776	3024	3028	3032	rBV	512	498	0.03%	0.004%
80	10.905	3065	3068	3072	rBV3	531	383	0.02%	0.003%
81	11.078	3119	3122	3126	rVV3	328	290	0.02%	0.002%
82	11.133	3135	3139	3142	rBV3	290	271	0.02%	0.002%
83	11.175	3147	3152	3158	rVB4	820	1050	0.07%	0.007%
84	11.239	3159	3172	3194	rBV	897594	1373046	87.58%	9.782%
85	11.384	3215	3217	3222	rVB4	645	559	0.04%	0.004%
86	11.545	3259	3267	3276	rBV3	7514	13659	0.87%	0.097%
87	11.612	3276	3288	3309	rVV	825044	1272194	81.15%	9.064%
88	11.709	3316	3318	3322	rBV2	423	290	0.02%	0.002%
89	11.931	3384	3387	3390	rVB2	379	245	0.02%	0.002%
90	11.998	3404	3408	3411	rBV2	406	289	0.02%	0.002%
91	12.024	3414	3416	3419	rVB2	376	225	0.01%	0.002%
92	12.191	3463	3468	3470	rBV3	449	355	0.02%	0.003%
93	12.223	3474	3478	3479	rBV	394	228	0.01%	0.002%
94	12.239	3481	3483	3491	rVB5	592	618	0.04%	0.004%
95	12.300	3500	3502	3505	rVB2	483	260	0.02%	0.002%
96	12.853	3670	3674	3677	rBV2	239	225	0.01%	0.002%
97	13.008	3720	3722	3726	rBV2	333	323	0.02%	0.002%
98	13.085	3744	3746	3749	rBV	563	397	0.03%	0.003%
99	13.410	3845	3847	3851	rVV4	490	301	0.02%	0.002%
100	13.442	3854	3857	3859	rBV3	453	290	0.02%	0.002%




Sum of corrected areas: 14035862

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029443.D
Acq On : 08 Dec 2022 01:48
Operator : SY/MD
Sample : N5919-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

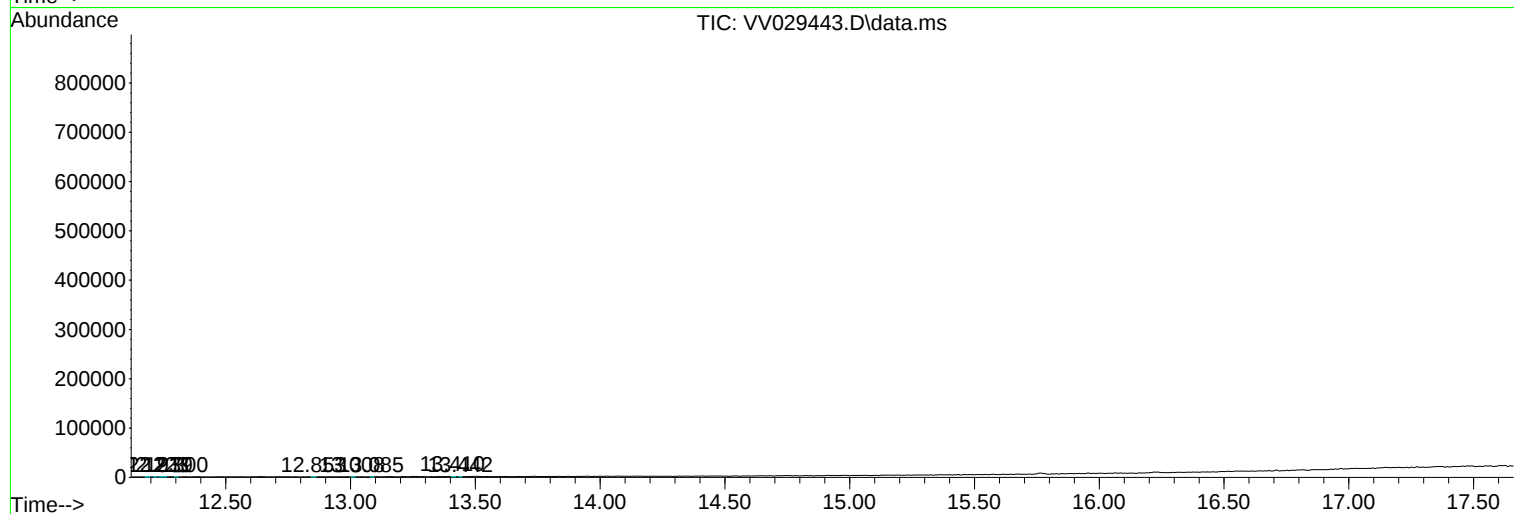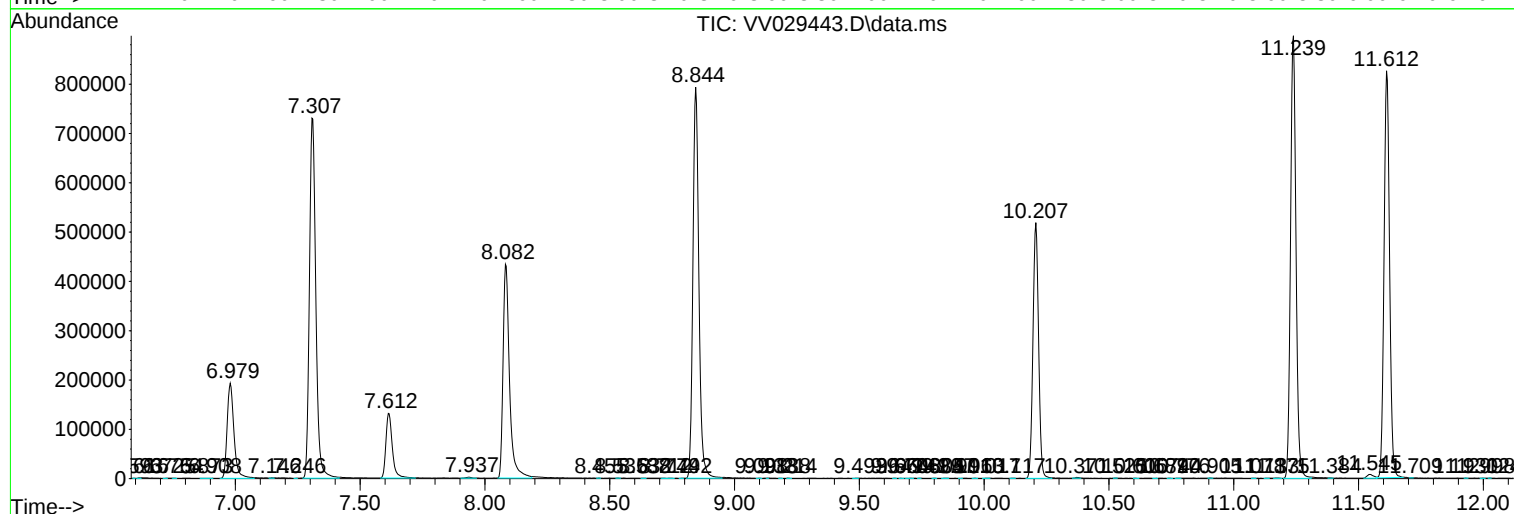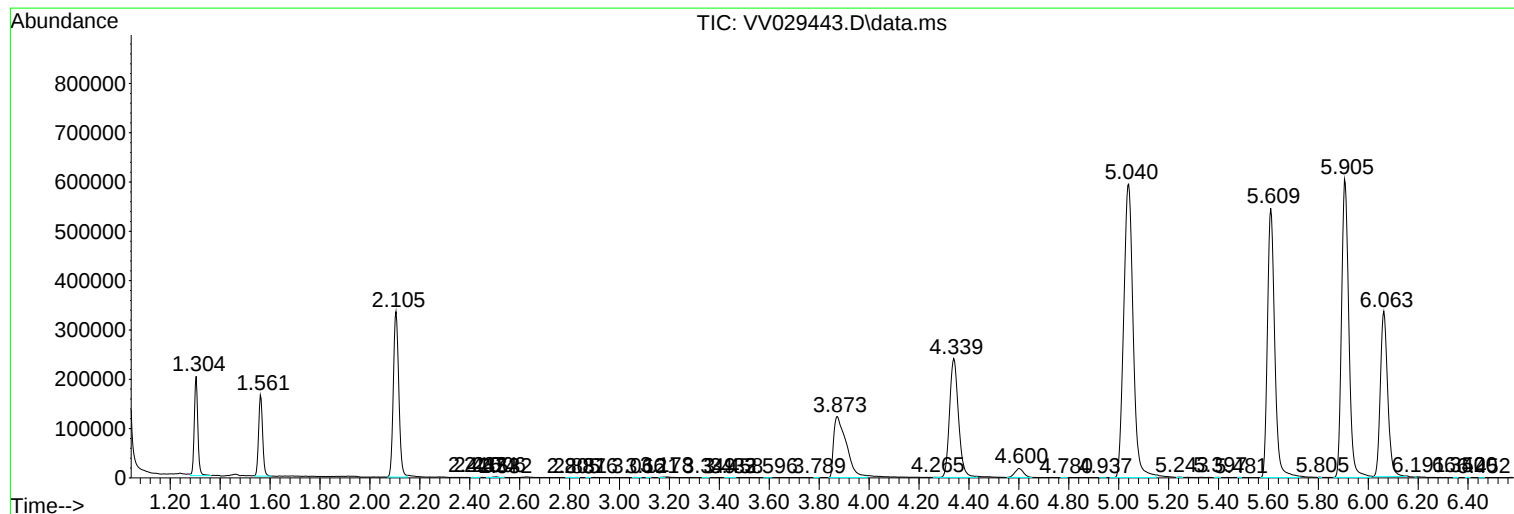

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029443.D
Acq On : 08 Dec 2022 01:48
Operator : SY/MD
Sample : N5919-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029443.D
Acq On : 08 Dec 2022 01:48
Operator : SY/MD
Sample : N5919-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc