

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029444.D
 Acq On : 08 Dec 2022 02:12
 Operator : SY/MD
 Sample : N5919-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029444.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	194654	194891	12.47%	1.538%
2	1.561	155	162	180	rVB	162383	184373	11.80%	1.455%
3	2.105	321	331	343	rBV	315235	448458	28.70%	3.539%
4	2.282	377	386	404	rVB2	13067	28479	1.82%	0.225%
5	2.507	450	456	461	rBV3	970	1040	0.07%	0.008%
6	2.613	487	489	490	rBV	266	138	0.01%	0.001%
7	2.728	523	525	528	rVB2	264	123	0.01%	0.001%
8	2.748	529	531	532	rBV	243	104	0.01%	0.001%
9	2.822	551	554	557	rBV2	197	102	0.01%	0.001%
10	2.883	568	573	578	rBV2	288	347	0.02%	0.003%
11	2.921	582	585	590	rVB2	463	333	0.02%	0.003%
12	2.957	590	596	599	rBV3	360	332	0.02%	0.003%
13	3.092	635	638	641	rBV3	395	250	0.02%	0.002%
14	3.127	645	649	652	rBV	276	191	0.01%	0.002%
15	3.192	667	669	671	rVB	304	130	0.01%	0.001%
16	3.227	676	680	683	rBV	115	110	0.01%	0.001%
17	3.301	700	703	706	rBV2	274	145	0.01%	0.001%
18	3.365	721	723	726	rVV2	151	88	0.01%	0.001%
19	3.407	733	736	739	rBV3	164	125	0.01%	0.001%
20	3.449	746	749	753	rVB2	275	195	0.01%	0.002%
21	3.471	753	756	758	rBV2	375	277	0.02%	0.002%
22	3.519	769	771	774	rBV2	135	103	0.01%	0.001%
23	3.555	779	782	785	rVB	348	202	0.01%	0.002%
24	3.574	785	788	790	rVB	238	105	0.01%	0.001%
25	3.593	790	794	798	rBV3	369	366	0.02%	0.003%
26	3.632	803	806	812	rBV2	263	229	0.01%	0.002%
27	3.661	812	815	818	rBV2	231	127	0.01%	0.001%
28	3.725	833	835	838	rVB2	330	110	0.01%	0.001%
29	3.745	838	841	843	rBV2	203	142	0.01%	0.001%
30	3.812	860	862	866	rBV	130	79	0.01%	0.001%
31	3.870	871	880	919	rBV	117666	331322	21.20%	2.615%
32	4.339	1010	1026	1056	rBV	239924	592941	37.94%	4.680%
33	4.600	1105	1107	1109	rBV3	306	182	0.01%	0.001%
34	4.638	1117	1119	1120	rBV	156	86	0.01%	0.001%
35	4.709	1139	1141	1143	rVB2	476	211	0.01%	0.002%
36	4.732	1144	1148	1152	rBV2	402	406	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029444.D
 Acq On : 08 Dec 2022 02:12
 Operator : SY/MD
 Sample : N5919-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	4.815	1169	1174	1177	rVB2	419	439	0.03%	0.003%
38	4.841	1177	1182	1186	rBV3	362	327	0.02%	0.003%
39	4.876	1186	1193	1197	rVB2	252	210	0.01%	0.002%
40	4.921	1202	1207	1208	rBV	252	189	0.01%	0.001%
41	4.950	1213	1216	1219	rBV2	262	198	0.01%	0.002%
42	5.040	1226	1244	1299	rBV2	589288	1562804	100.00%	12.334%
43	5.326	1329	1333	1337	rBV2	315	283	0.02%	0.002%
44	5.526	1391	1395	1401	rVB	323	349	0.02%	0.003%
45	5.609	1407	1421	1450	rBV	556564	1122241	71.81%	8.857%
46	5.912	1502	1515	1534	rBV5	26266	56856	3.64%	0.449%
47	5.998	1540	1542	1548	rVB2	351	241	0.02%	0.002%
48	6.063	1548	1562	1598	rBV	341052	698009	44.66%	5.509%
49	6.233	1613	1615	1622	rVB5	735	644	0.04%	0.005%
50	6.281	1627	1630	1632	rBV	359	224	0.01%	0.002%
51	6.310	1635	1639	1643	rBV3	223	271	0.02%	0.002%
52	6.371	1655	1658	1660	rVV3	200	127	0.01%	0.001%
53	6.388	1660	1663	1665	rVV	317	257	0.02%	0.002%
54	6.429	1669	1676	1680	rBV2	298	340	0.02%	0.003%
55	6.487	1691	1694	1695	rBV2	177	73	0.00%	0.001%
56	6.497	1695	1697	1698	rBV	174	75	0.00%	0.001%
57	6.564	1715	1718	1719	rBV2	244	131	0.01%	0.001%
58	6.625	1730	1737	1745	rBV3	1135	1970	0.13%	0.016%
59	6.725	1765	1768	1770	rBV	267	178	0.01%	0.001%
60	6.751	1774	1776	1778	rVV	289	133	0.01%	0.001%
61	6.789	1785	1788	1790	rBV	203	159	0.01%	0.001%
62	6.851	1804	1807	1811	rBV2	335	233	0.01%	0.002%
63	6.873	1811	1814	1816	rBV3	292	179	0.01%	0.001%
64	6.921	1827	1829	1833	rVB2	274	150	0.01%	0.001%
65	6.979	1833	1847	1878	rBV	193748	357470	22.87%	2.821%
66	7.143	1895	1898	1899	rBV	613	316	0.02%	0.002%
67	7.236	1926	1927	1928	rBV	312	91	0.01%	0.001%
68	7.307	1936	1949	1984	rBV	726719	1297465	83.02%	10.240%
69	7.613	2034	2044	2078	rBV	130447	232893	14.90%	1.838%
70	8.082	2180	2190	2231	rBV	431324	790206	50.56%	6.236%
71	8.667	2370	2372	2375	rBV2	253	112	0.01%	0.001%
72	8.715	2384	2387	2390	rBV2	299	200	0.01%	0.002%
73	8.776	2401	2406	2408	rBV3	438	395	0.03%	0.003%
74	8.844	2415	2427	2465	rBV	798891	1326579	84.88%	10.470%
75	9.233	2544	2548	2549	rBV2	388	263	0.02%	0.002%
76	9.297	2565	2568	2570	rBV	218	181	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029444.D
 Acq On : 08 Dec 2022 02:12
 Operator : SY/MD
 Sample : N5919-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.371	2587	2591	2592	rBV	182	151	0.01%	0.001%
78	9.397	2596	2599	2603	rVV3	267	226	0.01%	0.002%
79	9.455	2614	2617	2618	rBV	252	138	0.01%	0.001%
80	9.516	2631	2636	2638	rBV2	104	100	0.01%	0.001%
81	9.529	2638	2640	2642	rBV	156	103	0.01%	0.001%
82	9.629	2668	2671	2675	rVB	310	241	0.02%	0.002%
83	9.731	2701	2703	2708	rVB	221	130	0.01%	0.001%
84	9.757	2708	2711	2713	rBV3	190	113	0.01%	0.001%
85	9.773	2713	2716	2718	rBV	300	243	0.02%	0.002%
86	9.857	2739	2742	2743	rBV2	349	190	0.01%	0.001%
87	9.889	2750	2752	2753	rBV2	277	129	0.01%	0.001%
88	9.957	2770	2773	2778	rVB2	438	287	0.02%	0.002%
89	10.063	2804	2806	2808	rBV	315	171	0.01%	0.001%
90	10.207	2838	2851	2875	rBV	511102	800960	51.25%	6.321%
91	10.522	2947	2949	2955	rVB2	479	338	0.02%	0.003%
92	10.757	3019	3022	3023	rBV	364	176	0.01%	0.001%
93	10.847	3047	3050	3053	rBV2	589	369	0.02%	0.003%
94	10.876	3057	3059	3060	rBV2	225	108	0.01%	0.001%
95	10.902	3065	3067	3068	rBV	180	95	0.01%	0.001%
96	10.992	3090	3095	3096	rBV2	339	299	0.02%	0.002%
97	11.175	3148	3152	3158	rBV4	980	1134	0.07%	0.009%
98	11.239	3159	3172	3198	rBV	880822	1375582	88.02%	10.856%
99	11.612	3276	3288	3312	rBV	783594	1248618	79.90%	9.854%
100	12.024	3412	3416	3420	rBV3	533	477	0.03%	0.004%




Sum of corrected areas: 12670681

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029444.D
Acq On : 08 Dec 2022 02:12
Operator : SY/MD
Sample : N5919-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

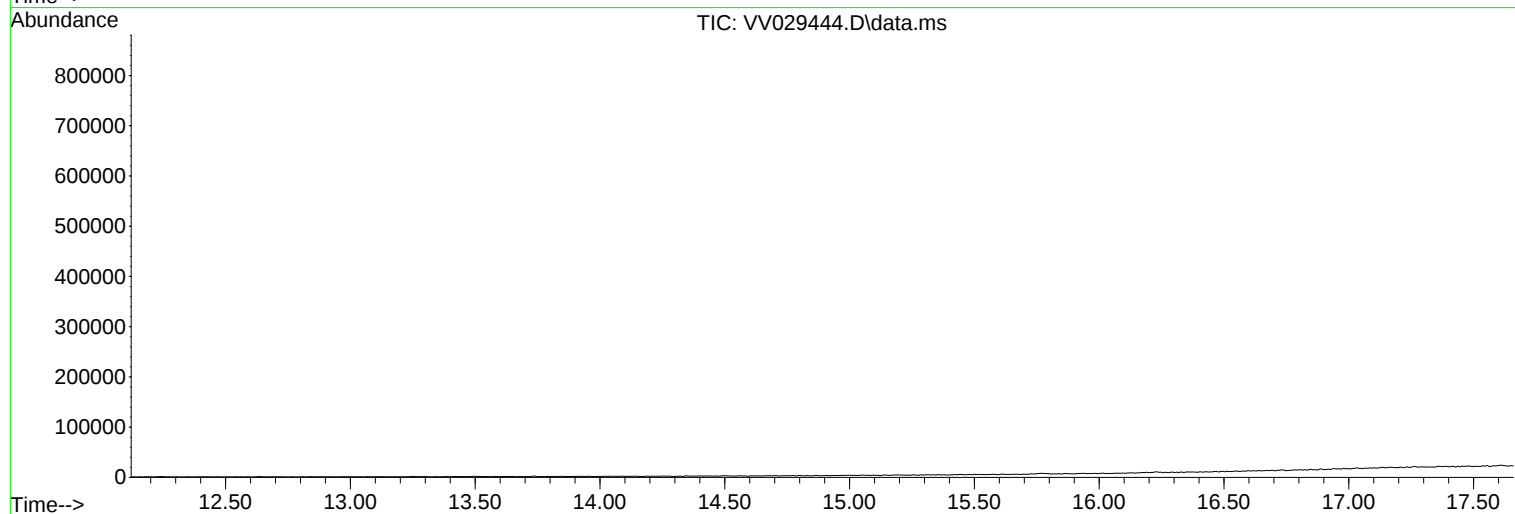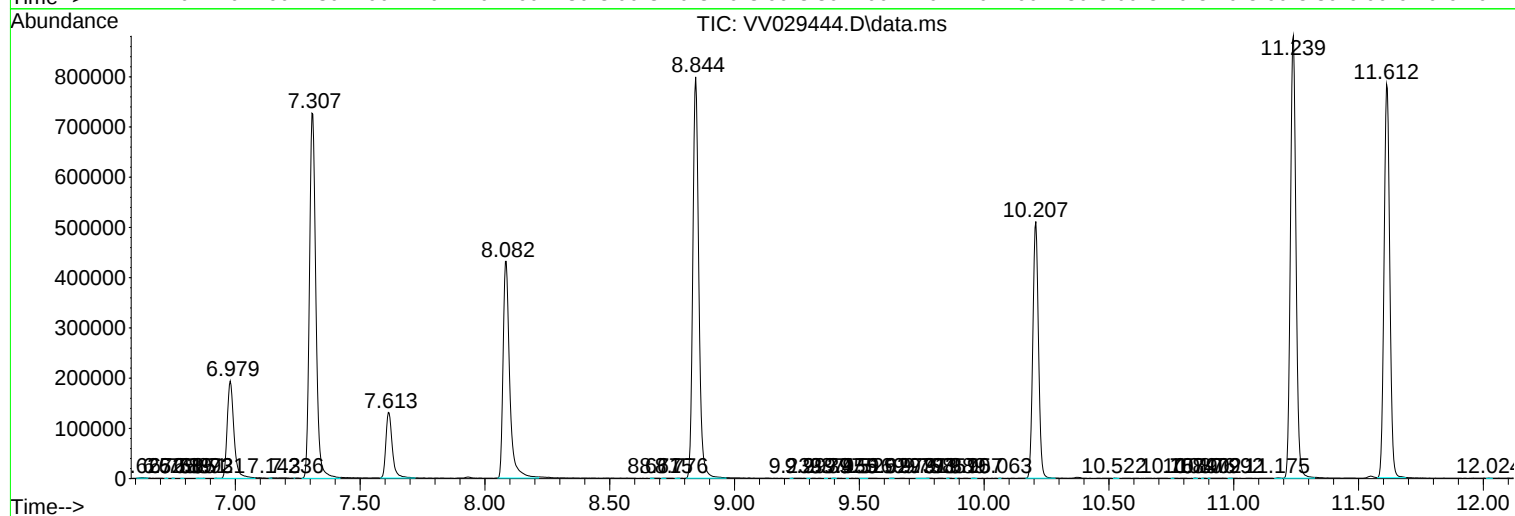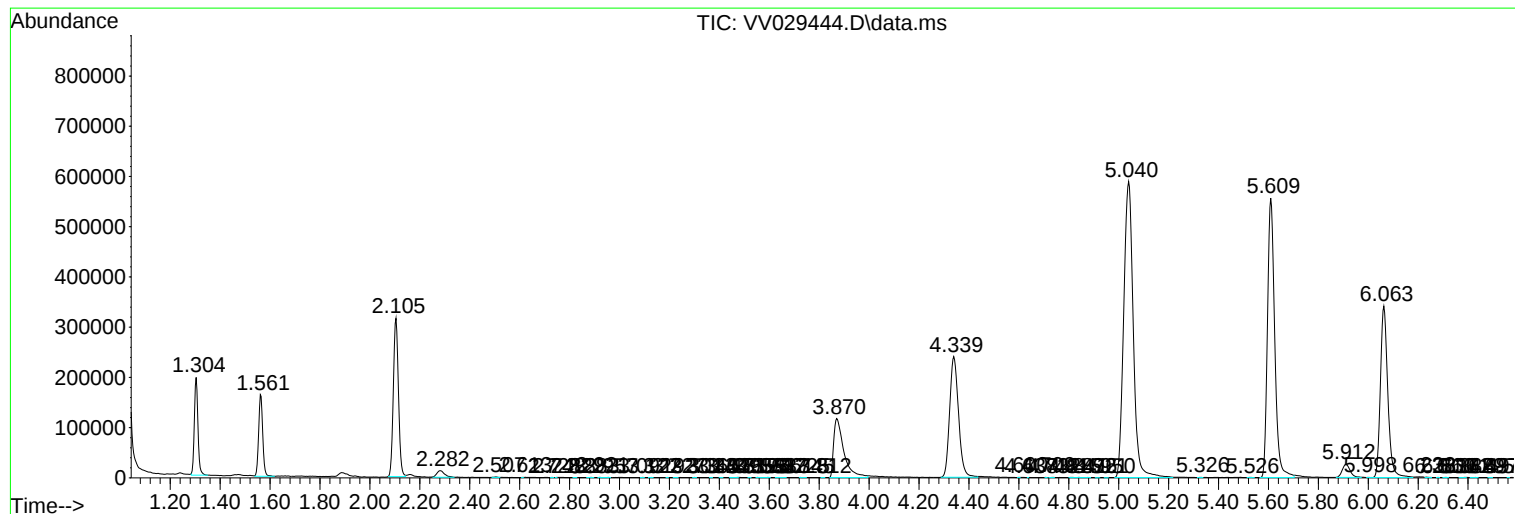

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029444.D
Acq On : 08 Dec 2022 02:12
Operator : SY/MD
Sample : N5919-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029444.D
Acq On : 08 Dec 2022 02:12
Operator : SY/MD
Sample : N5919-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc