

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029446.D
 Acq On : 08 Dec 2022 02:59
 Operator : SY/MD
 Sample : N5919-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	212405	210969	12.85%	1.615%
2	1.565	155	163	179	rVB	170605	194435	11.84%	1.489%
3	1.966	286	288	292	rBV2	461	278	0.02%	0.002%
4	2.105	320	331	343	rBV	336113	484262	29.49%	3.708%
5	2.468	441	444	447	rVB	304	193	0.01%	0.001%
6	2.507	447	456	462	rVB4	851	1563	0.10%	0.012%
7	2.539	463	466	470	rVB3	267	194	0.01%	0.001%
8	2.622	485	492	494	rBV	619	584	0.04%	0.004%
9	2.796	541	546	549	rBV2	360	259	0.02%	0.002%
10	2.838	554	559	565	rBV4	386	345	0.02%	0.003%
11	2.941	585	591	592	rBV	322	206	0.01%	0.002%
12	3.169	659	662	670	rVV3	282	337	0.02%	0.003%
13	3.304	702	704	710	rVB3	306	264	0.02%	0.002%
14	3.446	745	748	752	rVB	344	251	0.02%	0.002%
15	3.468	752	755	761	rBV3	228	213	0.01%	0.002%
16	3.632	803	806	812	rBV3	205	276	0.02%	0.002%
17	3.687	820	823	828	rVB2	324	194	0.01%	0.001%
18	3.809	855	861	865	rBV	239	295	0.02%	0.002%
19	3.870	869	880	908	rBV	129581	340773	20.76%	2.609%
20	4.339	1009	1026	1051	rBV	256671	636691	38.78%	4.875%
21	4.667	1122	1128	1131	rVV4	614	565	0.03%	0.004%
22	4.809	1168	1172	1176	rVB	248	191	0.01%	0.001%
23	4.931	1204	1210	1217	rBV3	389	492	0.03%	0.004%
24	5.040	1225	1244	1270	rBV2	630190	1641875	100.00%	12.570%
25	5.609	1406	1421	1465	rBV	541782	1105515	67.33%	8.464%
26	5.902	1502	1512	1525	rBV7	5398	10945	0.67%	0.084%
27	6.063	1548	1562	1594	rBV	354954	742892	45.25%	5.688%
28	6.320	1638	1642	1646	rBV3	303	277	0.02%	0.002%
29	6.339	1646	1648	1653	rVB2	260	190	0.01%	0.001%
30	6.365	1653	1656	1660	rBV2	301	239	0.01%	0.002%
31	6.558	1712	1716	1718	rBV2	236	197	0.01%	0.002%
32	6.622	1728	1736	1738	rBV4	1346	1422	0.09%	0.011%
33	6.732	1767	1770	1775	rVB2	362	295	0.02%	0.002%
34	6.764	1775	1780	1782	rBV3	343	263	0.02%	0.002%
35	6.802	1791	1792	1797	rVB3	280	194	0.01%	0.001%
36	6.899	1819	1822	1827	rBV2	375	307	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120722\
 Data File : VW029446.D
 Acq On : 08 Dec 2022 02:59
 Operator : SY/MD
 Sample : N5919-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.937	1829	1834	1835	rBV2	414	309	0.02%	0.002%
38	6.979	1835	1847	1881	rBV	202703	376515	22.93%	2.883%
39	7.146	1896	1899	1900	rBV2	700	387	0.02%	0.003%
40	7.307	1936	1949	1986	rBV	787266	1382253	84.19%	10.583%
41	7.613	2034	2044	2072	rBV	138714	244582	14.90%	1.873%
42	7.844	2113	2116	2118	rBV5	402	227	0.01%	0.002%
43	7.931	2139	2143	2146	rBV2	1269	1201	0.07%	0.009%
44	7.989	2157	2161	2165	rVB3	459	334	0.02%	0.003%
45	8.082	2178	2190	2225	rBV	456214	832441	50.70%	6.373%
46	8.529	2326	2329	2332	rBV3	325	204	0.01%	0.002%
47	8.561	2337	2339	2344	rBV3	229	204	0.01%	0.002%
48	8.635	2360	2362	2367	rVB3	331	270	0.02%	0.002%
49	8.674	2371	2374	2377	rVB2	436	214	0.01%	0.002%
50	8.719	2385	2388	2392	rVB2	331	240	0.01%	0.002%
51	8.741	2392	2395	2396	rBV2	380	224	0.01%	0.002%
52	8.780	2402	2407	2409	rBV3	262	242	0.01%	0.002%
53	8.844	2413	2427	2459	rBV	788789	1302567	79.33%	9.972%
54	9.088	2495	2503	2507	rBV4	598	660	0.04%	0.005%
55	9.146	2517	2521	2525	rVB2	578	622	0.04%	0.005%
56	9.175	2527	2530	2532	rBV	391	243	0.01%	0.002%
57	9.227	2541	2546	2548	rVV3	276	272	0.02%	0.002%
58	9.268	2557	2559	2563	rVB2	301	241	0.01%	0.002%
59	9.297	2563	2568	2571	rVB2	310	233	0.01%	0.002%
60	9.320	2571	2575	2579	rBV3	300	298	0.02%	0.002%
61	9.448	2613	2615	2618	rVB2	290	190	0.01%	0.001%
62	9.548	2639	2646	2648	rBV4	557	597	0.04%	0.005%
63	9.574	2648	2654	2663	rVV4	638	922	0.06%	0.007%
64	9.638	2669	2674	2677	rBV2	315	247	0.02%	0.002%
65	9.693	2688	2691	2695	rVB2	453	306	0.02%	0.002%
66	9.728	2695	2702	2706	rVB2	378	415	0.03%	0.003%
67	9.834	2732	2735	2740	rVB3	316	264	0.02%	0.002%
68	9.866	2740	2745	2749	rVB2	290	219	0.01%	0.002%
69	10.059	2801	2805	2808	rVV2	269	208	0.01%	0.002%
70	10.153	2829	2834	2836	rBV4	492	469	0.03%	0.004%
71	10.207	2838	2851	2873	rVV	550631	861767	52.49%	6.598%
72	10.432	2918	2921	2925	rBV2	262	227	0.01%	0.002%
73	10.535	2947	2953	2954	rBV3	482	381	0.02%	0.003%
74	10.612	2974	2977	2980	rBV3	324	229	0.01%	0.002%
75	10.670	2989	2995	2997	rBV3	270	276	0.02%	0.002%
76	10.683	2997	2999	3004	rVB2	427	271	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029446.D
 Acq On : 08 Dec 2022 02:59
 Operator : SY/MD
 Sample : N5919-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.712	3004	3008	3011	rBV2	266	265	0.02%	0.002%
78	10.738	3014	3016	3019	rVB3	326	192	0.01%	0.001%
79	10.792	3027	3033	3038	rBV2	488	606	0.04%	0.005%
80	10.837	3041	3047	3055	rBV4	527	734	0.04%	0.006%
81	10.979	3087	3091	3094	rVB3	387	382	0.02%	0.003%
82	11.008	3094	3100	3104	rBV2	324	458	0.03%	0.004%
83	11.172	3146	3151	3152	rBV2	271	194	0.01%	0.001%
84	11.239	3159	3172	3192	rBV	845418	1333660	81.23%	10.211%
85	11.436	3231	3233	3237	rBV4	269	218	0.01%	0.002%
86	11.548	3259	3268	3276	rVV3	2997	5220	0.32%	0.040%
87	11.612	3276	3288	3314	rVV	831645	1325256	80.72%	10.146%
88	11.786	3338	3342	3344	rBV3	290	253	0.02%	0.002%
89	12.194	3466	3469	3473	rVB3	382	321	0.02%	0.002%
90	12.227	3475	3479	3480	rBV2	346	262	0.02%	0.002%
91	12.281	3492	3496	3498	rBV3	218	196	0.01%	0.002%
92	12.329	3509	3511	3513	rBV3	387	227	0.01%	0.002%
93	12.368	3521	3523	3526	rVB2	385	204	0.01%	0.002%
94	12.390	3526	3530	3533	rBV2	294	274	0.02%	0.002%
95	12.532	3569	3574	3576	rBV3	428	412	0.03%	0.003%
96	12.612	3595	3599	3601	rBV	622	480	0.03%	0.004%
97	12.895	3683	3687	3694	rBV4	521	504	0.03%	0.004%
98	13.143	3760	3764	3767	rBV2	511	379	0.02%	0.003%
99	13.268	3802	3803	3806	rBV2	432	226	0.01%	0.002%
100	13.352	3827	3829	3834	rVB2	483	301	0.02%	0.002%




Sum of corrected areas: 13061636

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029446.D
Acq On : 08 Dec 2022 02:59
Operator : SY/MD
Sample : N5919-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

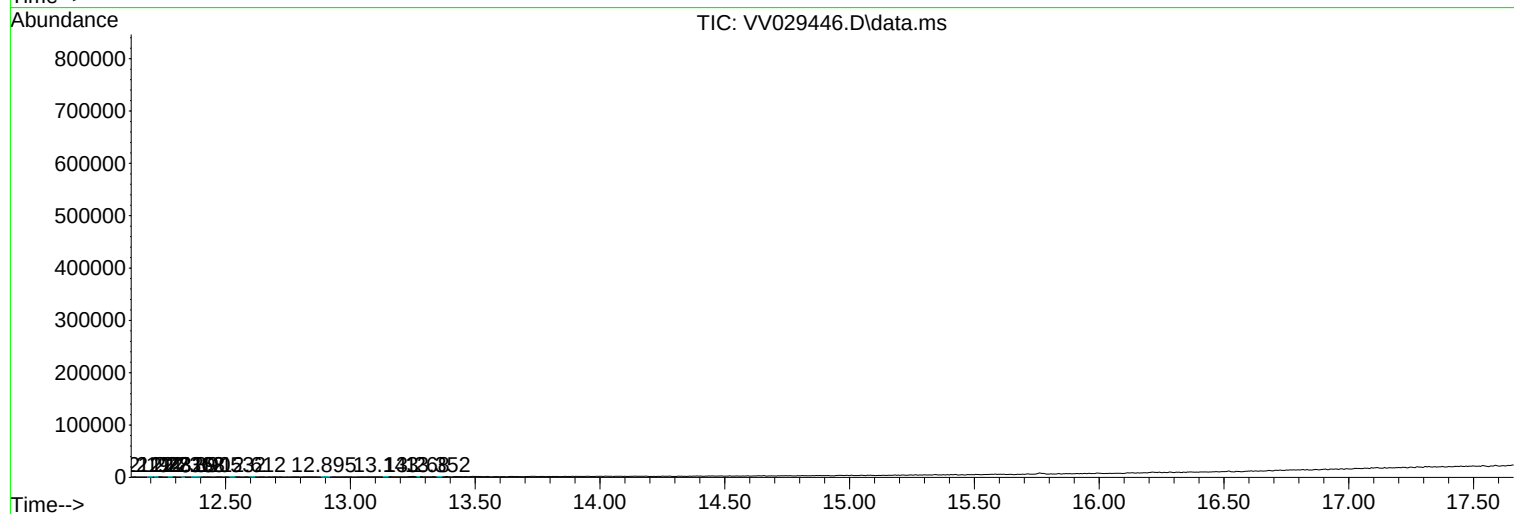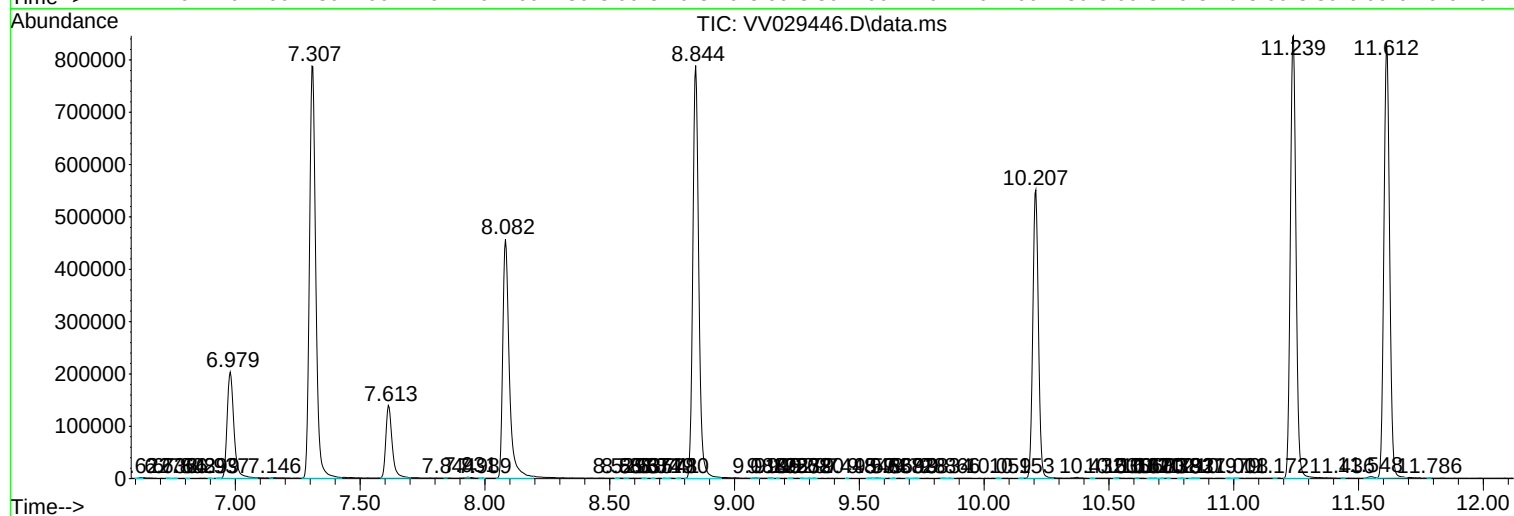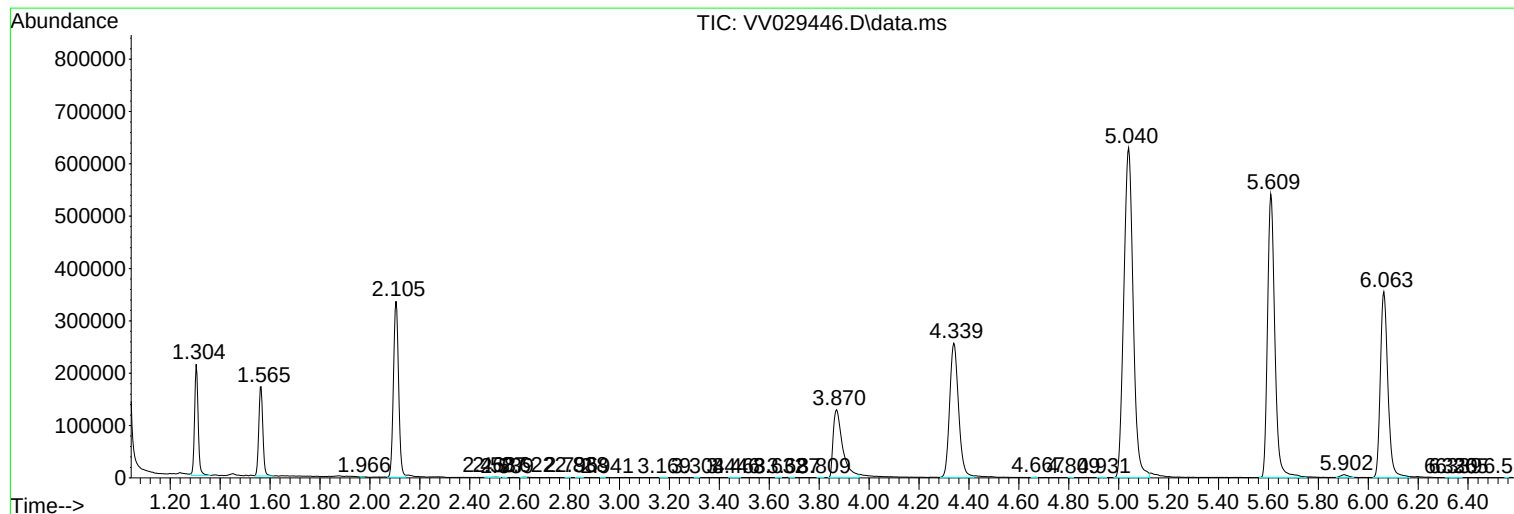

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029446.D
Acq On : 08 Dec 2022 02:59
Operator : SY/MD
Sample : N5919-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029446.D
Acq On : 08 Dec 2022 02:59
Operator : SY/MD
Sample : N5919-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------