

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029447.D
 Acq On : 08 Dec 2022 03:22
 Operator : SY/MD
 Sample : N5919-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029447.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	201752	199897	13.16%	1.629%
2	1.564	155	163	177	rVB	157297	178015	11.72%	1.451%
3	2.104	320	331	345	rBV	309125	445327	29.32%	3.629%
4	2.259	377	379	382	rBV	411	309	0.02%	0.003%
5	2.429	427	432	434	rBV3	404	357	0.02%	0.003%
6	2.503	449	455	460	rBV4	770	912	0.06%	0.007%
7	2.542	464	467	473	rBV4	349	305	0.02%	0.002%
8	2.600	482	485	487	rBV3	403	298	0.02%	0.002%
9	2.622	487	492	504	rVB5	1451	2179	0.14%	0.018%
10	2.757	531	534	541	rVB2	439	422	0.03%	0.003%
11	3.294	696	701	704	rVB2	227	208	0.01%	0.002%
12	3.786	849	854	860	rBV2	252	301	0.02%	0.002%
13	3.870	870	880	921	rBV	117920	319877	21.06%	2.607%
14	4.339	1008	1026	1057	rBV	233132	584964	38.52%	4.767%
15	4.535	1084	1087	1090	rBV2	452	238	0.02%	0.002%
16	4.670	1127	1129	1137	rVB4	427	346	0.02%	0.003%
17	4.786	1162	1165	1169	rVB	245	205	0.01%	0.002%
18	4.911	1201	1204	1213	rVB3	423	512	0.03%	0.004%
19	4.966	1216	1221	1223	rBV2	248	228	0.02%	0.002%
20	5.040	1226	1244	1280	rBV2	581468	1518726	100.00%	12.377%
21	5.365	1342	1345	1349	rVB3	339	218	0.01%	0.002%
22	5.407	1354	1358	1360	rVB3	446	309	0.02%	0.003%
23	5.609	1408	1421	1461	rBV	519544	1061274	69.88%	8.649%
24	5.911	1502	1515	1533	rVV4	35070	74516	4.91%	0.607%
25	6.063	1547	1562	1600	rBV	329091	679945	44.77%	5.541%
26	6.288	1626	1632	1633	rBV3	380	288	0.02%	0.002%
27	6.329	1641	1645	1650	rVB3	300	332	0.02%	0.003%
28	6.378	1654	1660	1662	rBV2	328	295	0.02%	0.002%
29	6.429	1672	1676	1681	rBV2	180	207	0.01%	0.002%
30	6.587	1722	1725	1728	rVB2	430	236	0.02%	0.002%
31	6.622	1728	1736	1737	rBV3	1047	1173	0.08%	0.010%
32	6.667	1748	1750	1755	rVB3	367	212	0.01%	0.002%
33	6.808	1792	1794	1799	rVB3	412	281	0.02%	0.002%
34	6.850	1804	1807	1810	rBV2	391	274	0.02%	0.002%
35	6.979	1835	1847	1878	rBV	188497	344540	22.69%	2.808%
36	7.146	1897	1899	1901	rBV3	476	264	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029447.D
 Acq On : 08 Dec 2022 03:22
 Operator : SY/MD
 Sample : N5919-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.239	1927	1928	1933	rVB2	494	291	0.02%	0.002%
38	7.310	1936	1950	1988	rVV	715745	1269624	83.60%	10.347%
39	7.522	2013	2016	2019	rVB3	423	223	0.01%	0.002%
40	7.615	2033	2045	2072	rBV	126832	228263	15.03%	1.860%
41	7.792	2097	2100	2104	rBV2	408	342	0.02%	0.003%
42	7.934	2139	2144	2155	rVB5	1765	3071	0.20%	0.025%
43	8.082	2180	2190	2226	rBV	418678	767812	50.56%	6.257%
44	8.458	2302	2307	2311	rBV4	357	390	0.03%	0.003%
45	8.638	2360	2363	2366	rBV4	501	315	0.02%	0.003%
46	8.683	2375	2377	2380	rVB2	476	273	0.02%	0.002%
47	8.844	2415	2427	2458	rBV	753868	1248481	82.21%	10.175%
48	9.117	2508	2512	2513	rVV2	301	231	0.02%	0.002%
49	9.140	2513	2519	2528	rVB5	1076	1799	0.12%	0.015%
50	9.226	2543	2546	2549	rVB3	348	228	0.02%	0.002%
51	9.265	2553	2558	2562	rBV2	403	403	0.03%	0.003%
52	9.307	2567	2571	2574	rVB	420	318	0.02%	0.003%
53	9.326	2574	2577	2582	rBV2	282	301	0.02%	0.002%
54	9.423	2602	2607	2610	rVV3	429	470	0.03%	0.004%
55	9.442	2610	2613	2617	rVB2	270	212	0.01%	0.002%
56	9.490	2624	2628	2631	rVB2	340	247	0.02%	0.002%
57	9.513	2631	2635	2637	rVB3	361	242	0.02%	0.002%
58	9.538	2637	2643	2645	rBV3	548	464	0.03%	0.004%
59	9.812	2725	2728	2730	rBV3	454	339	0.02%	0.003%
60	9.934	2761	2766	2769	rBV3	483	403	0.03%	0.003%
61	9.956	2769	2773	2776	rVV3	257	210	0.01%	0.002%
62	10.207	2838	2851	2870	rBV	492871	788971	51.95%	6.430%
63	10.316	2883	2885	2891	rVV3	486	442	0.03%	0.004%
64	10.377	2894	2904	2912	rVB3	1854	2726	0.18%	0.022%
65	10.509	2940	2945	2947	rBV3	587	505	0.03%	0.004%
66	10.641	2983	2986	2988	rBV	334	256	0.02%	0.002%
67	10.686	2998	3000	3005	rVB2	367	289	0.02%	0.002%
68	10.754	3016	3021	3024	rBV2	199	206	0.01%	0.002%
69	10.902	3061	3067	3068	rBV2	333	280	0.02%	0.002%
70	10.985	3091	3093	3095	rBV	288	202	0.01%	0.002%
71	11.040	3107	3110	3114	rVB2	314	223	0.01%	0.002%
72	11.091	3122	3126	3129	rBV2	383	405	0.03%	0.003%
73	11.239	3159	3172	3198	rBV	826018	1292415	85.10%	10.533%
74	11.413	3223	3226	3229	rBV2	333	240	0.02%	0.002%
75	11.445	3232	3236	3239	rBV2	389	284	0.02%	0.002%
76	11.548	3260	3268	3276	rBV3	5141	8865	0.58%	0.072%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029447.D
 Acq On : 08 Dec 2022 03:22
 Operator : SY/MD
 Sample : N5919-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.612	3276	3288	3318	rVB	773089	1223085	80.53%	9.968%
78	11.808	3348	3349	3352	rVB2	511	201	0.01%	0.002%
79	11.947	3390	3392	3396	rVB3	353	225	0.01%	0.002%
80	11.979	3400	3402	3406	rVB3	466	232	0.02%	0.002%
81	12.033	3416	3419	3424	rVB2	297	250	0.02%	0.002%
82	12.056	3424	3426	3433	rBV3	394	420	0.03%	0.003%
83	12.127	3446	3448	3451	rVB2	391	218	0.01%	0.002%
84	12.188	3462	3467	3470	rBV4	337	340	0.02%	0.003%
85	12.342	3513	3515	3518	rVB	577	291	0.02%	0.002%
86	12.554	3577	3581	3584	rBV2	581	449	0.03%	0.004%
87	12.696	3620	3625	3628	rBV4	321	321	0.02%	0.003%
88	12.853	3670	3674	3677	rBV2	663	621	0.04%	0.005%
89	13.056	3733	3737	3740	rBV4	469	339	0.02%	0.003%
90	13.210	3782	3785	3787	rBV	351	279	0.02%	0.002%
91	13.249	3795	3797	3798	rBV	521	244	0.02%	0.002%
92	13.384	3837	3839	3843	rVB3	467	309	0.02%	0.003%
93	13.416	3843	3849	3852	rBV3	783	890	0.06%	0.007%
94	13.477	3865	3868	3870	rBV3	555	389	0.03%	0.003%
95	13.538	3885	3887	3888	rBV2	511	259	0.02%	0.002%
96	13.593	3902	3904	3907	rVB2	699	361	0.02%	0.003%
97	13.670	3925	3928	3930	rBV2	402	331	0.02%	0.003%
98	13.741	3948	3950	3953	rBV2	644	357	0.02%	0.003%
99	13.863	3986	3988	3993	rBV	579	460	0.03%	0.004%
100	14.191	4088	4090	4093	rBV3	634	292	0.02%	0.002%




Sum of corrected areas: 12270414

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029447.D
Acq On : 08 Dec 2022 03:22
Operator : SY/MD
Sample : N5919-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

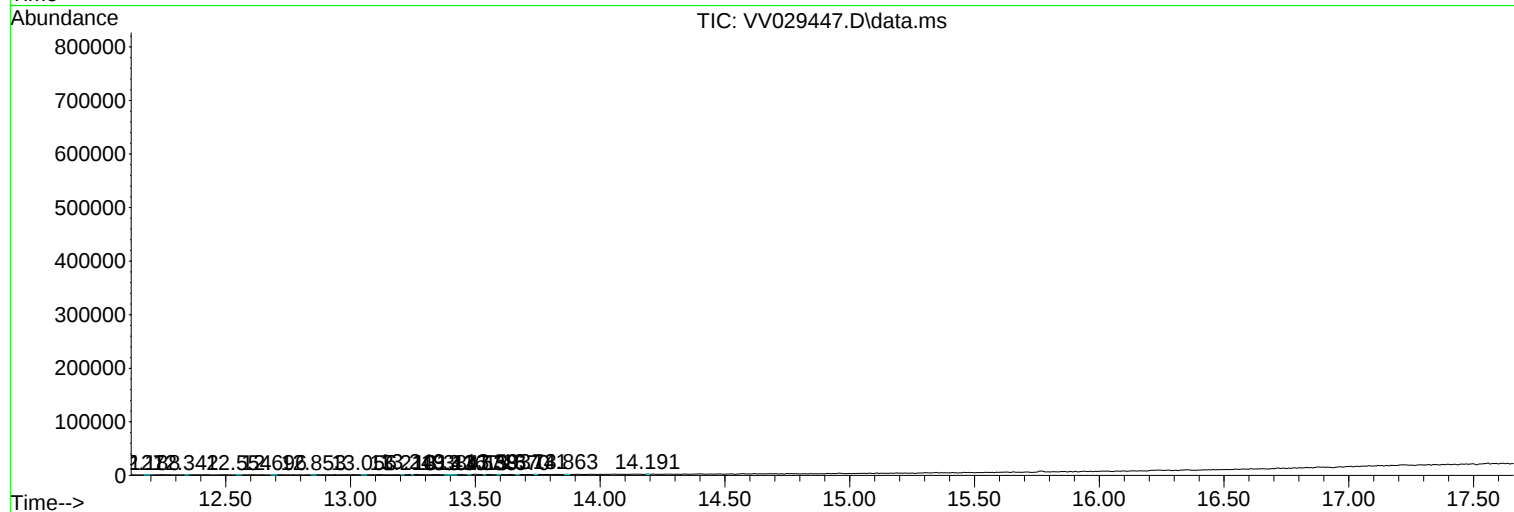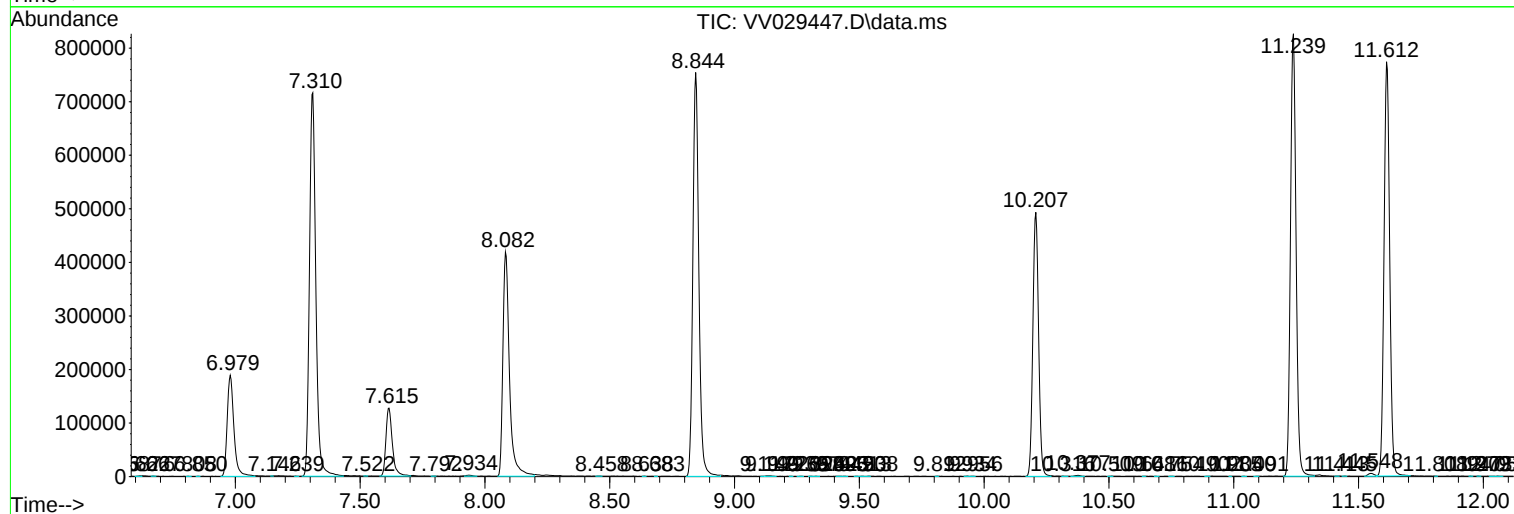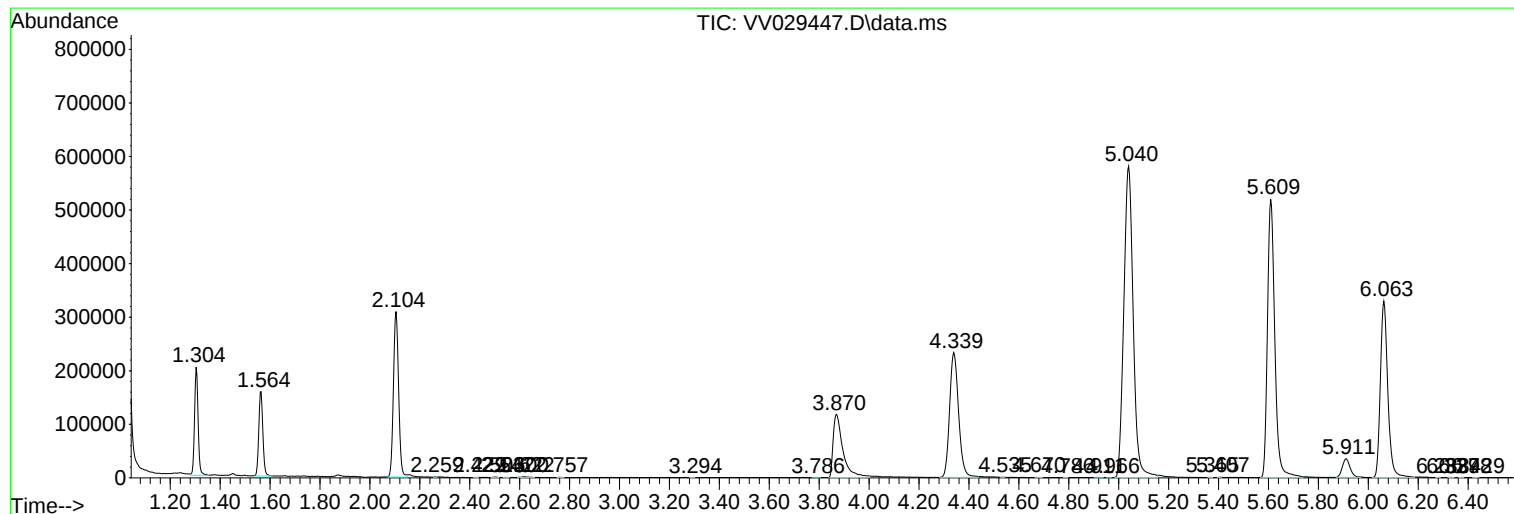

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029447.D
Acq On : 08 Dec 2022 03:22
Operator : SY/MD
Sample : N5919-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029447.D
Acq On : 08 Dec 2022 03:22
Operator : SY/MD
Sample : N5919-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------