

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029448.D
 Acq On : 08 Dec 2022 03:46
 Operator : SY/MD
 Sample : N5919-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	218280	212308	13.58%	1.676%
2	1.564	155	163	176	rVB	165755	187483	11.99%	1.480%
3	2.105	318	331	356	rBV2	350018	538351	34.42%	4.249%
4	2.285	383	387	396	rVB6	1289	1870	0.12%	0.015%
5	2.381	415	417	424	rVV2	400	359	0.02%	0.003%
6	2.497	448	453	458	rBV4	848	1060	0.07%	0.008%
7	2.551	464	470	473	rVB3	304	288	0.02%	0.002%
8	2.584	477	480	485	rVB3	321	277	0.02%	0.002%
9	2.616	485	490	495	rBV3	514	726	0.05%	0.006%
10	2.786	541	543	548	rVV2	243	207	0.01%	0.002%
11	2.870	566	569	573	rVB	459	216	0.01%	0.002%
12	2.892	573	576	582	rBV	217	258	0.02%	0.002%
13	2.960	595	597	601	rVB2	392	239	0.02%	0.002%
14	3.172	659	663	664	rBV2	698	462	0.03%	0.004%
15	3.262	685	691	694	rBV2	319	293	0.02%	0.002%
16	3.285	694	698	702	rVV3	268	235	0.02%	0.002%
17	3.323	707	710	713	rVV2	231	211	0.01%	0.002%
18	3.867	866	879	919	rBV	117703	379585	24.27%	2.996%
19	4.339	1009	1026	1063	rBV	239968	599142	38.31%	4.728%
20	4.539	1086	1088	1091	rVB3	367	222	0.01%	0.002%
21	4.600	1096	1107	1123	rVB2	6462	15175	0.97%	0.120%
22	4.664	1123	1127	1131	rVB2	324	287	0.02%	0.002%
23	4.805	1168	1171	1177	rVB	299	215	0.01%	0.002%
24	4.915	1198	1205	1210	rBV3	237	275	0.02%	0.002%
25	5.040	1226	1244	1284	rBV2	589442	1563919	100.00%	12.342%
26	5.272	1313	1316	1318	rBV2	297	213	0.01%	0.002%
27	5.413	1357	1360	1363	rBV3	520	352	0.02%	0.003%
28	5.458	1371	1374	1377	rBV2	332	295	0.02%	0.002%
29	5.477	1377	1380	1385	rVB2	193	220	0.01%	0.002%
30	5.609	1407	1421	1461	rBV	533014	1088369	69.59%	8.589%
31	5.908	1502	1514	1528	rBV7	11704	27650	1.77%	0.218%
32	6.063	1547	1562	1599	rBV	339304	697470	44.60%	5.504%
33	6.249	1618	1620	1623	rVB2	387	232	0.01%	0.002%
34	6.268	1623	1626	1629	rBV3	265	216	0.01%	0.002%
35	6.439	1674	1679	1682	rBV	245	228	0.01%	0.002%
36	6.558	1712	1716	1719	rBV	293	240	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029448.D
 Acq On : 08 Dec 2022 03:46
 Operator : SY/MD
 Sample : N5919-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.928	1824	1831	1835	rBV4	434	455	0.03%	0.004%
38	6.979	1835	1847	1878	rBV	191913	352791	22.56%	2.784%
39	7.159	1899	1903	1908	rBV4	725	789	0.05%	0.006%
40	7.243	1926	1929	1933	rBV3	519	455	0.03%	0.004%
41	7.307	1937	1949	1983	rBV	738878	1315753	84.13%	10.384%
42	7.612	2034	2044	2070	rBV	130199	233014	14.90%	1.839%
43	7.825	2106	2110	2112	rBV2	643	503	0.03%	0.004%
44	7.934	2138	2144	2154	rVB3	1736	2575	0.16%	0.020%
45	8.082	2179	2190	2225	rBV	416289	756918	48.40%	5.974%
46	8.400	2287	2289	2292	rBV2	333	226	0.01%	0.002%
47	8.452	2303	2305	2309	rVB3	507	215	0.01%	0.002%
48	8.587	2344	2347	2352	rBV3	502	493	0.03%	0.004%
49	8.844	2415	2427	2455	rBV	771949	1276067	81.59%	10.071%
50	9.027	2482	2484	2488	rVB3	475	251	0.02%	0.002%
51	9.062	2493	2495	2500	rVB4	407	256	0.02%	0.002%
52	9.130	2511	2516	2519	rBV3	562	644	0.04%	0.005%
53	9.320	2571	2575	2577	rBV3	388	287	0.02%	0.002%
54	9.371	2589	2591	2598	rVB2	315	360	0.02%	0.003%
55	9.538	2638	2643	2645	rBV2	352	316	0.02%	0.002%
56	9.554	2645	2648	2652	rVB	350	233	0.01%	0.002%
57	9.921	2753	2762	2765	rBV4	379	507	0.03%	0.004%
58	9.998	2783	2786	2793	rBV3	383	400	0.03%	0.003%
59	10.107	2813	2820	2822	rBV3	236	241	0.02%	0.002%
60	10.152	2827	2834	2838	rBV3	345	495	0.03%	0.004%
61	10.207	2838	2851	2869	rBV	503535	794926	50.83%	6.274%
62	10.297	2876	2879	2882	rVB	523	333	0.02%	0.003%
63	10.365	2897	2900	2901	rBV2	1243	696	0.04%	0.005%
64	10.535	2950	2953	2956	rBV2	382	292	0.02%	0.002%
65	10.779	3027	3029	3033	rVB2	414	234	0.01%	0.002%
66	10.844	3046	3049	3055	rVB3	504	501	0.03%	0.004%
67	10.879	3055	3060	3063	rBV	275	237	0.02%	0.002%
68	10.918	3067	3072	3076	rVB4	393	372	0.02%	0.003%
69	11.140	3135	3141	3144	rBV3	423	433	0.03%	0.003%
70	11.175	3149	3152	3155	rBV2	464	289	0.02%	0.002%
71	11.239	3160	3172	3191	rBV	868329	1325673	84.77%	10.462%
72	11.484	3245	3248	3251	rVB3	335	209	0.01%	0.002%
73	11.548	3260	3268	3276	rBV3	5382	9576	0.61%	0.076%
74	11.612	3276	3288	3318	rVB	795914	1264128	80.83%	9.976%
75	11.776	3336	3339	3344	rVB3	396	377	0.02%	0.003%
76	11.844	3357	3360	3362	rVB2	355	213	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029448.D
 Acq On : 08 Dec 2022 03:46
 Operator : SY/MD
 Sample : N5919-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.860	3362	3365	3368	rBV2	418	296	0.02%	0.002%
78	12.043	3417	3422	3425	rBV3	518	527	0.03%	0.004%
79	12.062	3425	3428	3431	rVV3	352	241	0.02%	0.002%
80	12.130	3445	3449	3452	rBV3	300	210	0.01%	0.002%
81	12.194	3466	3469	3475	rBV4	352	350	0.02%	0.003%
82	12.236	3480	3482	3486	rVV3	513	310	0.02%	0.002%
83	12.381	3520	3527	3530	rBV3	479	517	0.03%	0.004%
84	12.455	3547	3550	3552	rBV2	429	202	0.01%	0.002%
85	12.512	3564	3568	3574	rVV3	489	502	0.03%	0.004%
86	12.667	3610	3616	3618	rBV3	413	466	0.03%	0.004%
87	12.763	3642	3646	3648	rBV3	482	396	0.03%	0.003%
88	12.808	3656	3660	3661	rBV3	315	207	0.01%	0.002%
89	13.030	3727	3729	3733	rBV2	565	450	0.03%	0.004%
90	13.056	3734	3737	3740	rVV2	368	273	0.02%	0.002%
91	13.120	3754	3757	3758	rBV2	330	218	0.01%	0.002%
92	13.233	3789	3792	3795	rBV2	548	467	0.03%	0.004%
93	13.249	3795	3797	3804	rVB6	703	678	0.04%	0.005%
94	13.361	3829	3832	3837	rVB5	354	294	0.02%	0.002%
95	13.387	3837	3840	3844	rBV2	486	370	0.02%	0.003%
96	13.422	3848	3851	3852	rBV	560	345	0.02%	0.003%
97	13.490	3868	3872	3873	rBV2	442	305	0.02%	0.002%
98	13.644	3916	3920	3926	rBV5	399	529	0.03%	0.004%
99	13.731	3943	3947	3951	rBV3	874	788	0.05%	0.006%
100	13.953	4014	4016	4018	rBV2	599	297	0.02%	0.002%




Sum of corrected areas: 12671119

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029448.D
Acq On : 08 Dec 2022 03:46
Operator : SY/MD
Sample : N5919-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

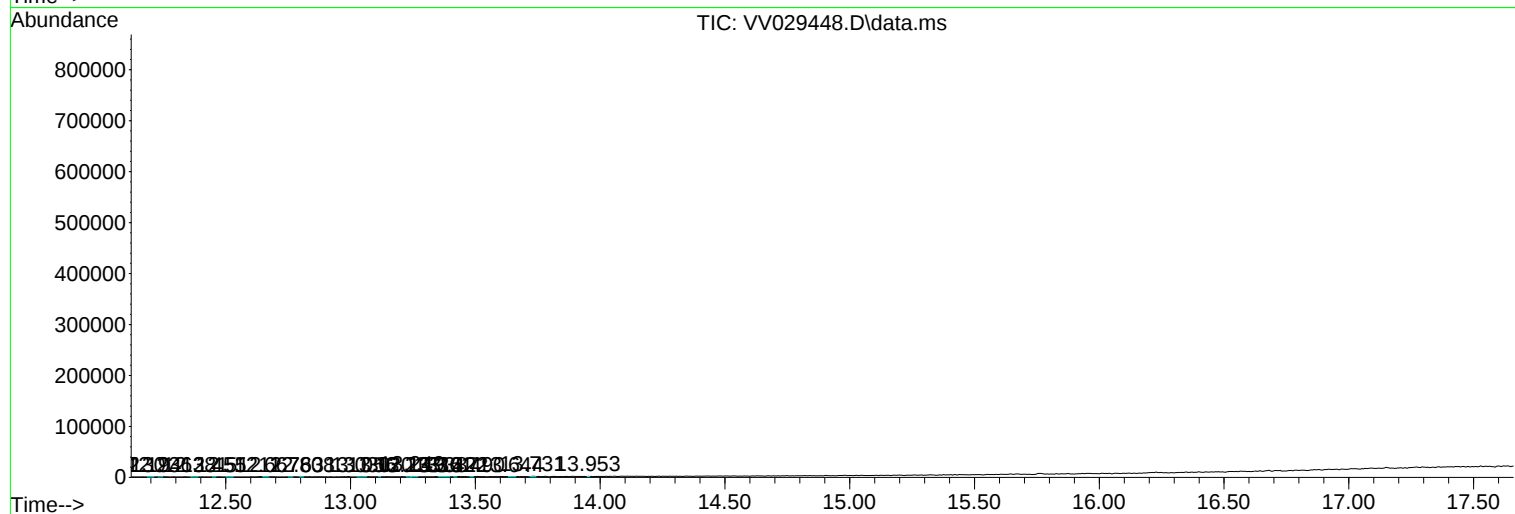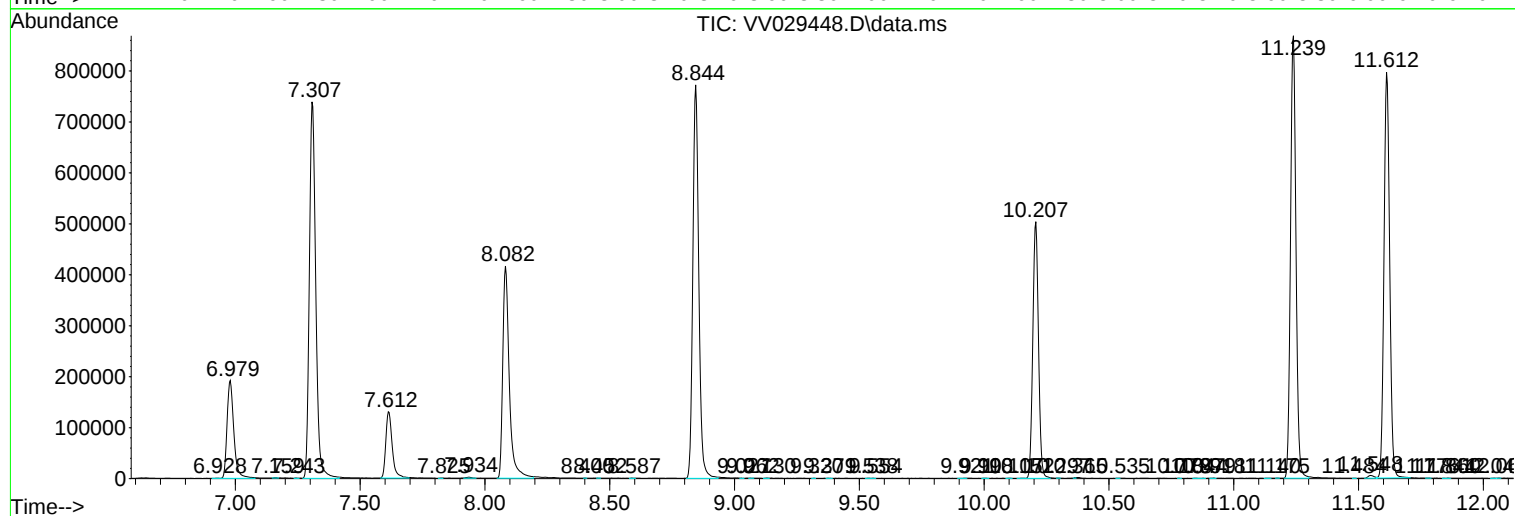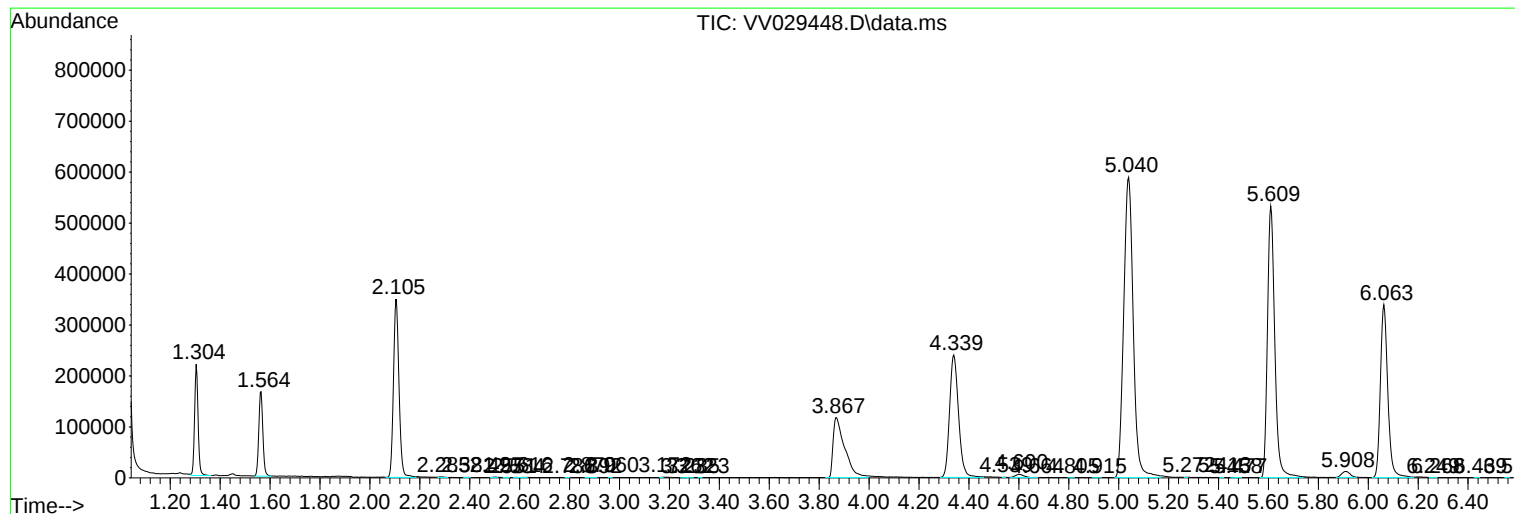

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029448.D
Acq On : 08 Dec 2022 03:46
Operator : SY/MD
Sample : N5919-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029448.D
Acq On : 08 Dec 2022 03:46
Operator : SY/MD
Sample : N5919-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------