

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029450.D
 Acq On : 08 Dec 2022 04:33
 Operator : SY/MD
 Sample : N5919-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	196985	196755	12.95%	1.615%
2	1.564	155	163	178	rVB	160700	179817	11.84%	1.476%
3	2.053	313	315	318	rBV4	350	238	0.02%	0.002%
4	2.105	319	331	354	rBV	308917	445619	29.34%	3.658%
5	2.265	377	381	383	rBV3	596	500	0.03%	0.004%
6	2.497	445	453	454	rBV3	685	599	0.04%	0.005%
7	2.834	553	558	565	rVB3	379	490	0.03%	0.004%
8	2.921	579	585	590	rBV3	250	340	0.02%	0.003%
9	3.185	664	667	672	rVV3	450	393	0.03%	0.003%
10	3.223	675	679	682	rBV2	285	246	0.02%	0.002%
11	3.445	745	748	755	rVB	261	214	0.01%	0.002%
12	3.487	755	761	765	rBV2	240	301	0.02%	0.002%
13	3.870	870	880	914	rBV	113208	304777	20.07%	2.502%
14	4.339	1007	1026	1049	rBV	235054	578984	38.12%	4.753%
15	4.497	1073	1075	1079	rVB2	673	370	0.02%	0.003%
16	4.635	1115	1118	1124	rVB3	324	282	0.02%	0.002%
17	4.738	1147	1150	1156	rVB3	344	341	0.02%	0.003%
18	4.773	1156	1161	1165	rBV3	485	387	0.03%	0.003%
19	4.934	1205	1211	1213	rVB2	268	211	0.01%	0.002%
20	5.040	1220	1244	1293	rBV2	576608	1518803	100.00%	12.468%
21	5.291	1317	1322	1326	rBV4	388	446	0.03%	0.004%
22	5.410	1357	1359	1366	rVB3	530	408	0.03%	0.003%
23	5.513	1388	1391	1395	rVB3	428	284	0.02%	0.002%
24	5.609	1408	1421	1463	rBV	522541	1069566	70.42%	8.780%
25	5.850	1494	1496	1501	rVB3	386	213	0.01%	0.002%
26	5.899	1501	1511	1513	rBV5	5151	6035	0.40%	0.050%
27	6.063	1548	1562	1600	rBV	325245	675000	44.44%	5.541%
28	6.278	1627	1629	1632	rBV	538	268	0.02%	0.002%
29	6.313	1636	1640	1645	rBV3	307	309	0.02%	0.003%
30	6.619	1728	1735	1737	rBV3	963	1021	0.07%	0.008%
31	6.809	1790	1794	1797	rVB3	383	276	0.02%	0.002%
32	6.886	1816	1818	1824	rVB3	445	343	0.02%	0.003%
33	6.979	1835	1847	1881	rVV	185788	341188	22.46%	2.801%
34	7.146	1896	1899	1902	rBV2	504	400	0.03%	0.003%
35	7.310	1937	1950	1982	rBV	704661	1264099	83.23%	10.377%
36	7.612	2034	2044	2065	rBV	127407	221549	14.59%	1.819%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029450.D
 Acq On : 08 Dec 2022 04:33
 Operator : SY/MD
 Sample : N5919-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.908	2129	2136	2137	rBV4	380	450	0.03%	0.004%
38	7.931	2137	2143	2151	rVB3	1683	2445	0.16%	0.020%
39	8.082	2179	2190	2228	rBV	418632	754757	49.69%	6.196%
40	8.413	2289	2293	2296	rBV4	441	357	0.02%	0.003%
41	8.477	2309	2313	2316	rBV2	264	257	0.02%	0.002%
42	8.545	2328	2334	2336	rBV4	449	383	0.03%	0.003%
43	8.693	2375	2380	2386	rBV3	247	290	0.02%	0.002%
44	8.844	2415	2427	2454	rVV	763139	1259917	82.95%	10.343%
45	9.246	2547	2552	2556	rBV2	418	472	0.03%	0.004%
46	9.287	2561	2565	2568	rVB3	404	346	0.02%	0.003%
47	9.403	2597	2601	2602	rBV	307	255	0.02%	0.002%
48	9.570	2651	2653	2658	rVB2	346	264	0.02%	0.002%
49	9.603	2659	2663	2669	rBV	403	415	0.03%	0.003%
50	9.635	2669	2673	2675	rBV2	260	230	0.02%	0.002%
51	9.648	2675	2677	2683	rVB3	375	331	0.02%	0.003%
52	9.731	2700	2703	2706	rVB2	406	228	0.02%	0.002%
53	9.773	2710	2716	2717	rBV2	277	252	0.02%	0.002%
54	9.821	2728	2731	2734	rVB	341	232	0.02%	0.002%
55	9.853	2738	2741	2743	rBV2	374	218	0.01%	0.002%
56	9.921	2759	2762	2765	rVB	521	394	0.03%	0.003%
57	9.963	2773	2775	2783	rBV2	212	285	0.02%	0.002%
58	10.017	2785	2792	2795	rBV3	363	389	0.03%	0.003%
59	10.043	2798	2800	2804	rVB2	548	331	0.02%	0.003%
60	10.078	2804	2811	2815	rBV3	397	487	0.03%	0.004%
61	10.207	2834	2851	2869	rBV	498672	786829	51.81%	6.459%
62	10.371	2893	2902	2912	rBV5	2000	3534	0.23%	0.029%
63	10.474	2928	2934	2941	rVB5	331	447	0.03%	0.004%
64	10.667	2987	2994	2995	rBV2	274	262	0.02%	0.002%
65	10.763	3022	3024	3029	rVB2	323	248	0.02%	0.002%
66	10.795	3029	3034	3040	rBV3	334	390	0.03%	0.003%
67	10.828	3040	3044	3047	rBV2	481	412	0.03%	0.003%
68	10.844	3047	3049	3052	rVB2	424	220	0.01%	0.002%
69	10.863	3052	3055	3059	rVB2	364	291	0.02%	0.002%
70	10.908	3064	3069	3072	rBV4	777	734	0.05%	0.006%
71	10.927	3072	3075	3079	rVB2	361	293	0.02%	0.002%
72	10.956	3079	3084	3085	rBV3	473	334	0.02%	0.003%
73	11.001	3095	3098	3101	rVB3	390	261	0.02%	0.002%
74	11.239	3159	3172	3197	rBV	841835	1315112	86.59%	10.796%
75	11.551	3261	3269	3276	rVV7	3869	6786	0.45%	0.056%
76	11.612	3276	3288	3320	rVB	776991	1222351	80.48%	10.035%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029450.D
 Acq On : 08 Dec 2022 04:33
 Operator : SY/MD
 Sample : N5919-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	12.139	3448	3452	3456	rVB3	462	383	0.03%	0.003%
78	12.168	3456	3461	3464	rBV2	363	364	0.02%	0.003%
79	12.271	3489	3493	3494	rBV3	537	325	0.02%	0.003%
80	12.339	3512	3514	3518	rVB3	560	256	0.02%	0.002%
81	12.490	3558	3561	3569	rVB2	462	509	0.03%	0.004%
82	12.570	3583	3586	3590	rVV2	318	243	0.02%	0.002%
83	12.625	3599	3603	3604	rBV2	325	259	0.02%	0.002%
84	12.635	3604	3606	3611	rVB4	343	264	0.02%	0.002%
85	12.686	3619	3622	3629	rBV3	397	394	0.03%	0.003%
86	12.718	3629	3632	3633	rBV2	343	212	0.01%	0.002%
87	12.747	3637	3641	3644	rVB3	294	234	0.02%	0.002%
88	12.779	3648	3651	3655	rBV2	385	347	0.02%	0.003%
89	12.824	3662	3665	3669	rBV2	489	362	0.02%	0.003%
90	12.908	3688	3691	3693	rBV3	370	266	0.02%	0.002%
91	12.934	3697	3699	3703	rVV4	323	234	0.02%	0.002%
92	13.008	3720	3722	3726	rBV3	409	261	0.02%	0.002%
93	13.130	3758	3760	3763	rBV2	470	217	0.01%	0.002%
94	13.348	3825	3828	3830	rBV2	526	407	0.03%	0.003%
95	13.403	3843	3845	3847	rBV3	526	225	0.01%	0.002%
96	13.419	3848	3850	3854	rVB3	668	406	0.03%	0.003%
97	13.599	3903	3906	3909	rBV2	493	299	0.02%	0.002%
98	13.895	3996	3998	4002	rVB2	611	306	0.02%	0.003%
99	13.921	4004	4006	4009	rBV2	496	339	0.02%	0.003%
100	14.892	4305	4308	4310	rBV3	972	778	0.05%	0.006%


Sum of corrected areas: 12181451

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029450.D
Acq On : 08 Dec 2022 04:33
Operator : SY/MD
Sample : N5919-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

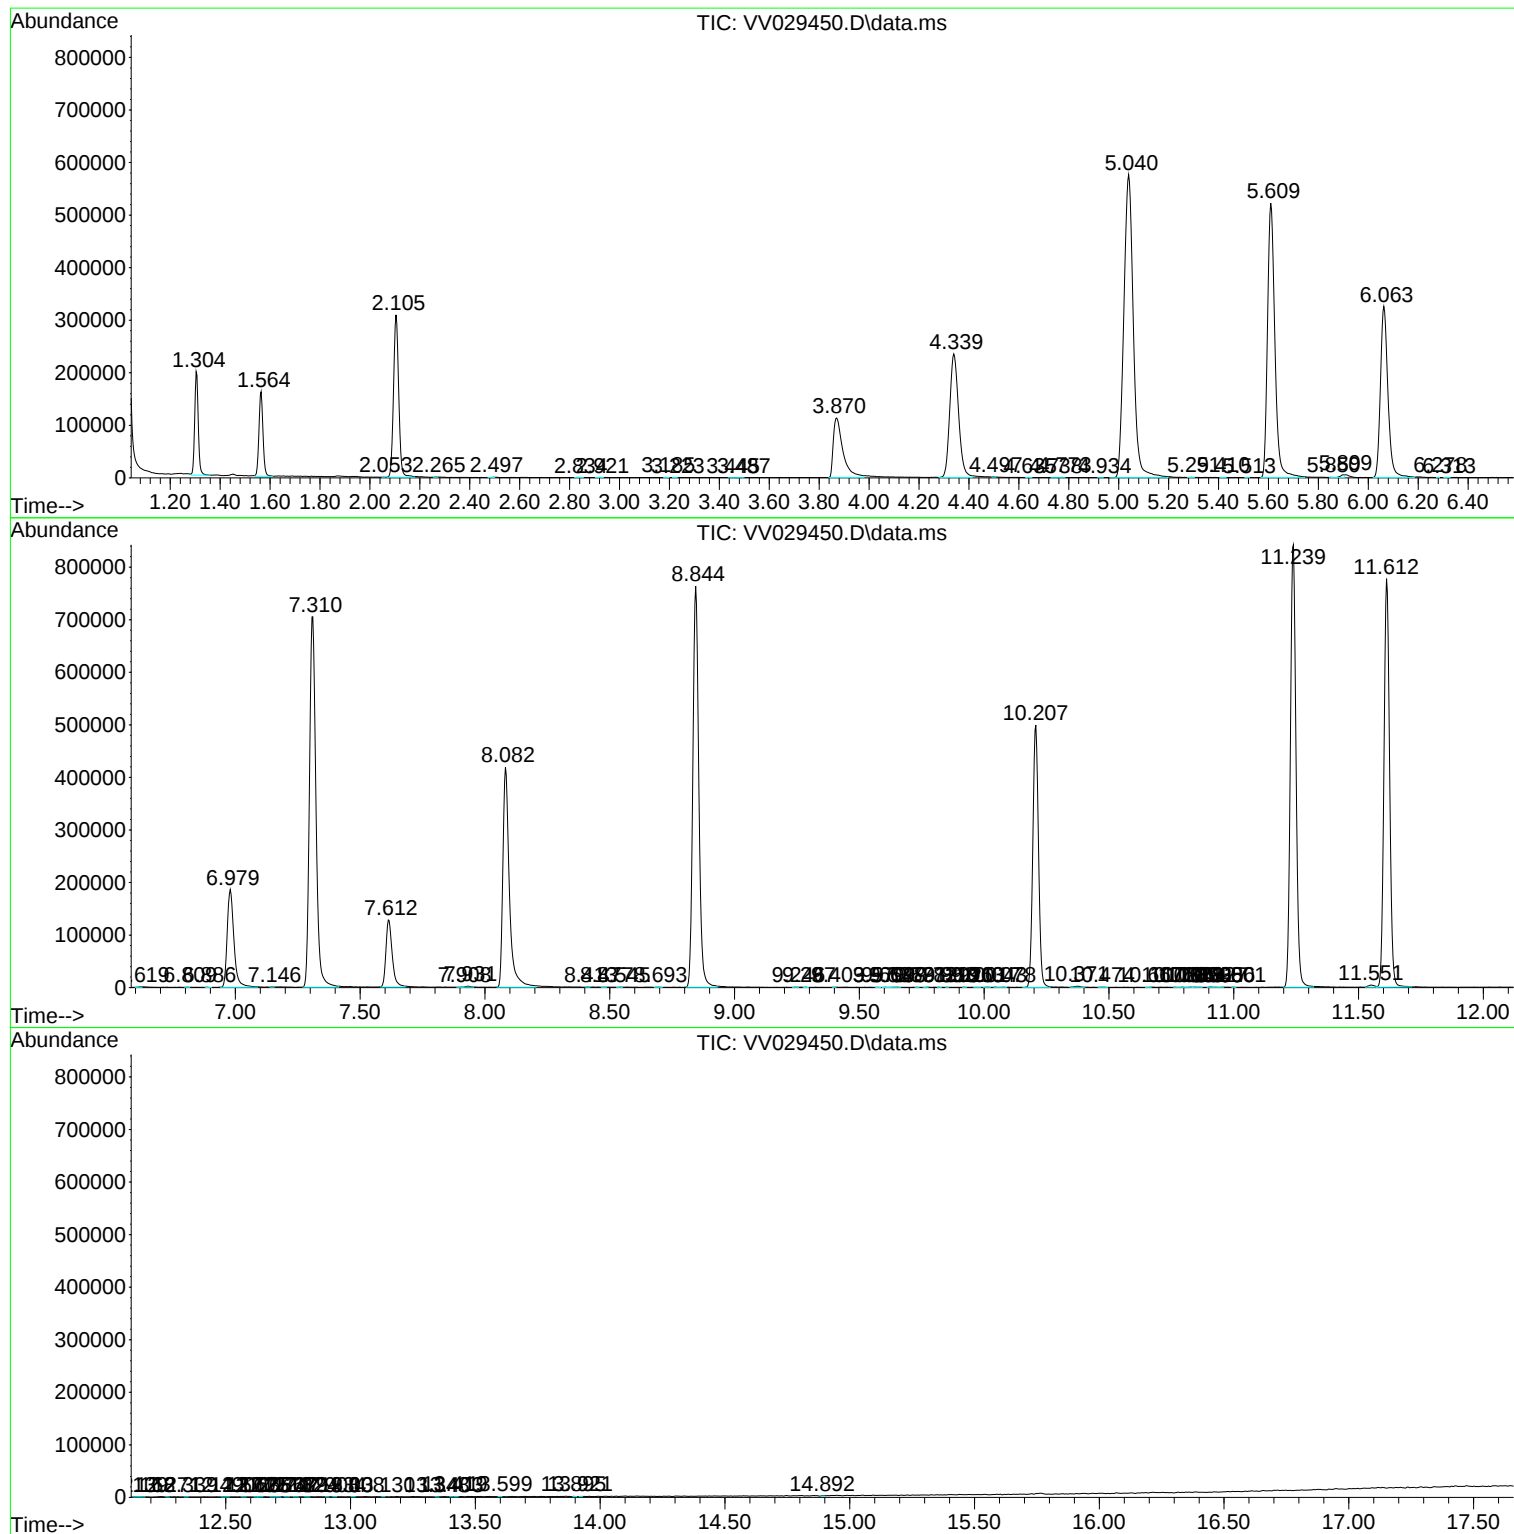

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029450.D
Acq On : 08 Dec 2022 04:33
Operator : SY/MD
Sample : N5919-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029450.D
Acq On : 08 Dec 2022 04:33
Operator : SY/MD
Sample : N5919-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------