

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029451.D
 Acq On : 08 Dec 2022 04:57
 Operator : SY/MD
 Sample : N5919-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	198762	192028	12.10%	1.509%
2	1.561	155	162	179	rVB	166622	187225	11.80%	1.471%
3	2.105	320	331	345	rBV	320524	459078	28.93%	3.608%
4	2.503	450	455	462	rVB4	922	1144	0.07%	0.009%
5	2.536	462	465	468	rBV3	322	244	0.02%	0.002%
6	2.587	479	481	484	rBV	181	77	0.00%	0.001%
7	2.606	484	487	488	rBV	353	162	0.01%	0.001%
8	2.896	574	577	580	rBV2	304	208	0.01%	0.002%
9	2.941	588	591	596	rBV2	425	498	0.03%	0.004%
10	3.044	621	623	627	rVB2	309	161	0.01%	0.001%
11	3.069	629	631	635	rVB2	160	71	0.00%	0.001%
12	3.092	635	638	640	rBV	228	149	0.01%	0.001%
13	3.246	684	686	688	rVB	327	117	0.01%	0.001%
14	3.272	692	694	696	rVB2	197	80	0.01%	0.001%
15	3.327	709	711	712	rBV2	213	94	0.01%	0.001%
16	3.359	719	721	723	rBV3	299	138	0.01%	0.001%
17	3.462	751	753	756	rVB	243	105	0.01%	0.001%
18	3.481	756	759	760	rBV2	140	76	0.00%	0.001%
19	3.548	777	780	782	rBV	127	74	0.00%	0.001%
20	3.561	782	784	786	rVB	210	71	0.00%	0.001%
21	3.648	806	811	813	rBV	208	149	0.01%	0.001%
22	3.667	813	817	819	rBV	174	137	0.01%	0.001%
23	3.700	825	827	835	rVB2	231	149	0.01%	0.001%
24	3.757	843	845	848	rBV	152	107	0.01%	0.001%
25	3.870	870	880	911	rBV	121809	327845	20.66%	2.577%
26	4.339	1009	1026	1051	rBV	246207	608119	38.32%	4.779%
27	4.616	1110	1112	1117	rVB3	497	224	0.01%	0.002%
28	4.703	1138	1139	1142	rVB	257	108	0.01%	0.001%
29	4.728	1144	1147	1149	rVB	177	100	0.01%	0.001%
30	4.757	1152	1156	1158	rBV	321	216	0.01%	0.002%
31	4.783	1161	1164	1168	rVB2	247	149	0.01%	0.001%
32	4.831	1176	1179	1181	rBV	136	85	0.01%	0.001%
33	4.870	1186	1191	1194	rVB2	197	157	0.01%	0.001%
34	4.909	1199	1203	1207	rBV3	299	267	0.02%	0.002%
35	4.954	1211	1217	1220	rBV2	242	225	0.01%	0.002%
36	4.973	1220	1223	1226	rBV2	194	118	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029451.D
 Acq On : 08 Dec 2022 04:57
 Operator : SY/MD
 Sample : N5919-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.040	1226	1244	1283	rBV2	601811	1587062	100.00%	12.473%
38	5.355	1339	1342	1346	rBV2	415	277	0.02%	0.002%
39	5.404	1353	1357	1362	rBV3	361	413	0.03%	0.003%
40	5.545	1393	1401	1406	rBV4	563	874	0.06%	0.007%
41	5.609	1408	1421	1451	rBV	551165	1115480	70.29%	8.767%
42	5.912	1503	1515	1532	rVB5	21749	45670	2.88%	0.359%
43	6.063	1547	1562	1587	rBV	342378	703890	44.35%	5.532%
44	6.304	1635	1637	1638	rBV	115	29	0.00%	0.000%
45	6.349	1650	1651	1654	rBV2	172	88	0.01%	0.001%
46	6.394	1663	1665	1667	rBV	171	64	0.00%	0.001%
47	6.420	1671	1673	1677	rBV3	253	182	0.01%	0.001%
48	6.487	1691	1694	1695	rBV2	260	164	0.01%	0.001%
49	6.593	1723	1727	1728	rBV2	345	204	0.01%	0.002%
50	6.709	1761	1763	1765	rVB2	381	153	0.01%	0.001%
51	6.793	1786	1789	1795	rVB4	465	394	0.02%	0.003%
52	6.818	1795	1797	1798	rBV	163	88	0.01%	0.001%
53	6.867	1809	1812	1815	rVB2	249	180	0.01%	0.001%
54	6.886	1815	1818	1821	rBV2	230	181	0.01%	0.001%
55	6.912	1825	1826	1829	rBV2	132	92	0.01%	0.001%
56	6.979	1836	1847	1884	rBV	191039	355208	22.38%	2.792%
57	7.307	1937	1949	1977	rBV	747295	1321046	83.24%	10.383%
58	7.613	2034	2044	2070	rBV	130868	232553	14.65%	1.828%
59	8.082	2179	2190	2233	rBV	448130	805237	50.74%	6.329%
60	8.641	2360	2364	2367	rBV	599	385	0.02%	0.003%
61	8.844	2415	2427	2463	rBV	799604	1327249	83.63%	10.431%
62	9.047	2487	2490	2492	rBV2	368	249	0.02%	0.002%
63	9.175	2529	2530	2534	rVB	211	88	0.01%	0.001%
64	9.217	2537	2543	2546	rBV3	634	513	0.03%	0.004%
65	9.278	2558	2562	2564	rBV	214	180	0.01%	0.001%
66	9.384	2590	2595	2596	rBV	292	252	0.02%	0.002%
67	9.416	2603	2605	2607	rBV	119	55	0.00%	0.000%
68	9.487	2625	2627	2631	rVB2	257	139	0.01%	0.001%
69	9.606	2659	2664	2666	rBV2	373	310	0.02%	0.002%
70	9.703	2686	2694	2703	rBV3	315	640	0.04%	0.005%
71	9.834	2732	2735	2736	rBV2	211	96	0.01%	0.001%
72	9.876	2746	2748	2752	rBV2	231	200	0.01%	0.002%
73	9.902	2753	2756	2759	rVV3	359	242	0.02%	0.002%
74	10.088	2813	2814	2817	rBV3	266	107	0.01%	0.001%
75	10.124	2823	2825	2827	rBV	223	147	0.01%	0.001%
76	10.207	2838	2851	2874	rBV	518728	820926	51.73%	6.452%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029451.D
 Acq On : 08 Dec 2022 04:57
 Operator : SY/MD
 Sample : N5919-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.371	2897	2902	2913	rVB4	1718	2478	0.16%	0.019%
78	10.632	2981	2983	2987	rBV	142	107	0.01%	0.001%
79	10.712	3004	3008	3012	rBV2	376	372	0.02%	0.003%
80	10.857	3051	3053	3056	rVB2	341	167	0.01%	0.001%
81	10.963	3082	3086	3090	rBV	425	336	0.02%	0.003%
82	11.075	3117	3121	3123	rBV2	506	392	0.02%	0.003%
83	11.146	3140	3143	3145	rBV	294	161	0.01%	0.001%
84	11.239	3160	3172	3200	rBV	890271	1378615	86.87%	10.835%
85	11.503	3248	3254	3258	rBV4	455	543	0.03%	0.004%
86	11.548	3261	3268	3277	rVV4	5335	9341	0.59%	0.073%
87	11.612	3277	3288	3311	rVB	779794	1228924	77.43%	9.659%
88	11.818	3349	3352	3354	rBV2	369	260	0.02%	0.002%
89	12.034	3417	3419	3423	rBV2	328	235	0.01%	0.002%
90	12.821	3660	3664	3667	rBV2	624	534	0.03%	0.004%




Sum of corrected areas: 12723727

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029451.D
Acq On : 08 Dec 2022 04:57
Operator : SY/MD
Sample : N5919-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EG8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

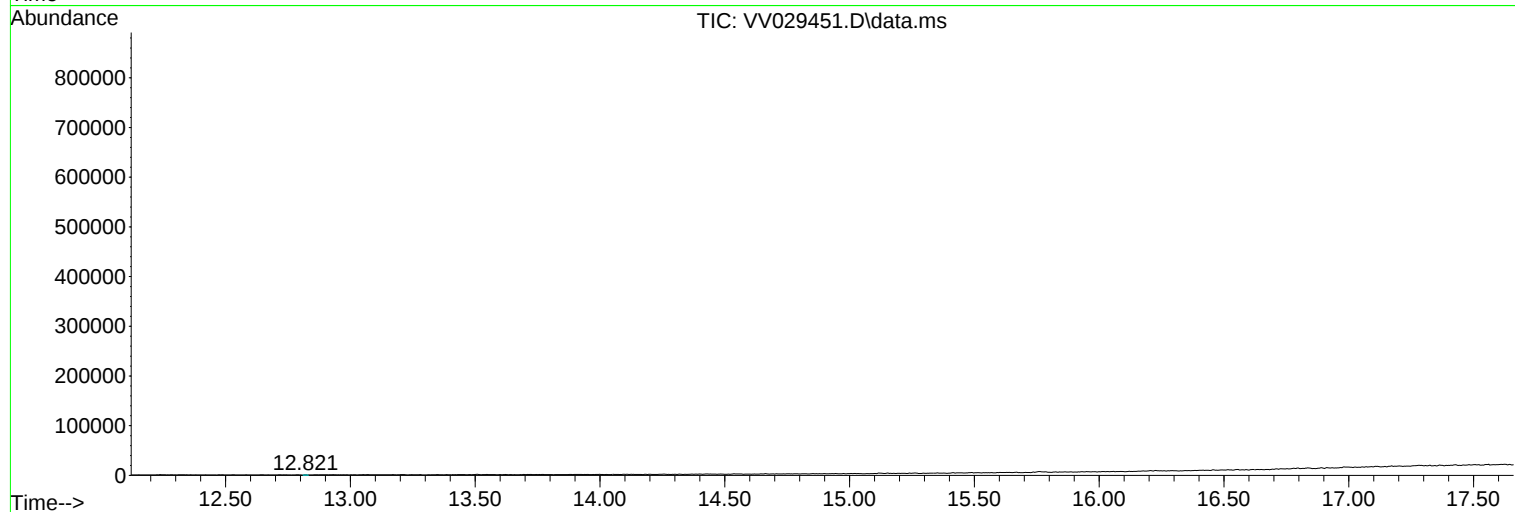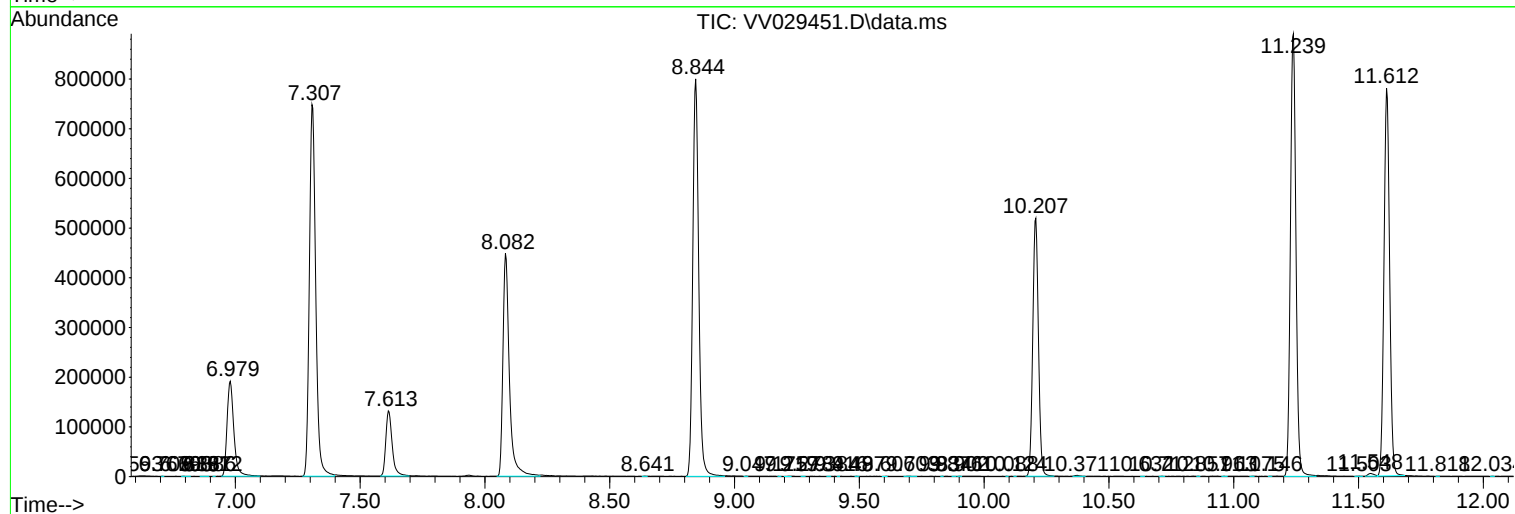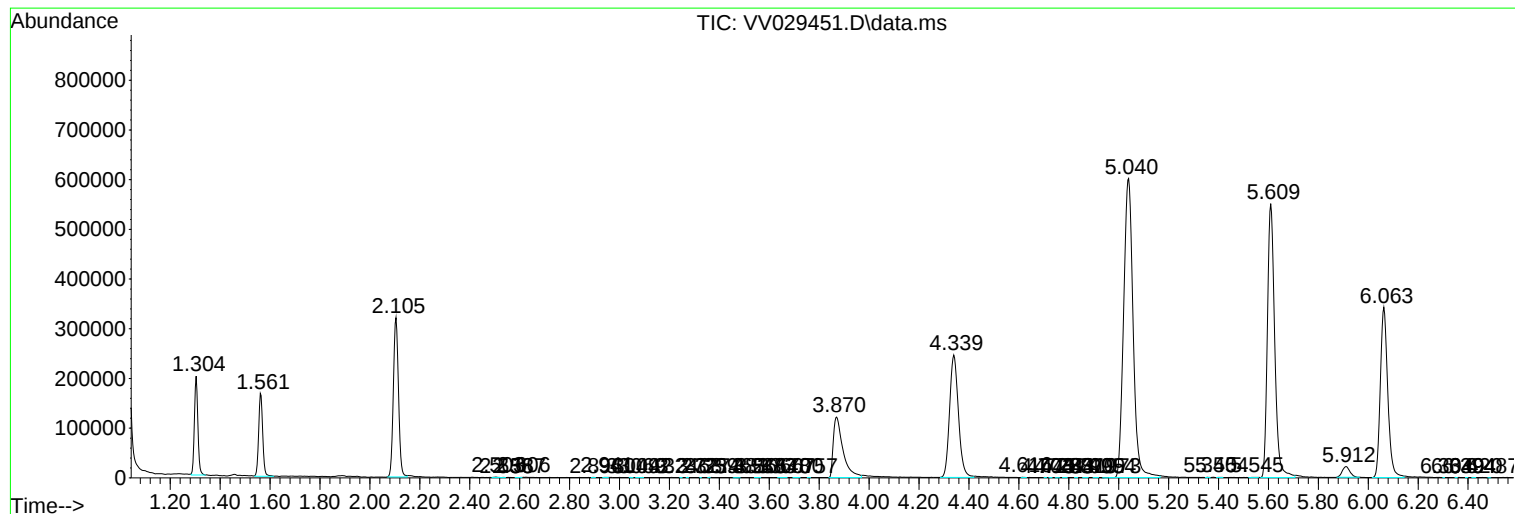

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029451.D
Acq On : 08 Dec 2022 04:57
Operator : SY/MD
Sample : N5919-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EG8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029451.D
Acq On : 08 Dec 2022 04:57
Operator : SY/MD
Sample : N5919-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EG8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------