

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120722\
 Data File : VW029452.D
 Acq On : 08 Dec 2022 05:20
 Operator : SY/MD
 Sample : N5919-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COEH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	201444	195410	13.03%	1.624%
2	1.564	155	163	178	rVB	155121	177899	11.86%	1.478%
3	1.796	233	235	238	rBV	825	536	0.04%	0.004%
4	2.104	319	331	344	rBV	307041	440516	29.37%	3.660%
5	2.272	377	383	396	rVB3	4360	8300	0.55%	0.069%
6	2.436	430	434	435	rBV	297	215	0.01%	0.002%
7	2.497	450	453	454	rBV	564	336	0.02%	0.003%
8	2.619	487	491	501	rVV3	906	1161	0.08%	0.010%
9	2.754	530	533	537	rVB2	360	310	0.02%	0.003%
10	2.863	563	567	572	rBV2	299	269	0.02%	0.002%
11	2.892	572	576	581	rBV3	319	230	0.02%	0.002%
12	3.030	610	619	622	rBV2	313	340	0.02%	0.003%
13	3.201	669	672	676	rVB2	303	211	0.01%	0.002%
14	3.487	756	761	763	rBV2	250	247	0.02%	0.002%
15	3.539	774	777	781	rVB2	290	208	0.01%	0.002%
16	3.651	807	812	816	rVB2	256	207	0.01%	0.002%
17	3.870	870	880	922	rBV	114375	311350	20.76%	2.587%
18	4.339	1009	1026	1057	rBV	233115	582232	38.82%	4.837%
19	4.593	1101	1105	1109	rBV4	467	438	0.03%	0.004%
20	4.651	1121	1123	1127	rBV2	243	197	0.01%	0.002%
21	4.744	1147	1152	1155	rVB2	265	228	0.02%	0.002%
22	5.040	1226	1244	1282	rBV3	567433	1499836	100.00%	12.461%
23	5.609	1408	1421	1467	rBV	510599	1037096	69.15%	8.617%
24	5.854	1495	1497	1502	rVB	564	243	0.02%	0.002%
25	5.905	1502	1513	1526	rVB8	4693	10831	0.72%	0.090%
26	5.966	1526	1532	1536	rBV4	339	420	0.03%	0.003%
27	6.063	1548	1562	1593	rBV	325132	669017	44.61%	5.558%
28	6.265	1621	1625	1627	rVB3	560	382	0.03%	0.003%
29	6.436	1674	1678	1681	rBV	342	278	0.02%	0.002%
30	6.509	1697	1701	1703	rVB2	275	220	0.01%	0.002%
31	6.625	1729	1737	1738	rBV3	1129	1154	0.08%	0.010%
32	6.654	1744	1746	1749	rVB	610	359	0.02%	0.003%
33	6.757	1773	1778	1779	rBV2	221	200	0.01%	0.002%
34	6.799	1787	1791	1794	rBV2	457	390	0.03%	0.003%
35	6.876	1813	1815	1820	rBV2	219	238	0.02%	0.002%
36	6.979	1835	1847	1872	rBV	184280	337795	22.52%	2.807%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029452.D
 Acq On : 08 Dec 2022 05:20
 Operator : SY/MD
 Sample : N5919-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COEH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.136	1893	1896	1897	rBV2	402	219	0.01%	0.002%
38	7.204	1915	1917	1920	rVB3	491	261	0.02%	0.002%
39	7.310	1936	1950	1984	rBV	709197	1259175	83.95%	10.462%
40	7.612	2034	2044	2080	rVV	127821	225651	15.05%	1.875%
41	7.738	2080	2083	2086	rVB3	463	257	0.02%	0.002%
42	7.828	2110	2111	2115	rVB3	460	191	0.01%	0.002%
43	8.082	2180	2190	2225	rBV	415743	753853	50.26%	6.263%
44	8.384	2282	2284	2288	rVB	495	308	0.02%	0.003%
45	8.493	2316	2318	2320	rBV3	321	193	0.01%	0.002%
46	8.628	2356	2360	2361	rBV2	305	219	0.01%	0.002%
47	8.731	2389	2392	2396	rVB2	280	252	0.02%	0.002%
48	8.754	2396	2399	2401	rBV3	327	206	0.01%	0.002%
49	8.783	2405	2408	2411	rBV4	357	294	0.02%	0.002%
50	8.844	2413	2427	2452	rBV	746469	1217686	81.19%	10.117%
51	9.056	2490	2493	2496	rVB3	397	233	0.02%	0.002%
52	9.117	2507	2512	2515	rBV3	527	401	0.03%	0.003%
53	9.136	2515	2518	2521	rBV4	487	317	0.02%	0.003%
54	9.172	2527	2529	2535	rBV3	355	284	0.02%	0.002%
55	9.326	2573	2577	2582	rVB3	363	304	0.02%	0.003%
56	9.355	2582	2586	2588	rBV2	293	200	0.01%	0.002%
57	9.371	2588	2591	2595	rVB2	310	227	0.02%	0.002%
58	9.538	2638	2643	2645	rBV3	580	385	0.03%	0.003%
59	9.561	2648	2650	2654	rVV3	997	719	0.05%	0.006%
60	9.635	2670	2673	2677	rBV	347	327	0.02%	0.003%
61	9.744	2705	2707	2713	rVB3	251	204	0.01%	0.002%
62	9.850	2738	2740	2746	rVB3	317	326	0.02%	0.003%
63	9.914	2753	2760	2764	rBV4	420	445	0.03%	0.004%
64	9.937	2764	2767	2775	rVB3	315	345	0.02%	0.003%
65	9.969	2775	2777	2782	rBV2	204	225	0.02%	0.002%
66	10.207	2835	2851	2874	rBV	496995	782962	52.20%	6.505%
67	10.284	2874	2875	2883	rVV3	639	692	0.05%	0.006%
68	10.377	2893	2904	2911	rVB6	1728	2806	0.19%	0.023%
69	10.467	2929	2932	2936	rBV3	234	210	0.01%	0.002%
70	10.493	2936	2940	2941	rBV2	363	249	0.02%	0.002%
71	10.644	2985	2987	2994	rVB2	318	296	0.02%	0.002%
72	10.738	3013	3016	3021	rBV2	288	214	0.01%	0.002%
73	10.776	3025	3028	3037	rBV2	341	400	0.03%	0.003%
74	10.818	3037	3041	3046	rVV5	295	277	0.02%	0.002%
75	10.840	3046	3048	3055	rVB4	501	292	0.02%	0.002%
76	10.908	3065	3069	3073	rBV3	624	549	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029452.D
 Acq On : 08 Dec 2022 05:20
 Operator : SY/MD
 Sample : N5919-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.959	3078	3085	3087	rBV3	334	341	0.02%	0.003%
78	11.014	3100	3102	3107	rVB3	331	323	0.02%	0.003%
79	11.088	3121	3125	3128	rBV	271	251	0.02%	0.002%
80	11.239	3160	3172	3204	rBV	821069	1276852	85.13%	10.609%
81	11.387	3216	3218	3221	rVB2	649	303	0.02%	0.003%
82	11.461	3239	3241	3245	rVB2	370	263	0.02%	0.002%
83	11.548	3261	3268	3276	rBV4	3596	6626	0.44%	0.055%
84	11.612	3276	3288	3310	rVV	790285	1213302	80.90%	10.081%
85	11.837	3353	3358	3360	rBV3	343	325	0.02%	0.003%
86	11.853	3360	3363	3371	rVV5	332	393	0.03%	0.003%
87	11.992	3404	3406	3412	rVB2	302	263	0.02%	0.002%
88	12.020	3412	3415	3420	rBV3	471	417	0.03%	0.003%
89	12.111	3439	3443	3445	rBV2	270	202	0.01%	0.002%
90	12.342	3511	3515	3517	rBV2	363	300	0.02%	0.002%
91	12.628	3601	3604	3607	rBV2	506	307	0.02%	0.003%
92	12.686	3619	3622	3624	rBV2	365	295	0.02%	0.002%
93	12.815	3658	3662	3665	rVB3	353	253	0.02%	0.002%
94	13.178	3773	3775	3777	rVB2	518	221	0.01%	0.002%
95	13.242	3792	3795	3799	rBV5	594	654	0.04%	0.005%
96	13.416	3847	3849	3852	rBV2	538	231	0.02%	0.002%
97	13.490	3868	3872	3878	rBV4	668	840	0.06%	0.007%
98	13.590	3900	3903	3906	rBB3	577	368	0.02%	0.003%
99	13.631	3913	3916	3918	rBV3	380	276	0.02%	0.002%
100	14.107	4061	4064	4069	rBV4	757	523	0.03%	0.004%




Sum of corrected areas: 12036082

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029452.D
Acq On : 08 Dec 2022 05:20
Operator : SY/MD
Sample : N5919-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COEH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

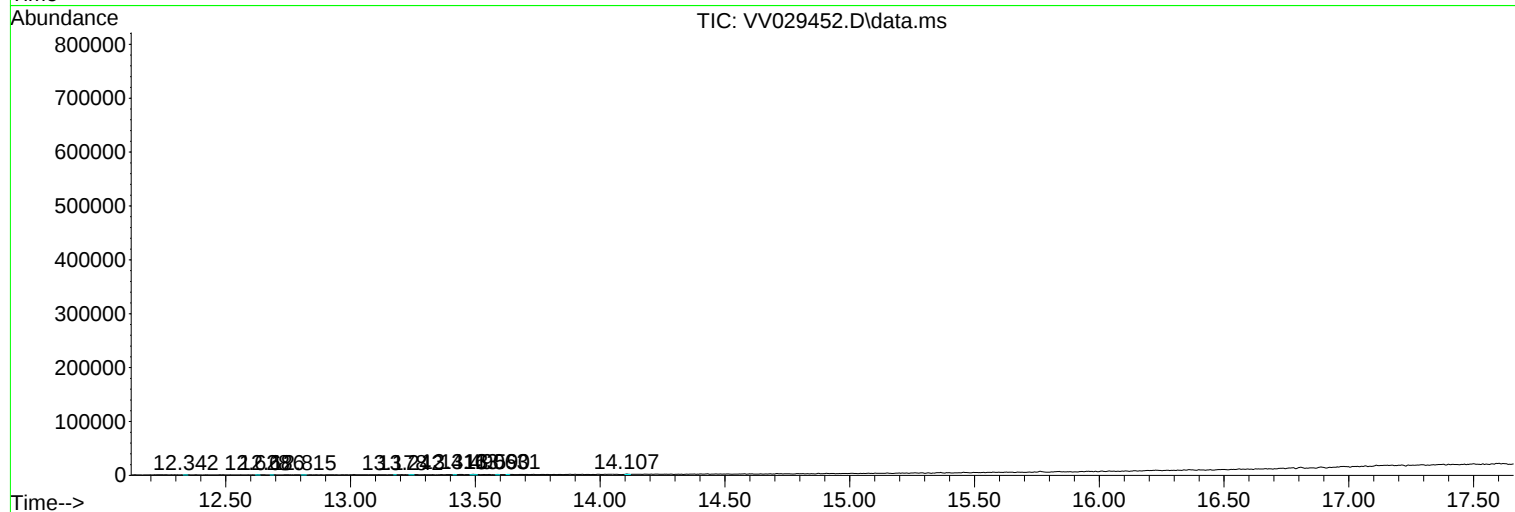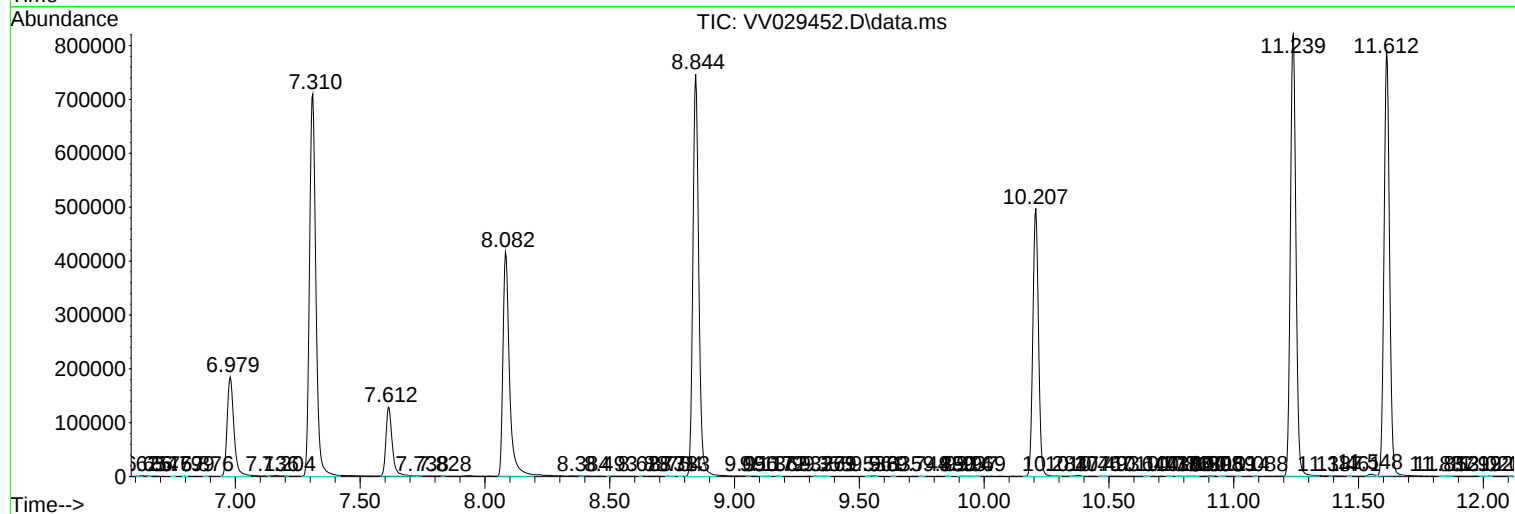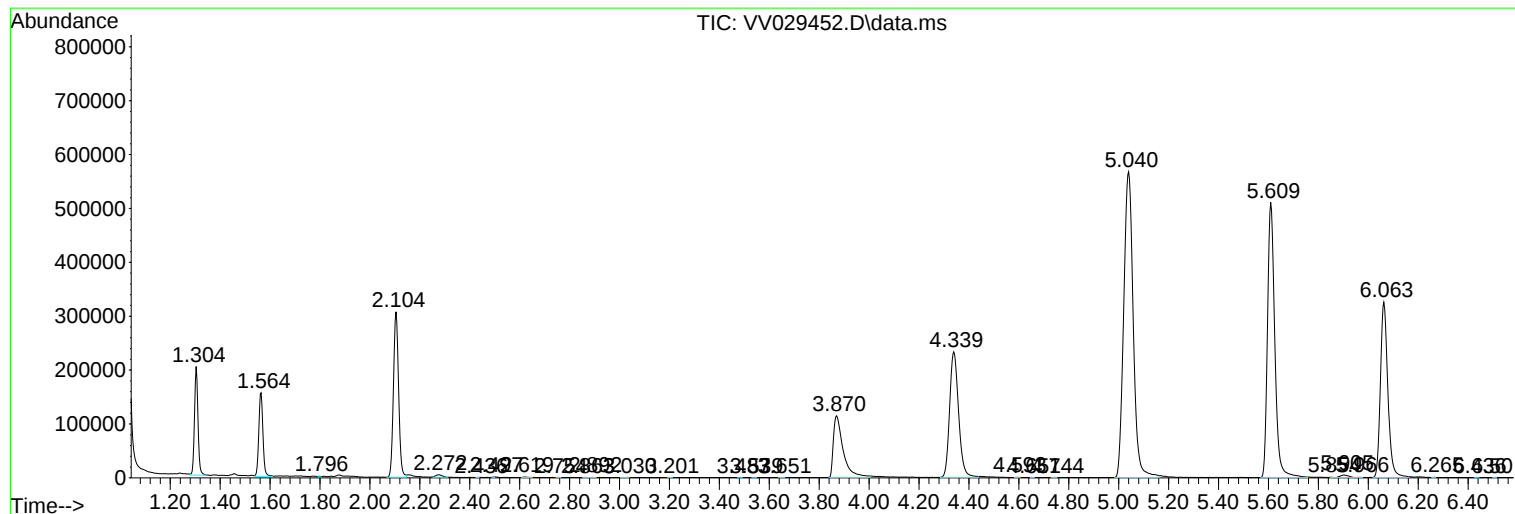

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029452.D
Acq On : 08 Dec 2022 05:20
Operator : SY/MD
Sample : N5919-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029452.D
Acq On : 08 Dec 2022 05:20
Operator : SY/MD
Sample : N5919-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc