

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029453.D
 Acq On : 08 Dec 2022 05:44
 Operator : SY/MD
 Sample : N5919-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	198874	197306	12.40%	1.545%
2	1.564	155	163	179	rVB	168577	188623	11.86%	1.477%
3	1.873	254	259	266	rVB3	2754	3585	0.23%	0.028%
4	2.056	314	316	320	rBV4	381	223	0.01%	0.002%
5	2.104	320	331	346	rBV	320789	464409	29.19%	3.636%
6	2.268	373	382	395	rVB	5750	10925	0.69%	0.086%
7	2.503	449	455	456	rBV2	901	813	0.05%	0.006%
8	2.622	490	492	496	rVV2	349	199	0.01%	0.002%
9	2.786	540	543	546	rBV2	318	232	0.01%	0.002%
10	2.944	588	592	595	rBV2	292	202	0.01%	0.002%
11	3.297	700	702	709	rVV2	205	210	0.01%	0.002%
12	3.870	870	880	912	rBV	121812	323123	20.31%	2.530%
13	4.201	979	983	986	rBV3	391	271	0.02%	0.002%
14	4.339	1010	1026	1064	rBV	245697	611993	38.47%	4.792%
15	4.616	1110	1112	1121	rVB2	523	637	0.04%	0.005%
16	4.696	1133	1137	1140	rBV	318	254	0.02%	0.002%
17	4.796	1164	1168	1170	rBV2	283	214	0.01%	0.002%
18	4.815	1172	1174	1179	rVB2	274	229	0.01%	0.002%
19	4.899	1195	1200	1204	rVB2	350	304	0.02%	0.002%
20	4.931	1204	1210	1213	rBV2	341	314	0.02%	0.002%
21	5.040	1226	1244	1294	rBV2	601999	1590908	100.00%	12.457%
22	5.445	1368	1370	1372	rBV	368	206	0.01%	0.002%
23	5.477	1377	1380	1384	rVB3	344	233	0.01%	0.002%
24	5.609	1407	1421	1458	rBV	550481	1124646	70.69%	8.806%
25	5.911	1502	1515	1537	rVB4	22083	48590	3.05%	0.380%
26	6.063	1547	1562	1599	rBV	343743	705486	44.34%	5.524%
27	6.284	1628	1631	1633	rBV2	391	244	0.02%	0.002%
28	6.410	1665	1670	1672	rBV2	240	205	0.01%	0.002%
29	6.580	1716	1723	1726	rBV3	301	399	0.03%	0.003%
30	6.625	1729	1737	1746	rVV5	998	1965	0.12%	0.015%
31	6.979	1835	1847	1881	rBV	190499	357973	22.50%	2.803%
32	7.252	1928	1932	1934	rBV4	456	298	0.02%	0.002%
33	7.310	1937	1950	1983	rBV	734165	1318837	82.90%	10.327%
34	7.570	2025	2031	2032	rBV2	385	314	0.02%	0.002%
35	7.612	2034	2044	2072	rVV	129275	231304	14.54%	1.811%
36	7.776	2091	2095	2097	rBV4	282	251	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120722\
 Data File : VW029453.D
 Acq On : 08 Dec 2022 05:44
 Operator : SY/MD
 Sample : N5919-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.812	2103	2106	2110	rVB4	501	372	0.02%	0.003%
38	7.931	2138	2143	2145	rBV3	975	1090	0.07%	0.009%
39	8.017	2168	2170	2173	rBV2	310	204	0.01%	0.002%
40	8.082	2179	2190	2227	rBV	425480	783407	49.24%	6.134%
41	8.606	2349	2353	2356	rBV3	374	283	0.02%	0.002%
42	8.660	2364	2370	2374	rBV3	431	496	0.03%	0.004%
43	8.705	2382	2384	2391	rVB3	251	272	0.02%	0.002%
44	8.760	2399	2401	2404	rBV2	288	210	0.01%	0.002%
45	8.844	2415	2427	2454	rBV	809633	1322422	83.12%	10.355%
46	9.085	2499	2502	2506	rBV3	519	557	0.04%	0.004%
47	9.111	2506	2510	2513	rVV3	531	471	0.03%	0.004%
48	9.127	2513	2515	2517	rVV2	408	226	0.01%	0.002%
49	9.143	2517	2520	2523	rVV3	601	526	0.03%	0.004%
50	9.162	2524	2526	2529	rVV2	602	333	0.02%	0.003%
51	9.181	2529	2532	2534	rVV3	280	209	0.01%	0.002%
52	9.201	2534	2538	2543	rVB5	576	599	0.04%	0.005%
53	9.242	2543	2551	2553	rBV3	386	527	0.03%	0.004%
54	9.281	2559	2563	2568	rVB2	373	450	0.03%	0.004%
55	9.429	2607	2609	2618	rVB2	249	202	0.01%	0.002%
56	9.535	2640	2642	2648	rVB2	475	358	0.02%	0.003%
57	9.561	2648	2650	2652	rBV2	387	199	0.01%	0.002%
58	9.574	2652	2654	2659	rVB2	580	356	0.02%	0.003%
59	9.609	2659	2665	2669	rBV3	522	505	0.03%	0.004%
60	10.056	2800	2804	2809	rVB2	552	440	0.03%	0.003%
61	10.130	2824	2827	2830	rBV2	356	273	0.02%	0.002%
62	10.207	2838	2851	2872	rBV	518261	811485	51.01%	6.354%
63	10.284	2872	2875	2878	rBV3	428	310	0.02%	0.002%
64	10.374	2896	2903	2910	rBV5	1781	2140	0.13%	0.017%
65	10.603	2969	2974	2978	rBV3	260	314	0.02%	0.002%
66	10.699	2996	3004	3012	rBV2	289	489	0.03%	0.004%
67	10.738	3013	3016	3022	rVB2	455	469	0.03%	0.004%
68	10.789	3031	3032	3040	rVB3	271	260	0.02%	0.002%
69	10.840	3044	3048	3053	rBV3	558	461	0.03%	0.004%
70	10.902	3064	3067	3069	rBV2	378	238	0.01%	0.002%
71	10.943	3075	3080	3085	rBV4	416	575	0.04%	0.005%
72	11.075	3119	3121	3127	rVB2	341	317	0.02%	0.002%
73	11.159	3144	3147	3149	rBV	335	216	0.01%	0.002%
74	11.239	3158	3172	3197	rBV	877420	1374259	86.38%	10.761%
75	11.519	3255	3259	3261	rBV3	302	280	0.02%	0.002%
76	11.548	3261	3268	3276	rBV5	2662	4751	0.30%	0.037%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029453.D
 Acq On : 08 Dec 2022 05:44
 Operator : SY/MD
 Sample : N5919-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.612	3276	3288	3318	rVB	802092	1265118	79.52%	9.906%
78	11.840	3356	3359	3360	rBV2	356	219	0.01%	0.002%
79	11.963	3394	3397	3401	rBV3	294	312	0.02%	0.002%
80	12.098	3435	3439	3443	rBV2	406	372	0.02%	0.003%
81	12.239	3479	3483	3489	rVB3	636	731	0.05%	0.006%
82	12.268	3489	3492	3496	rBV3	570	538	0.03%	0.004%
83	12.316	3502	3507	3511	rBV4	595	600	0.04%	0.005%
84	12.342	3511	3515	3518	rVV3	438	305	0.02%	0.002%
85	12.442	3541	3546	3550	rBV3	371	333	0.02%	0.003%
86	12.480	3556	3558	3560	rBV2	432	213	0.01%	0.002%
87	12.609	3595	3598	3600	rBV2	346	204	0.01%	0.002%
88	12.786	3647	3653	3655	rBV2	570	528	0.03%	0.004%
89	12.889	3683	3685	3689	rVB3	389	265	0.02%	0.002%
90	12.985	3711	3715	3716	rBV2	316	256	0.02%	0.002%
91	13.053	3733	3736	3739	rVB2	502	312	0.02%	0.002%
92	13.078	3739	3744	3746	rBV3	462	416	0.03%	0.003%
93	13.101	3749	3751	3754	rBV2	312	206	0.01%	0.002%
94	13.252	3795	3798	3803	rBV5	421	411	0.03%	0.003%
95	13.339	3822	3825	3826	rBV2	434	248	0.02%	0.002%
96	13.432	3851	3854	3857	rBV4	577	335	0.02%	0.003%
97	13.612	3908	3910	3914	rVB4	449	289	0.02%	0.002%
98	13.734	3946	3948	3952	rVB3	734	298	0.02%	0.002%
99	13.908	3999	4002	4004	rBV2	690	477	0.03%	0.004%
100	14.290	4118	4121	4126	rBV4	795	747	0.05%	0.006%




Sum of corrected areas: 12771209

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029453.D
Acq On : 08 Dec 2022 05:44
Operator : SY/MD
Sample : N5919-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

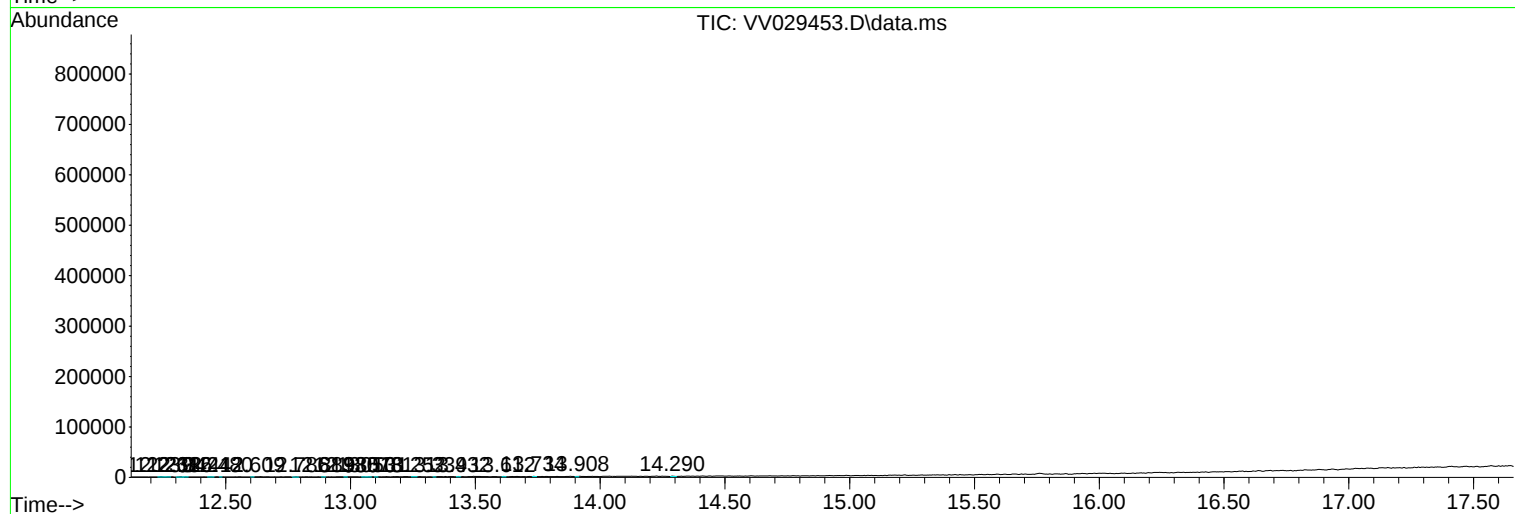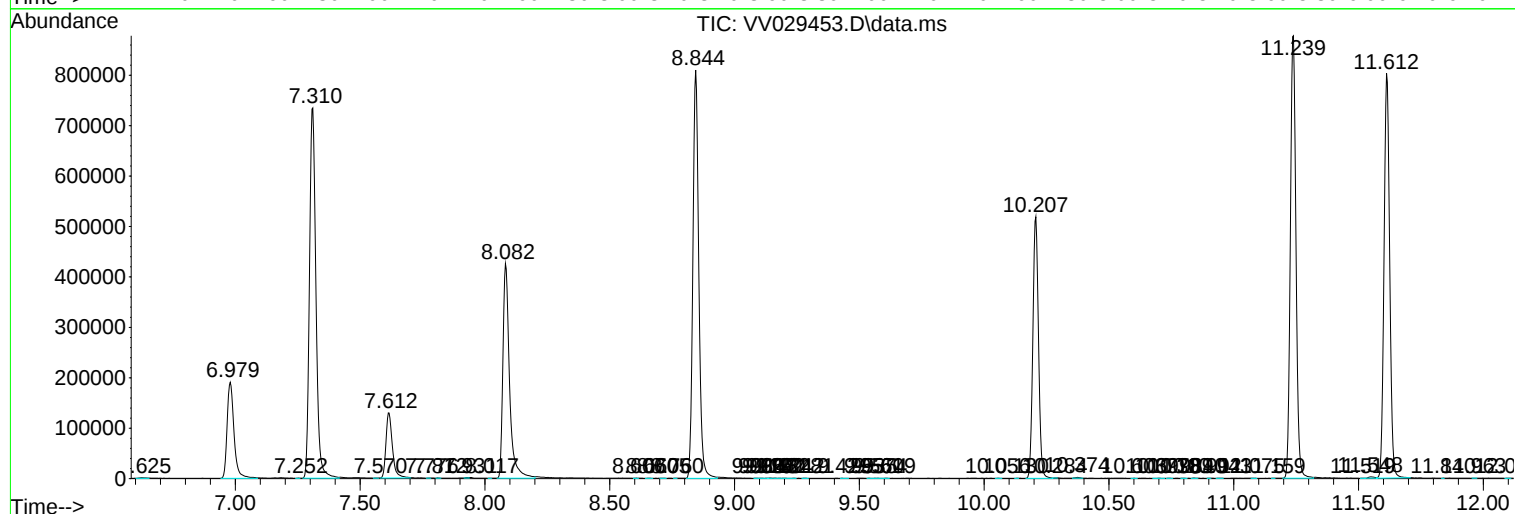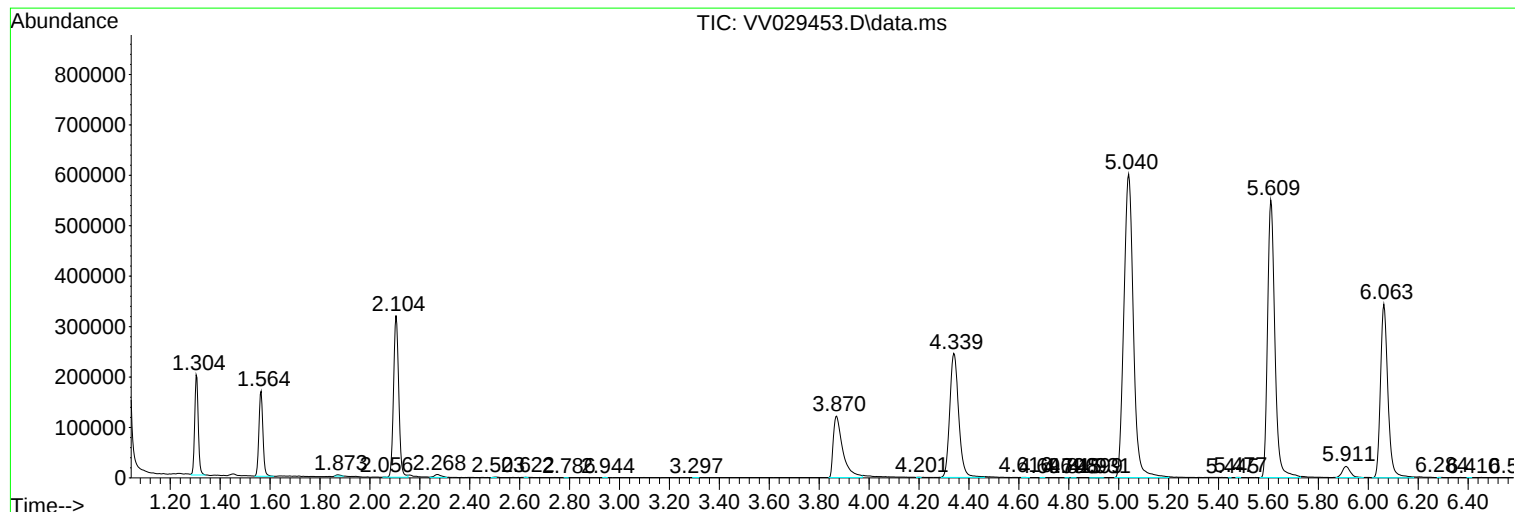

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029453.D
Acq On : 08 Dec 2022 05:44
Operator : SY/MD
Sample : N5919-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029453.D
Acq On : 08 Dec 2022 05:44
Operator : SY/MD
Sample : N5919-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc