

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029455.D
 Acq On : 08 Dec 2022 06:31
 Operator : SY/MD
 Sample : N5919-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029455.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	198454	195693	13.03%	1.624%
2	1.564	156	163	176	rVB	158570	177857	11.85%	1.476%
3	2.105	321	331	349	rBV	303615	436827	29.09%	3.626%
4	2.410	423	426	427	rBV	316	172	0.01%	0.001%
5	2.503	449	455	460	rVB5	811	1045	0.07%	0.009%
6	2.664	502	505	509	rVB	459	357	0.02%	0.003%
7	2.696	509	515	516	rBV	146	148	0.01%	0.001%
8	2.754	531	533	535	rBV	162	93	0.01%	0.001%
9	2.773	536	539	541	rVV2	199	138	0.01%	0.001%
10	2.815	549	552	555	rBV	165	130	0.01%	0.001%
11	2.838	555	559	564	rVB2	260	284	0.02%	0.002%
12	2.950	593	594	598	rVB	236	94	0.01%	0.001%
13	2.989	605	606	608	rVB2	266	80	0.01%	0.001%
14	3.031	615	619	627	rVB	230	240	0.02%	0.002%
15	3.069	629	631	632	rBV	146	62	0.00%	0.001%
16	3.146	653	655	658	rBV2	170	120	0.01%	0.001%
17	3.162	658	660	662	rVB	243	106	0.01%	0.001%
18	3.268	689	693	696	rBV2	290	211	0.01%	0.002%
19	3.394	729	732	735	rBV	153	101	0.01%	0.001%
20	3.519	768	771	775	rVB	214	138	0.01%	0.001%
21	3.558	775	783	785	rBV2	198	212	0.01%	0.002%
22	3.584	785	791	793	rBV2	130	115	0.01%	0.001%
23	3.667	814	817	823	rBV	287	206	0.01%	0.002%
24	3.690	823	824	828	rBV2	147	65	0.00%	0.001%
25	3.770	847	849	854	rVB2	216	123	0.01%	0.001%
26	3.825	862	866	870	rBV	141	122	0.01%	0.001%
27	3.870	870	880	928	rBV	114992	318000	21.18%	2.639%
28	4.339	1010	1026	1054	rBV	232762	576556	38.40%	4.785%
29	4.706	1137	1140	1144	rBV2	275	271	0.02%	0.002%
30	4.731	1146	1148	1151	rVV2	129	75	0.00%	0.001%
31	4.776	1159	1162	1166	rVB	169	130	0.01%	0.001%
32	4.799	1166	1169	1172	rBV2	210	131	0.01%	0.001%
33	4.821	1173	1176	1178	rBV2	149	71	0.00%	0.001%
34	4.899	1197	1200	1201	rBV	159	66	0.00%	0.001%
35	4.950	1213	1216	1217	rBV	137	67	0.00%	0.001%
36	4.976	1221	1224	1226	rBV	182	96	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120722\
 Data File : VW029455.D
 Acq On : 08 Dec 2022 06:31
 Operator : SY/MD
 Sample : N5919-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.040	1226	1244	1297	rBV2	567171	1501523	100.00%	12.463%
38	5.352	1339	1341	1345	rVB3	480	280	0.02%	0.002%
39	5.374	1346	1348	1350	rVB	280	97	0.01%	0.001%
40	5.477	1373	1380	1381	rBV2	422	392	0.03%	0.003%
41	5.510	1388	1390	1393	rVB2	255	113	0.01%	0.001%
42	5.538	1395	1399	1404	rBV	445	302	0.02%	0.003%
43	5.609	1408	1421	1466	rBV	513360	1054671	70.24%	8.754%
44	5.908	1501	1514	1533	rVB5	17726	39142	2.61%	0.325%
45	6.063	1547	1562	1586	rBV	329199	669974	44.62%	5.561%
46	6.300	1632	1636	1640	rVB4	308	279	0.02%	0.002%
47	6.320	1640	1642	1644	rBV	364	188	0.01%	0.002%
48	6.333	1644	1646	1647	rVB	195	49	0.00%	0.000%
49	6.378	1658	1660	1664	rBV	214	103	0.01%	0.001%
50	6.400	1664	1667	1670	rBV3	272	225	0.01%	0.002%
51	6.464	1682	1687	1688	rBV2	206	157	0.01%	0.001%
52	6.503	1694	1699	1701	rBV	261	188	0.01%	0.002%
53	6.519	1703	1704	1705	rVV	187	58	0.00%	0.000%
54	6.538	1708	1710	1714	rVB2	197	150	0.01%	0.001%
55	6.574	1719	1721	1723	rVB	215	89	0.01%	0.001%
56	6.593	1723	1727	1729	rBV	230	208	0.01%	0.002%
57	6.622	1729	1736	1737	rBV3	1079	1022	0.07%	0.008%
58	6.657	1745	1747	1752	rVB4	416	256	0.02%	0.002%
59	6.809	1789	1794	1799	rVB3	516	579	0.04%	0.005%
60	6.844	1799	1805	1807	rBV	330	389	0.03%	0.003%
61	6.921	1827	1829	1832	rBV2	277	177	0.01%	0.001%
62	6.979	1836	1847	1877	rBV	185695	336944	22.44%	2.797%
63	7.243	1927	1929	1930	rBV	293	119	0.01%	0.001%
64	7.310	1937	1950	1983	rBV	703241	1251555	83.35%	10.388%
65	7.612	2034	2044	2074	rBV	125392	221163	14.73%	1.836%
66	8.046	2176	2179	2180	rBV2	301	131	0.01%	0.001%
67	8.082	2180	2190	2229	rBV	414011	755526	50.32%	6.271%
68	8.718	2386	2388	2391	rBV2	165	111	0.01%	0.001%
69	8.747	2395	2397	2398	rBV	323	119	0.01%	0.001%
70	8.802	2412	2414	2415	rBV	246	92	0.01%	0.001%
71	8.844	2415	2427	2461	rBV	751115	1231861	82.04%	10.224%
72	9.127	2513	2515	2517	rBV3	389	229	0.02%	0.002%
73	9.188	2526	2534	2536	rBV4	334	430	0.03%	0.004%
74	9.252	2549	2554	2558	rBV2	579	577	0.04%	0.005%
75	9.304	2567	2570	2572	rBV	182	102	0.01%	0.001%
76	9.378	2590	2593	2596	rBV	238	168	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029455.D
 Acq On : 08 Dec 2022 06:31
 Operator : SY/MD
 Sample : N5919-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.406	2599	2602	2604	rVV2	388	258	0.02%	0.002%
78	9.429	2607	2609	2612	rVV2	224	121	0.01%	0.001%
79	9.464	2616	2620	2625	rVV3	434	347	0.02%	0.003%
80	9.564	2648	2651	2652	rBV3	304	139	0.01%	0.001%
81	9.609	2661	2665	2667	rBV2	208	156	0.01%	0.001%
82	9.677	2681	2686	2689	rBV3	263	280	0.02%	0.002%
83	9.776	2714	2717	2718	rBV	239	118	0.01%	0.001%
84	9.841	2735	2737	2740	rBV2	257	118	0.01%	0.001%
85	9.892	2750	2753	2755	rBV2	310	198	0.01%	0.002%
86	9.934	2762	2766	2769	rVB3	380	302	0.02%	0.003%
87	9.953	2769	2772	2774	rBV	150	80	0.01%	0.001%
88	9.992	2782	2784	2785	rBV	127	51	0.00%	0.000%
89	10.114	2820	2822	2828	rVB3	278	156	0.01%	0.001%
90	10.207	2839	2851	2877	rBV	496599	779373	51.91%	6.469%
91	10.339	2888	2892	2894	rVB3	317	243	0.02%	0.002%
92	10.374	2894	2903	2909	rBV5	1277	2055	0.14%	0.017%
93	10.632	2978	2983	2986	rBV2	410	405	0.03%	0.003%
94	10.722	3008	3011	3017	rBV2	230	227	0.02%	0.002%
95	10.956	3081	3084	3088	rBV2	387	360	0.02%	0.003%
96	11.027	3104	3106	3109	rVB	242	97	0.01%	0.001%
97	11.049	3109	3113	3117	rBV2	334	307	0.02%	0.003%
98	11.130	3136	3138	3142	rVB2	387	273	0.02%	0.002%
99	11.239	3160	3172	3197	rBV	821867	1277608	85.09%	10.604%
100	11.612	3276	3288	3305	rBV	763831	1204972	80.25%	10.001%




Sum of corrected areas: 12048184

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029455.D
Acq On : 08 Dec 2022 06:31
Operator : SY/MD
Sample : N5919-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

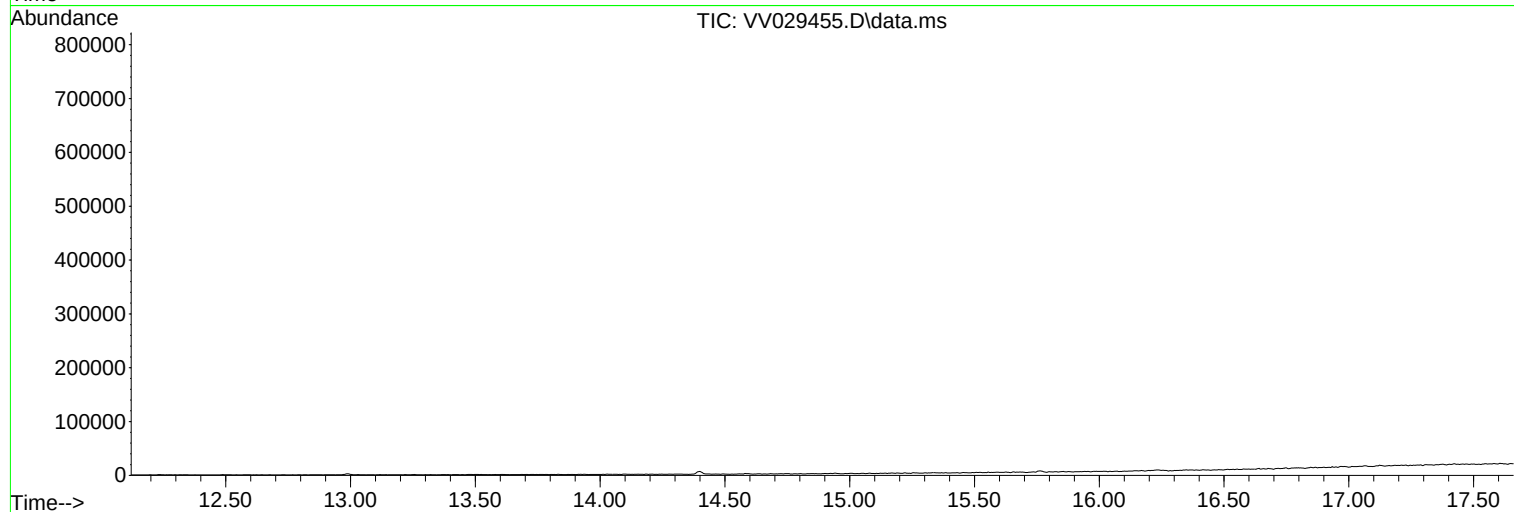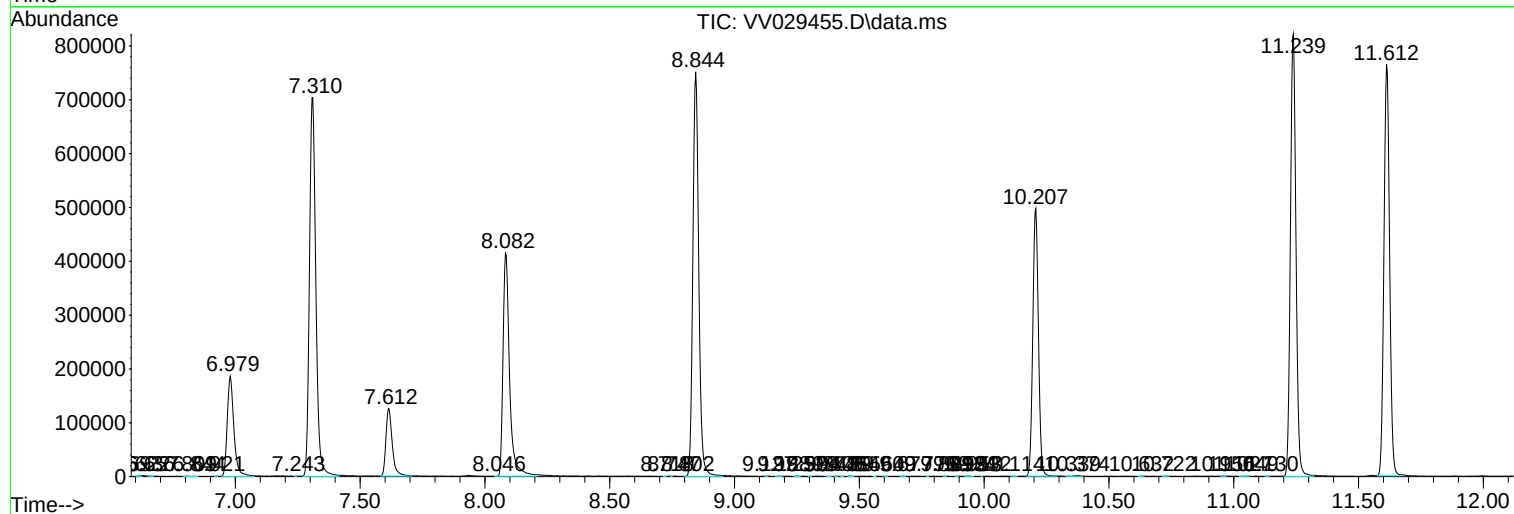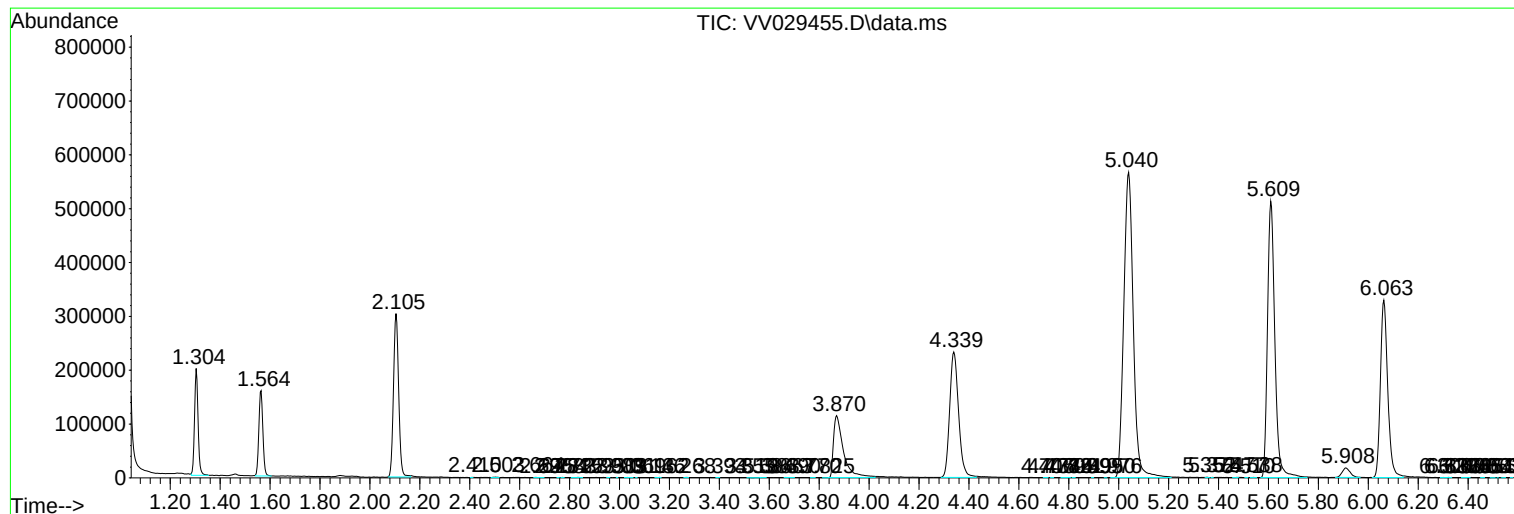

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029455.D
Acq On : 08 Dec 2022 06:31
Operator : SY/MD
Sample : N5919-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029455.D
Acq On : 08 Dec 2022 06:31
Operator : SY/MD
Sample : N5919-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc