

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029456.D
 Acq On : 08 Dec 2022 06:54
 Operator : SY/MD
 Sample : N5920-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029456.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	197729	198283	12.66%	1.543%
2	1.564	155	163	179	rVB	164819	187728	11.99%	1.461%
3	1.995	293	297	299	rBV3	301	271	0.02%	0.002%
4	2.008	299	301	307	rVB4	562	426	0.03%	0.003%
5	2.105	320	331	356	rBV2	340966	524999	33.52%	4.086%
6	2.497	449	453	463	rVB2	866	1222	0.08%	0.010%
7	2.551	467	470	477	rVB2	356	277	0.02%	0.002%
8	2.625	483	493	498	rBV3	1089	1832	0.12%	0.014%
9	2.815	550	552	560	rVB3	276	260	0.02%	0.002%
10	2.950	592	594	603	rVB4	353	490	0.03%	0.004%
11	3.169	658	662	663	rBV	352	269	0.02%	0.002%
12	3.182	663	666	669	rBV4	448	390	0.02%	0.003%
13	3.619	797	802	808	rVB2	308	344	0.02%	0.003%
14	3.719	828	833	839	rVB	217	257	0.02%	0.002%
15	3.870	866	880	914	rBV	124220	393857	25.15%	3.066%
16	4.178	971	976	979	rBV2	395	331	0.02%	0.003%
17	4.339	1009	1026	1063	rBV	242464	609118	38.89%	4.741%
18	4.561	1092	1095	1097	rBV3	363	248	0.02%	0.002%
19	4.600	1097	1107	1124	rVB6	5664	13233	0.84%	0.103%
20	4.754	1149	1155	1156	rBV	368	273	0.02%	0.002%
21	4.960	1214	1219	1222	rBV	293	275	0.02%	0.002%
22	5.040	1225	1244	1274	rBV2	597141	1566126	100.00%	12.190%
23	5.368	1343	1346	1348	rBV2	371	224	0.01%	0.002%
24	5.407	1355	1358	1360	rVB3	351	228	0.01%	0.002%
25	5.423	1360	1363	1366	rBV3	481	373	0.02%	0.003%
26	5.461	1370	1375	1378	rBV3	550	563	0.04%	0.004%
27	5.497	1383	1386	1392	rVB2	485	417	0.03%	0.003%
28	5.567	1402	1408	1409	rBV3	540	518	0.03%	0.004%
29	5.609	1409	1421	1460	rBV	546654	1119400	71.48%	8.713%
30	5.770	1469	1471	1475	rVB3	526	311	0.02%	0.002%
31	5.908	1499	1514	1529	rBV6	11145	25920	1.66%	0.202%
32	6.063	1548	1562	1599	rVV	341724	708643	45.25%	5.516%
33	6.262	1622	1624	1628	rVB2	350	226	0.01%	0.002%
34	6.304	1633	1637	1640	rVB3	401	275	0.02%	0.002%
35	6.326	1640	1644	1650	rVB2	336	259	0.02%	0.002%
36	6.394	1659	1665	1670	rBV2	426	551	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120722\
 Data File : VW029456.D
 Acq On : 08 Dec 2022 06:54
 Operator : SY/MD
 Sample : N5920-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.532	1704	1708	1711	rBV	310	239	0.02%	0.002%
38	6.625	1728	1737	1743	rBV5	1167	2201	0.14%	0.017%
39	6.683	1753	1755	1759	rVB2	366	251	0.02%	0.002%
40	6.764	1778	1780	1785	rVB2	408	270	0.02%	0.002%
41	6.979	1834	1847	1877	rBV	193514	354843	22.66%	2.762%
42	7.201	1914	1916	1921	rVB3	476	347	0.02%	0.003%
43	7.307	1936	1949	1983	rBV	740414	1318568	84.19%	10.263%
44	7.612	2034	2044	2070	rBV	131769	231703	14.79%	1.803%
45	7.866	2120	2123	2127	rBV3	393	335	0.02%	0.003%
46	7.931	2137	2143	2146	rBV4	1381	1493	0.10%	0.012%
47	8.082	2179	2190	2234	rBV	436350	795855	50.82%	6.194%
48	8.281	2250	2252	2255	rBV3	382	285	0.02%	0.002%
49	8.513	2321	2324	2328	rBV3	246	247	0.02%	0.002%
50	8.683	2373	2377	2380	rBV2	376	314	0.02%	0.002%
51	8.741	2390	2395	2398	rBV4	471	485	0.03%	0.004%
52	8.844	2415	2427	2458	rVV	804099	1327134	84.74%	10.330%
53	9.107	2505	2509	2512	rVB2	335	231	0.01%	0.002%
54	9.124	2512	2514	2518	rVB2	455	321	0.02%	0.002%
55	9.149	2518	2522	2526	rBV3	507	475	0.03%	0.004%
56	9.345	2578	2583	2586	rBV	283	295	0.02%	0.002%
57	9.407	2598	2602	2604	rBV2	384	280	0.02%	0.002%
58	9.480	2621	2625	2629	rBV2	263	253	0.02%	0.002%
59	9.574	2648	2654	2658	rBV4	350	435	0.03%	0.003%
60	9.596	2658	2661	2665	rVB3	383	341	0.02%	0.003%
61	9.619	2665	2668	2673	rBV2	387	493	0.03%	0.004%
62	9.673	2682	2685	2690	rVB3	251	237	0.02%	0.002%
63	9.921	2758	2762	2766	rVB2	499	432	0.03%	0.003%
64	10.001	2781	2787	2790	rBV3	241	220	0.01%	0.002%
65	10.207	2838	2851	2880	rVV	517504	817751	52.21%	6.365%
66	10.352	2892	2896	2897	rBV	453	278	0.02%	0.002%
67	10.374	2899	2903	2912	rVB4	1504	1988	0.13%	0.015%
68	10.487	2936	2938	2942	rVB2	365	240	0.02%	0.002%
69	10.532	2950	2952	2956	rVB2	434	282	0.02%	0.002%
70	10.705	3002	3006	3007	rBV	290	215	0.01%	0.002%
71	10.783	3026	3030	3034	rBV3	357	404	0.03%	0.003%
72	10.889	3060	3063	3066	rBV3	322	261	0.02%	0.002%
73	10.937	3073	3078	3082	rBV3	313	308	0.02%	0.002%
74	11.037	3106	3109	3112	rVB2	273	218	0.01%	0.002%
75	11.069	3112	3119	3122	rBV2	474	602	0.04%	0.005%
76	11.168	3146	3150	3153	rBV2	467	374	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029456.D
 Acq On : 08 Dec 2022 06:54
 Operator : SY/MD
 Sample : N5920-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.181	3153	3154	3157	rVB2	507	230	0.01%	0.002%
78	11.239	3160	3172	3199	rBV	890105	1383478	88.34%	10.768%
79	11.406	3221	3224	3227	rVB2	398	232	0.01%	0.002%
80	11.551	3258	3269	3276	rBV7	3081	5556	0.35%	0.043%
81	11.612	3276	3288	3316	rVV	786153	1231430	78.63%	9.585%
82	11.799	3343	3346	3349	rBV3	460	335	0.02%	0.003%
83	11.908	3372	3380	3383	rBV4	463	579	0.04%	0.005%
84	11.934	3383	3388	3391	rVB2	374	379	0.02%	0.003%
85	12.046	3420	3423	3426	rVB2	408	288	0.02%	0.002%
86	12.239	3478	3483	3488	rVB4	580	732	0.05%	0.006%
87	12.291	3497	3499	3502	rVB2	360	218	0.01%	0.002%
88	12.529	3570	3573	3576	rBV2	374	224	0.01%	0.002%
89	12.664	3611	3615	3617	rBV4	444	253	0.02%	0.002%
90	12.757	3641	3644	3646	rBV2	358	241	0.02%	0.002%
91	12.789	3650	3654	3657	rBV3	289	247	0.02%	0.002%
92	12.860	3673	3676	3679	rBV2	255	240	0.02%	0.002%
93	12.998	3713	3719	3723	rBV4	472	470	0.03%	0.004%
94	13.066	3737	3740	3746	rBV3	352	330	0.02%	0.003%
95	13.278	3804	3806	3809	rBV	332	227	0.01%	0.002%
96	13.429	3850	3853	3856	rVB2	402	289	0.02%	0.002%
97	13.895	3995	3998	4001	rBV2	572	456	0.03%	0.004%
98	13.911	4001	4003	4007	rVB2	853	552	0.04%	0.004%
99	14.133	4069	4072	4073	rBV2	505	250	0.02%	0.002%
100	14.670	4235	4239	4241	rBV4	905	789	0.05%	0.006%




Sum of corrected areas: 12847946

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029456.D
Acq On : 08 Dec 2022 06:54
Operator : SY/MD
Sample : N5920-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EH8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

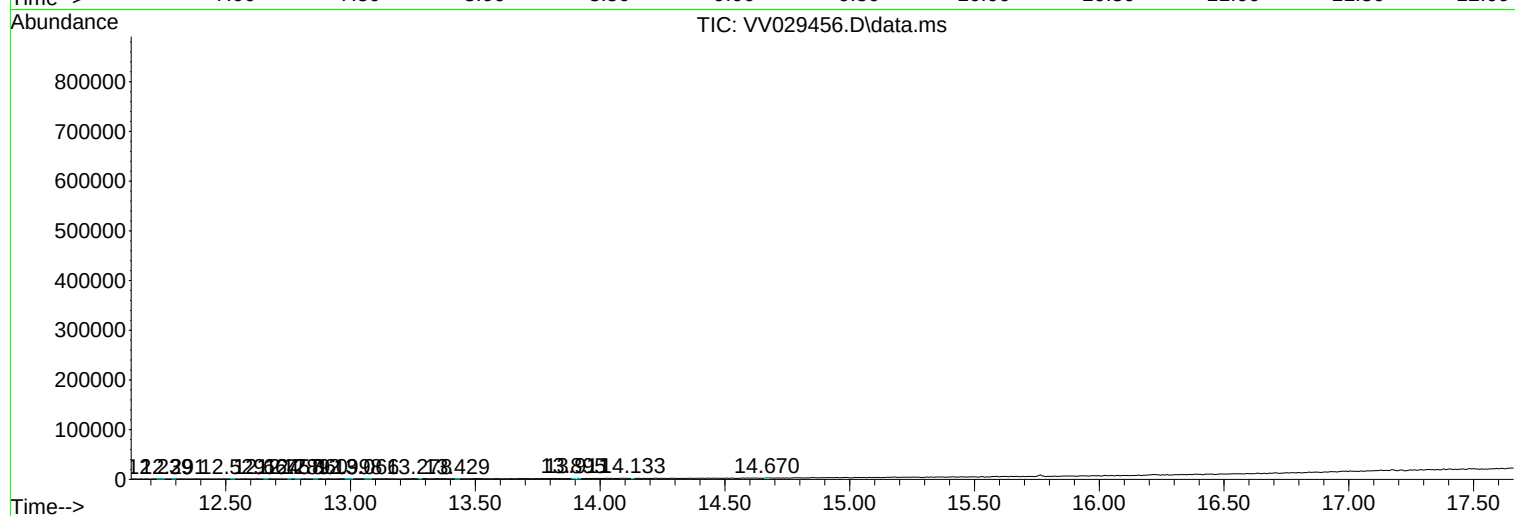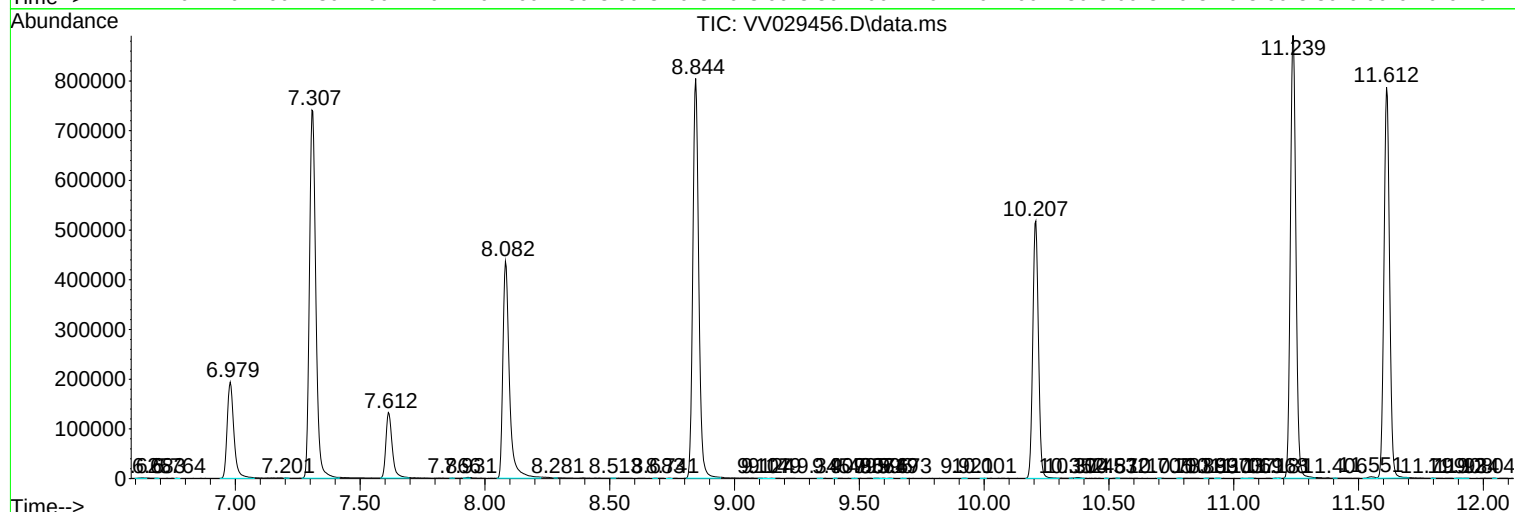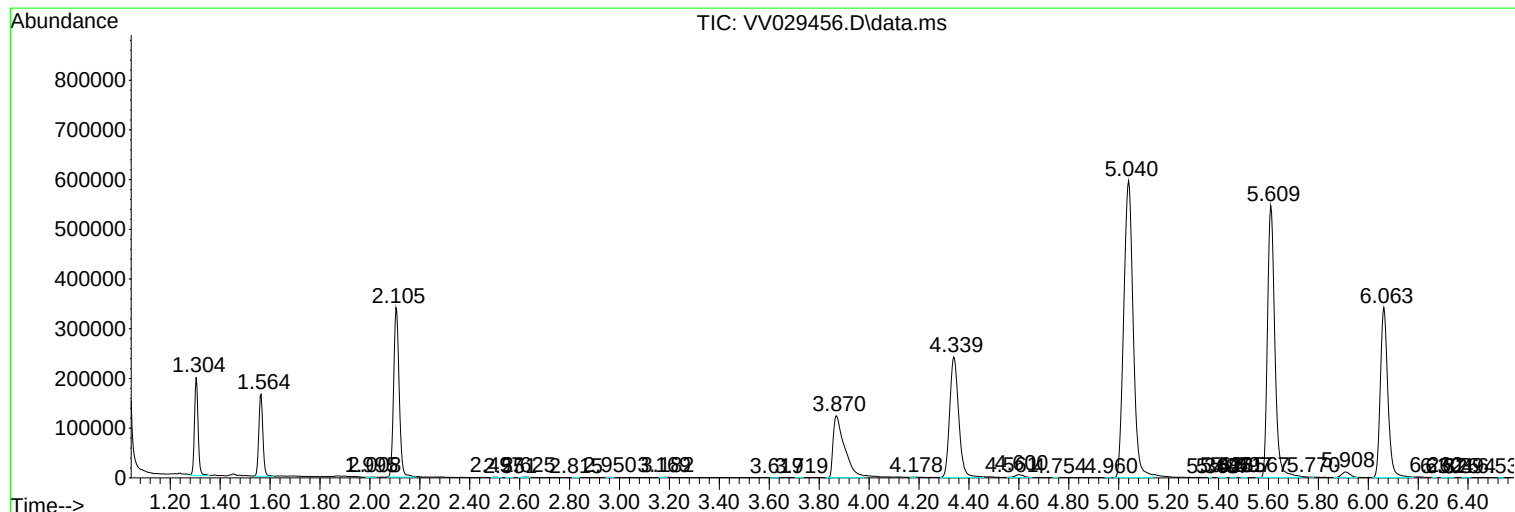

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029456.D
Acq On : 08 Dec 2022 06:54
Operator : SY/MD
Sample : N5920-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EH8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029456.D
Acq On : 08 Dec 2022 06:54
Operator : SY/MD
Sample : N5920-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EH8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------