

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029457.D
 Acq On : 08 Dec 2022 07:18
 Operator : SY/MD
 Sample : N5920-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	195363	196707	13.13%	1.609%
2	1.564	155	163	175	rVB	157717	176493	11.78%	1.443%
3	1.873	251	259	270	rBV2	4834	9020	0.60%	0.074%
4	1.982	291	293	297	rVB2	605	337	0.02%	0.003%
5	2.005	297	300	301	rBV2	601	332	0.02%	0.003%
6	2.105	320	331	344	rBV	307364	437719	29.23%	3.579%
7	2.272	375	383	403	rVB2	6505	13279	0.89%	0.109%
8	2.510	449	457	463	rVV6	940	1330	0.09%	0.011%
9	2.619	489	491	500	rVV3	387	574	0.04%	0.005%
10	2.728	521	525	528	rBV2	262	210	0.01%	0.002%
11	3.127	646	649	653	rVB3	374	255	0.02%	0.002%
12	3.153	653	657	662	rVB2	274	266	0.02%	0.002%
13	3.439	742	746	749	rBV2	428	317	0.02%	0.003%
14	3.584	787	791	795	rVB2	351	278	0.02%	0.002%
15	3.834	862	869	870	rBV2	302	307	0.02%	0.003%
16	3.866	870	879	911	rBV	114339	307114	20.51%	2.511%
17	4.214	985	987	994	rVB4	629	510	0.03%	0.004%
18	4.339	1009	1026	1060	rBV	232471	577637	38.57%	4.724%
19	4.555	1091	1093	1098	rVB2	336	259	0.02%	0.002%
20	4.654	1120	1124	1128	rVB4	317	233	0.02%	0.002%
21	4.844	1178	1183	1190	rBV2	258	248	0.02%	0.002%
22	4.969	1218	1222	1226	rVB2	342	274	0.02%	0.002%
23	5.040	1226	1244	1276	rBV2	565441	1497749	100.00%	12.248%
24	5.252	1307	1310	1313	rBV2	268	204	0.01%	0.002%
25	5.394	1352	1354	1363	rVB5	390	322	0.02%	0.003%
26	5.609	1408	1421	1464	rBV	535913	1089783	72.76%	8.912%
27	5.911	1501	1515	1535	rVB4	18739	41897	2.80%	0.343%
28	5.998	1538	1542	1547	rBV3	297	249	0.02%	0.002%
29	6.063	1547	1562	1598	rBV	324269	671465	44.83%	5.491%
30	6.362	1652	1655	1662	rVV3	169	219	0.01%	0.002%
31	6.426	1669	1675	1680	rVB2	201	207	0.01%	0.002%
32	6.606	1724	1731	1732	rBV2	480	402	0.03%	0.003%
33	6.632	1732	1739	1744	rVV4	755	1248	0.08%	0.010%
34	6.677	1751	1753	1758	rVB2	430	328	0.02%	0.003%
35	6.828	1798	1800	1804	rVB3	368	212	0.01%	0.002%
36	6.979	1836	1847	1877	rBV	183572	338304	22.59%	2.766%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029457.D
 Acq On : 08 Dec 2022 07:18
 Operator : SY/MD
 Sample : N5920-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.233	1922	1926	1928	rVB2	468	328	0.02%	0.003%
38	7.259	1929	1934	1936	rBV3	435	297	0.02%	0.002%
39	7.310	1936	1950	1987	rBV	703986	1259144	84.07%	10.296%
40	7.616	2034	2045	2071	rBV	124900	220143	14.70%	1.800%
41	7.757	2086	2089	2094	rVV3	517	415	0.03%	0.003%
42	7.831	2108	2112	2116	rBV3	505	472	0.03%	0.004%
43	7.931	2138	2143	2152	rVB4	1600	2263	0.15%	0.019%
44	8.014	2165	2169	2172	rVB2	410	336	0.02%	0.003%
45	8.082	2179	2190	2229	rBV	409778	746570	49.85%	6.105%
46	8.387	2283	2285	2288	rVB2	357	226	0.02%	0.002%
47	8.529	2327	2329	2332	rBV	353	254	0.02%	0.002%
48	8.577	2340	2344	2347	rBV3	420	321	0.02%	0.003%
49	8.844	2415	2427	2464	rBV	781723	1291587	86.24%	10.562%
50	9.001	2474	2476	2481	rBV3	433	246	0.02%	0.002%
51	9.050	2489	2491	2497	rVB2	493	432	0.03%	0.004%
52	9.162	2523	2526	2532	rVB3	372	276	0.02%	0.002%
53	9.204	2536	2539	2545	rVB4	353	360	0.02%	0.003%
54	9.239	2545	2550	2554	rBV	349	471	0.03%	0.004%
55	9.268	2554	2559	2564	rVB2	349	376	0.03%	0.003%
56	9.400	2592	2600	2604	rBV3	434	673	0.04%	0.006%
57	9.468	2617	2621	2623	rVB2	353	245	0.02%	0.002%
58	9.487	2623	2627	2629	rBV2	274	222	0.01%	0.002%
59	9.535	2638	2642	2643	rBV	534	351	0.02%	0.003%
60	9.574	2651	2654	2660	rVB3	347	342	0.02%	0.003%
61	9.667	2677	2683	2685	rBV2	213	217	0.01%	0.002%
62	9.705	2692	2695	2699	rVB2	298	229	0.02%	0.002%
63	9.889	2748	2752	2757	rBV3	238	229	0.02%	0.002%
64	9.963	2770	2775	2778	rBV2	272	237	0.02%	0.002%
65	10.072	2805	2809	2812	rVB2	312	273	0.02%	0.002%
66	10.120	2820	2824	2828	rVB3	303	334	0.02%	0.003%
67	10.146	2828	2832	2834	rBV	332	262	0.02%	0.002%
68	10.207	2838	2851	2872	rBV	499531	773697	51.66%	6.327%
69	10.374	2893	2903	2909	rBV5	1686	2895	0.19%	0.024%
70	10.596	2968	2972	2976	rBV4	413	374	0.02%	0.003%
71	10.660	2986	2992	2995	rBV2	340	282	0.02%	0.002%
72	10.866	3051	3056	3060	rBV2	289	298	0.02%	0.002%
73	10.914	3068	3071	3076	rVB3	379	380	0.03%	0.003%
74	10.947	3077	3081	3086	rVB3	320	285	0.02%	0.002%
75	11.094	3125	3127	3132	rVB4	307	245	0.02%	0.002%
76	11.123	3132	3136	3137	rBV2	348	237	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029457.D
 Acq On : 08 Dec 2022 07:18
 Operator : SY/MD
 Sample : N5920-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.239	3159	3172	3193	rBV	862405	1327800	88.65%	10.858%
78	11.490	3246	3250	3254	rVB3	385	288	0.02%	0.002%
79	11.551	3262	3269	3275	rBV6	2294	3657	0.24%	0.030%
80	11.612	3276	3288	3308	rVV	791503	1216576	81.23%	9.948%
81	11.834	3352	3357	3361	rBV3	390	388	0.03%	0.003%
82	11.956	3388	3395	3398	rBV3	402	533	0.04%	0.004%
83	12.040	3416	3421	3424	rVB4	279	255	0.02%	0.002%
84	12.082	3431	3434	3438	rBV	322	247	0.02%	0.002%
85	12.188	3464	3467	3470	rVB3	324	199	0.01%	0.002%
86	12.352	3514	3518	3524	rVB3	383	395	0.03%	0.003%
87	12.429	3539	3542	3544	rBV3	400	249	0.02%	0.002%
88	12.638	3603	3607	3609	rBV2	559	378	0.03%	0.003%
89	12.770	3646	3648	3654	rBV3	287	207	0.01%	0.002%
90	12.821	3660	3664	3667	rVB3	411	312	0.02%	0.003%
91	12.882	3680	3683	3685	rVB2	368	230	0.02%	0.002%
92	12.927	3691	3697	3699	rBV3	432	410	0.03%	0.003%
93	12.947	3700	3703	3706	rVV3	370	240	0.02%	0.002%
94	13.072	3739	3742	3745	rBV2	400	266	0.02%	0.002%
95	13.249	3794	3797	3801	rBV4	820	699	0.05%	0.006%
96	13.438	3854	3856	3859	rBV2	375	287	0.02%	0.002%
97	13.628	3913	3915	3918	rBV	493	308	0.02%	0.003%
98	13.670	3924	3928	3933	rBV5	706	645	0.04%	0.005%
99	13.834	3977	3979	3981	rBV2	520	250	0.02%	0.002%
100	14.001	4026	4031	4034	rBV3	898	942	0.06%	0.008%




Sum of corrected areas: 12228873

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029457.D
Acq On : 08 Dec 2022 07:18
Operator : SY/MD
Sample : N5920-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

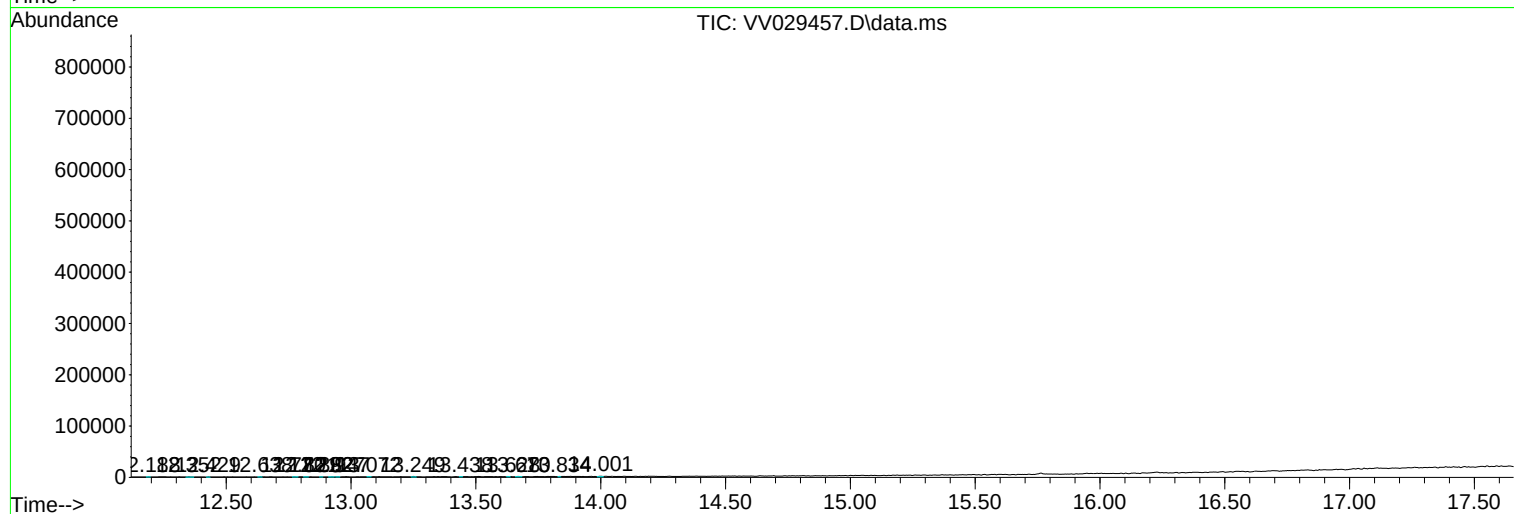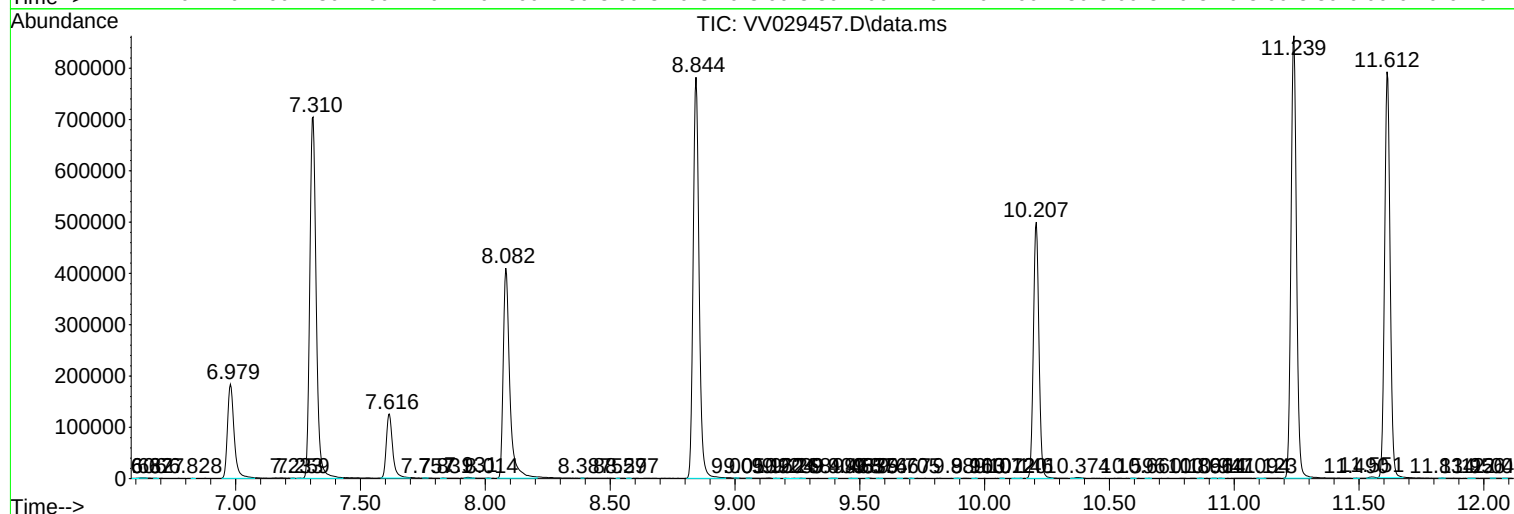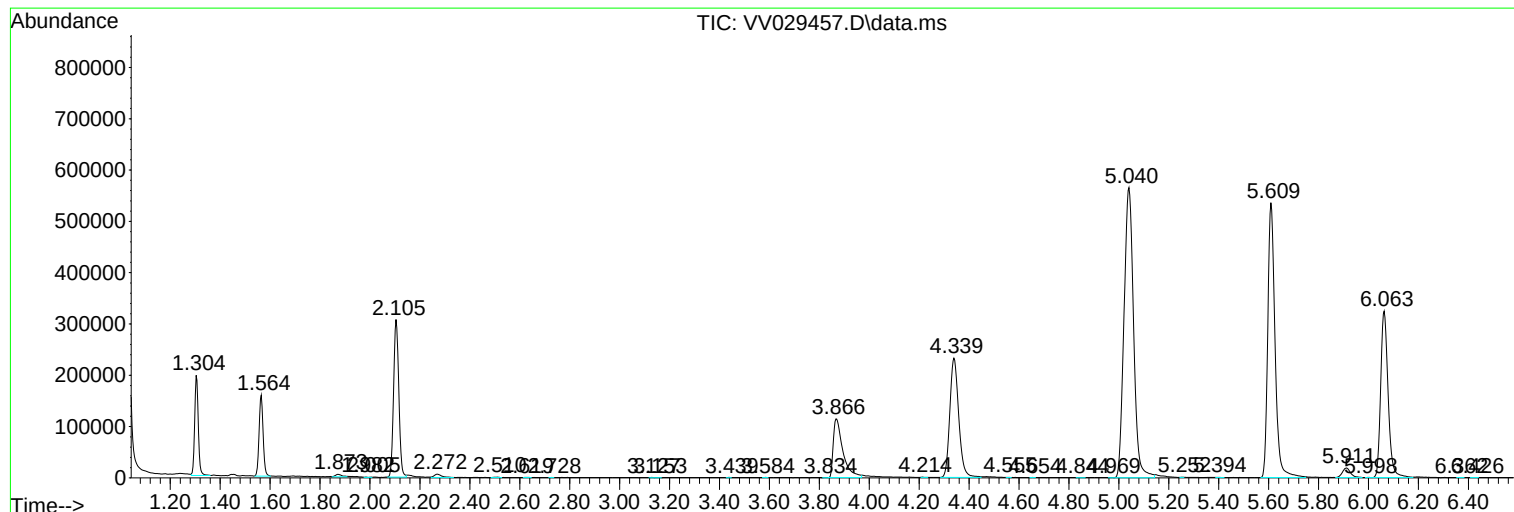

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029457.D
Acq On : 08 Dec 2022 07:18
Operator : SY/MD
Sample : N5920-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029457.D
Acq On : 08 Dec 2022 07:18
Operator : SY/MD
Sample : N5920-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------