


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029409.D
Acq On : 07 Dec 2022 10:59
Operator : SY/MD
Sample : BFB351
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB351

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Title : VOC Analysis
Last Update : Thu Dec 08 01:48:46 2022

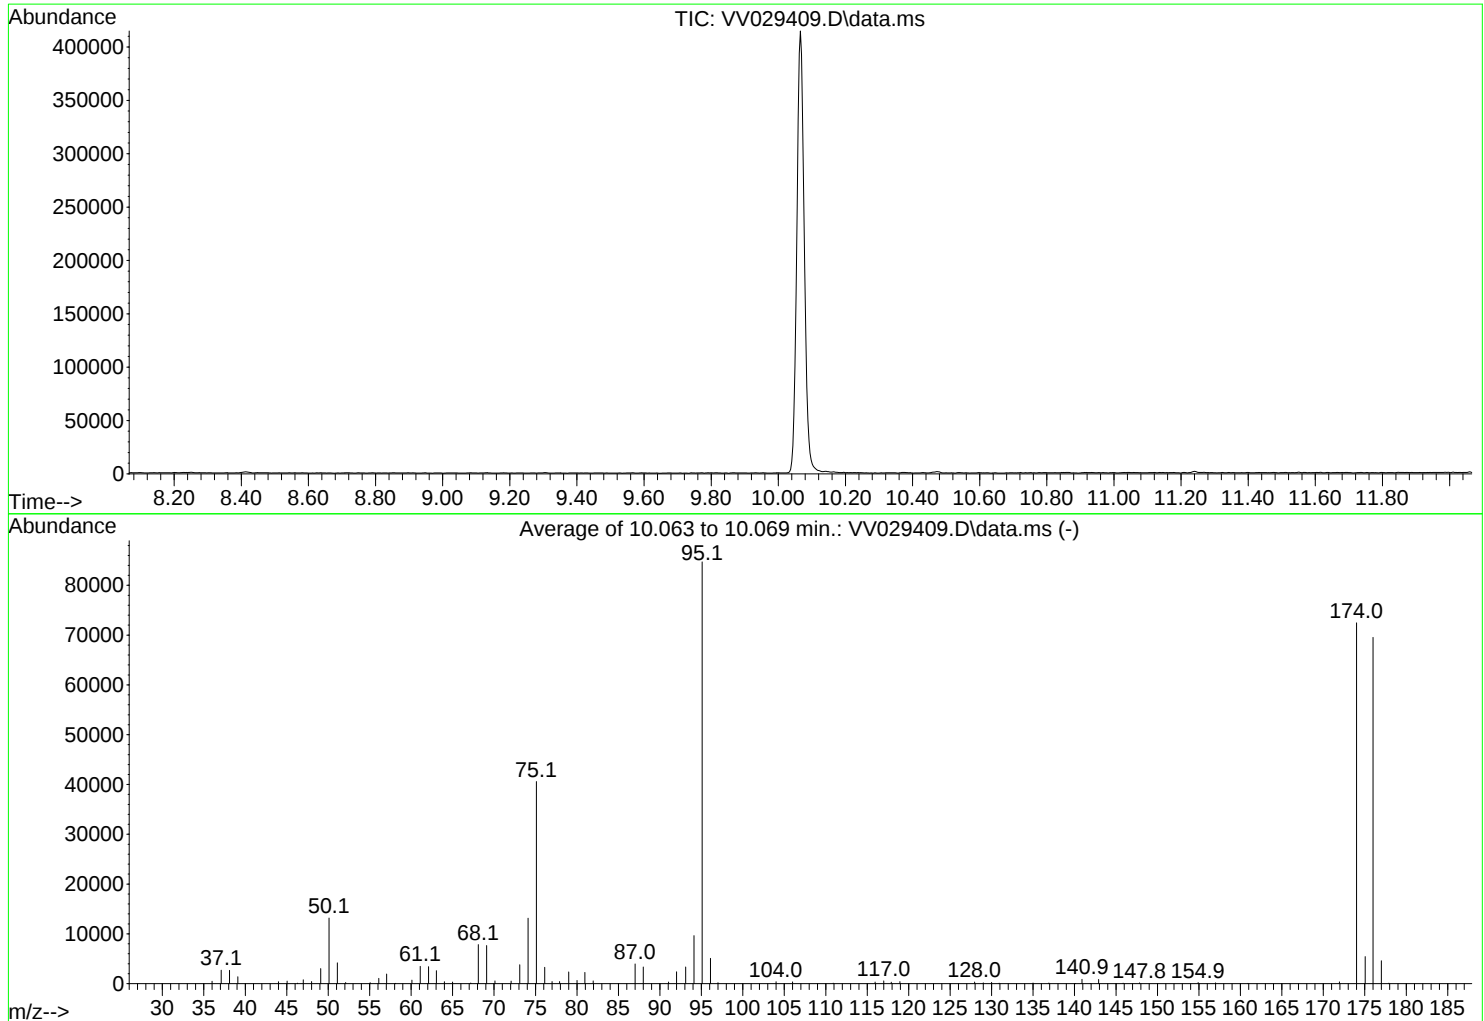

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	13194	PASS
75	95	30	80	47.9	40595	PASS
95	95	100	100	100.0	84715	PASS
96	95	5	9	6.0	5066	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.6	72480	PASS
175	174	5	9	7.5	5433	PASS
176	174	95	105	95.9	69544	PASS
177	176	5	10	6.6	4613	PASS

m/z	Abundance
40.00	302.0
44.10	445.0
76.90	133.0
206.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351

m/z	Abundance
36.00	480.0
37.10	2729.0
38.10	2568.0
39.10	1329.0
40.10	268.0
44.00	804.0
45.10	513.0
46.30	145.0
47.00	781.0
48.00	513.0
49.10	2923.0
50.10	13428.0
51.10	4343.0
52.10	260.0
55.10	181.0
56.10	1063.0
57.10	1973.0
60.10	750.0
61.10	3455.0
62.10	3449.0
63.10	2608.0
64.00	372.0
65.00	279.0
68.10	7753.0
69.10	7888.0
70.10	596.0
72.10	579.0
73.10	3882.0
74.10	13145.0
75.10	40192.0
76.10	3344.0
77.00	570.0
77.90	431.0
79.00	2330.0
80.00	631.0
80.90	2225.0
82.00	539.0
87.00	3713.0
88.00	3519.0
91.10	275.0
92.00	2424.0
93.10	3245.0
94.10	9643.0
95.10	83544.0
96.10	5185.0
97.00	206.0
104.00	361.0
106.00	306.0
110.90	117.0
116.00	344.0
117.00	521.0
117.90	317.0
119.00	416.0
128.00	284.0
129.00	124.0
130.00	286.0
130.90	109.0
135.00	117.0
136.90	145.0
140.90	823.0
141.90	129.0
142.90	852.0
145.80	122.0
147.90	162.0
154.90	195.0
157.00	139.0
160.90	126.0
172.00	311.0
174.00	69408.0
175.10	5428.0
176.00	67144.0
177.00	4658.0
177.90	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351

m/z	Abundance
36.00	507.0
37.10	2801.0
38.10	2791.0
39.10	1462.0
40.00	256.0
44.00	839.0
45.10	529.0
46.30	123.0
47.00	749.0
48.00	436.0
49.10	3132.0
50.10	13631.0
51.10	4316.0
52.10	251.0
55.10	180.0
56.10	1098.0
57.10	1995.0
58.10	102.0
60.10	713.0
61.10	3581.0
62.10	3561.0
63.00	2691.0
64.00	385.0
65.00	332.0
68.10	8182.0
69.10	7935.0
70.10	576.0
72.10	516.0
73.10	3930.0
74.10	13657.0
75.10	42072.0
76.10	3367.0
77.10	573.0
77.90	424.0
79.00	2429.0
80.00	667.0
81.00	2314.0
82.00	579.0
87.00	4106.0
88.00	3452.0
91.10	331.0
92.00	2413.0
93.10	3453.0
94.10	10016.0
95.10	87760.0
96.10	5176.0
97.00	208.0
104.00	382.0
106.00	355.0
110.90	120.0
115.90	341.0
117.00	556.0
117.90	310.0
118.90	424.0
127.90	320.0
129.00	164.0
130.00	280.0
130.90	114.0
135.00	141.0
136.90	148.0
140.90	906.0
142.90	878.0
145.80	118.0
147.90	157.0
154.90	219.0
157.00	160.0
160.90	111.0
171.90	382.0
174.00	75216.0
175.10	5602.0
176.00	72064.0
177.00	4713.0
177.90	105.0
206.90	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351

m/z	Abundance
36.00	465.0
37.10	2599.0
38.10	2624.0
39.10	1318.0
40.00	245.0
44.00	813.0
45.00	522.0
47.00	769.0
48.00	346.0
49.10	2973.0
50.10	12524.0
51.10	3842.0
52.10	209.0
55.00	203.0
56.10	1024.0
57.00	1824.0
58.10	111.0
60.10	633.0
61.10	3410.0
62.10	3251.0
63.00	2510.0
64.00	385.0
65.00	334.0
67.20	379.0
68.10	7581.0
69.10	7092.0
70.10	488.0
72.00	417.0
73.10	3535.0
74.10	12593.0
75.10	39520.0
76.10	3096.0
77.00	562.0
77.90	361.0
79.00	2255.0
80.00	654.0
81.00	2169.0
81.90	549.0
87.00	4037.0
88.00	3105.0
91.00	342.0
92.00	2258.0
93.10	3311.0
94.10	9252.0
95.10	82840.0
96.10	4837.0
97.00	175.0
104.00	389.0
106.00	375.0
110.90	106.0
115.90	275.0
117.00	524.0
117.90	278.0
118.90	419.0
127.90	320.0
129.00	181.0
130.00	235.0
130.90	108.0
135.00	159.0
136.90	127.0
140.10	103.0
140.90	878.0
142.90	814.0
145.00	102.0
145.90	104.0
147.80	155.0
154.90	226.0
157.00	174.0
172.00	396.0
174.00	72816.0
175.00	5269.0
176.00	69424.0
177.00	4467.0
206.90	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB351