

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033140.D
 Acq On : 07 Dec 2023 12:43
 Operator : SY/MD
 Sample : 05645-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 08 01:37:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 01:34:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	297691	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	293645	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	153995	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	62425	35.078	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	70.160%
7) Chloroethane-d5	1.532	69	49417	39.854	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.700%
11) 1,1-Dichloroethene-d2	2.060	65	26335	38.899	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.800%
21) 2-Butanone-d5	3.783	46	85378	96.593	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.590%
24) Chloroform-d	4.249	84	160569	42.516	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.040%
26) 1,2-Dichloroethane-d4	4.940	65	106962	45.554	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.100%
32) Benzene-d6	4.960	84	290716	42.331	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.660%
36) 1,2-Dichloropropane-d6	5.989	67	81605	44.193	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.380%
41) Toluene-d8	7.243	98	267389	40.814	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.620%
43) trans-1,3-Dichloroprop...	7.554	79	45521	38.985	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.960%
47) 2-Hexanone-d5	8.024	63	69436	93.601	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.600%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	120858	46.042	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.080%
66) 1,2-Dichlorobenzene-d4	11.561	152	129723	47.345	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.700%
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	11.185	75	14715	7.663	ug/L	# 61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033140.D
Acq On : 07 Dec 2023 12:43
Operator : SY/MD
Sample : 05645-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 08 01:37:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 01:34:57 2023
Response via : Initial Calibration

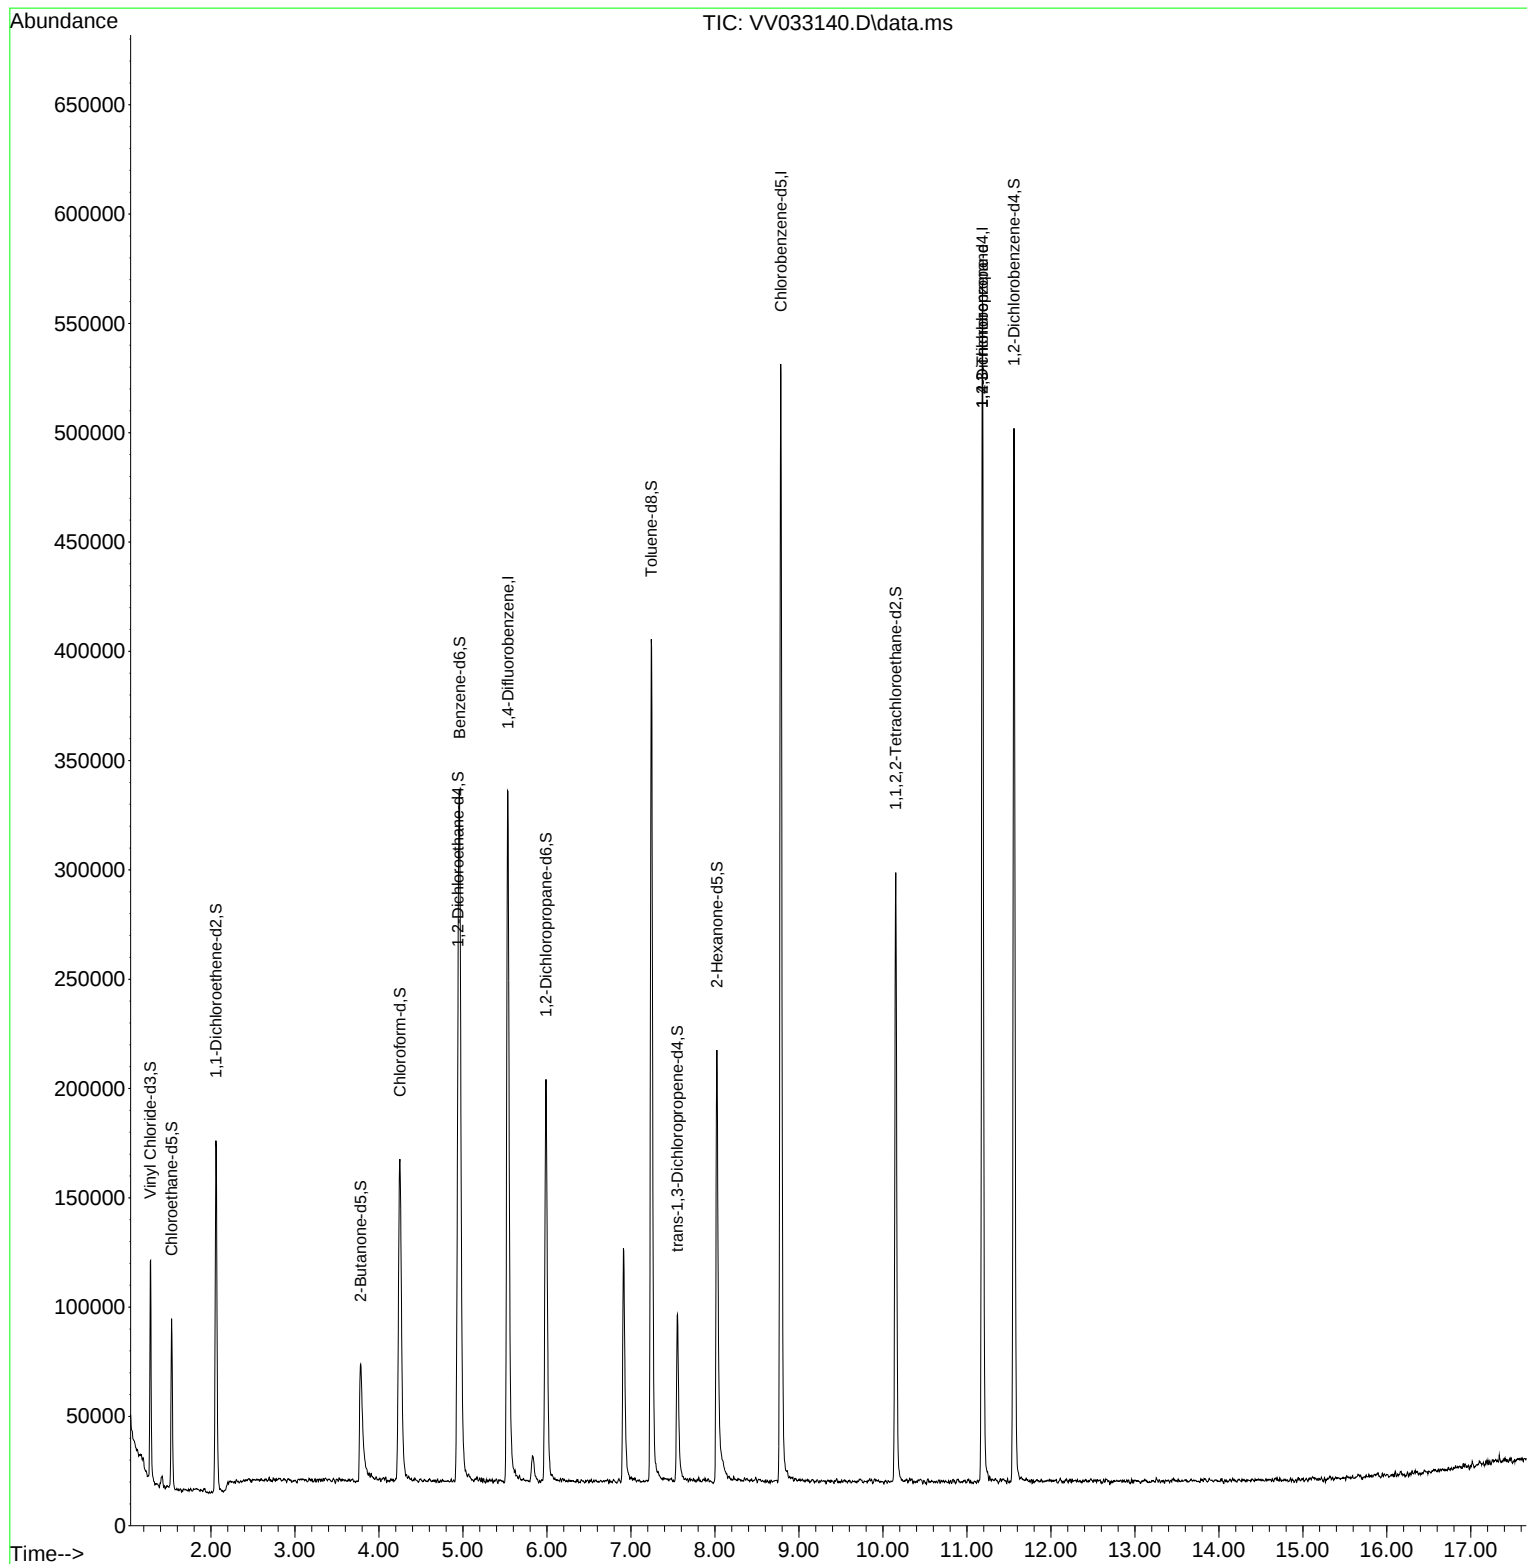

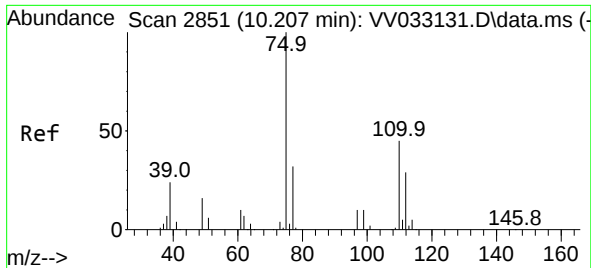

#61
1,2,3-Trichloropropane
Concen: 7.663 ug/L
RT: 11.185 min Scan# 31
Delta R.T. 0.977 min
Lab File: VV033140.D
Acq: 07 Dec 2023 12:43

Instrument :
MSVOA_V
ClientSampleId :

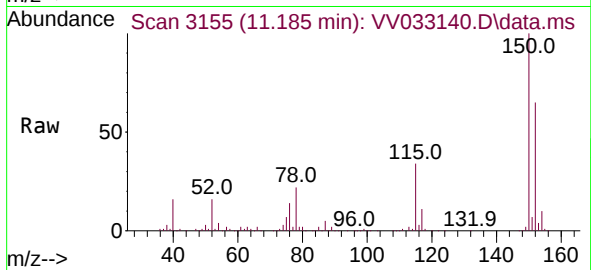

Tgt Ion	Ratio	Lower	Upper
75	100		
77	35.9	27.0	40.6
110	4.3	38.1	57.1#

