

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033138.D
 Acq On : 07 Dec 2023 11:57
 Operator : SY/MD
 Sample : 05645-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G38

Quant Time: Dec 08 01:37:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 01:34:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	295051	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	289580	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	148108	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	61599	34.924	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	69.840%
7) Chloroethane-d5	1.532	69	48396	39.379	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	78.760%
11) 1,1-Dichloroethene-d2	2.060	65	25207	37.566	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.140%
21) 2-Butanone-d5	3.783	46	75191	85.829	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.830%
24) Chloroform-d	4.249	84	155173	41.455	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.920%
26) 1,2-Dichloroethane-d4	4.941	65	101096	43.441	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.880%
32) Benzene-d6	4.960	84	283297	41.830	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.660%
36) 1,2-Dichloropropane-d6	5.989	67	80872	44.411	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.820%
41) Toluene-d8	7.243	98	259964	40.238	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.480%
43) trans-1,3-Dichloroprop...	7.551	79	45591	39.593	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.180%
47) 2-Hexanone-d5	8.024	63	61550	84.136	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.140%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	113826	43.972	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.940%
66) 1,2-Dichlorobenzene-d4	11.561	152	124595	47.281	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.560%
Target Compounds						
					Qvalue	
13) Acetone	2.111	43	3307	3.954	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033138.D
Acq On : 07 Dec 2023 11:57
Operator : SY/MD
Sample : 05645-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G38

Quant Time: Dec 08 01:37:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 01:34:57 2023
Response via : Initial Calibration

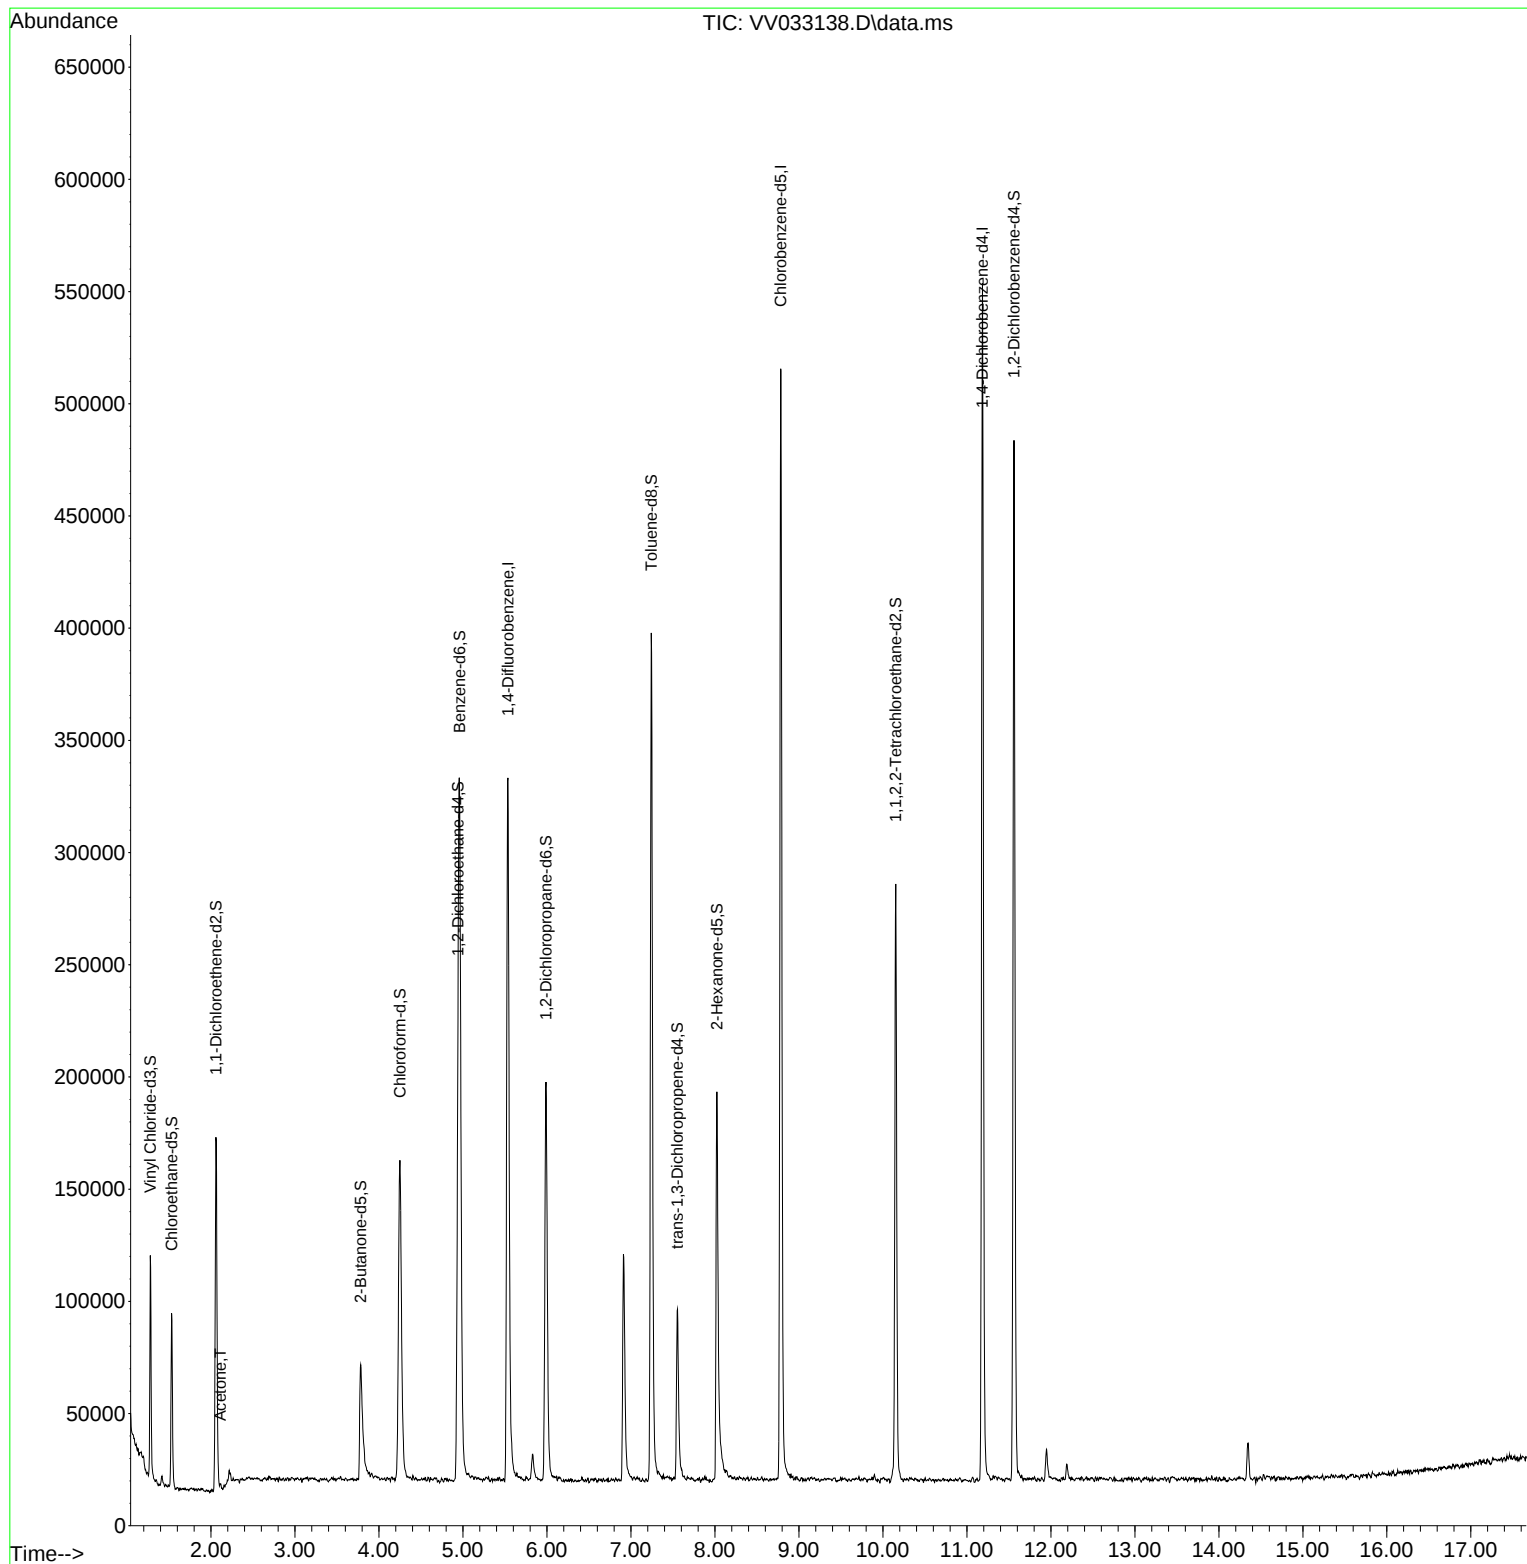

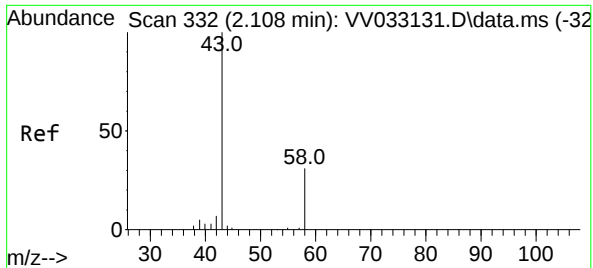

#13
 Acetone
 Concen: 3.954 ug/L
 RT: 2.111 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV033138.D
 Acq: 07 Dec 2023 11:57

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G38

Tgt Ion:	43	Resp:	3307
Ion	Ratio	Lower	Upper
43	100		
58	27.6	0.0	62.8

