

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033142.D
 Acq On : 07 Dec 2023 13:29
 Operator : SY/MD
 Sample : 05644-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G61

Quant Time: Dec 08 01:38:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 01:34:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	288271	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	287027	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	146610	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	58726	34.078	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	68.160%
7) Chloroethane-d5	1.532	69	45929	38.251	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	76.500%
11) 1,1-Dichloroethene-d2	2.060	65	24828	37.872	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.740%
21) 2-Butanone-d5	3.783	46	80134	93.623	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.620%
24) Chloroform-d	4.249	84	149089	40.767	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.540%
26) 1,2-Dichloroethane-d4	4.941	65	98970	43.527	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.060%
32) Benzene-d6	4.960	84	269790	40.190	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.380%
36) 1,2-Dichloropropane-d6	5.989	67	77358	42.859	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.720%
41) Toluene-d8	7.243	98	249844	39.015	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	78.040%#
43) trans-1,3-Dichloroprop...	7.555	79	42474	37.214	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.420%
47) 2-Hexanone-d5	8.024	63	65786	90.726	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.730%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	109979	42.863	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.720%
66) 1,2-Dichlorobenzene-d4	11.561	152	123117	47.198	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.400%
Target Compounds					Qvalue	
13) Acetone	2.118	43	3125	3.824	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033142.D
Acq On : 07 Dec 2023 13:29
Operator : SY/MD
Sample : 05644-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G61

Quant Time: Dec 08 01:38:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 01:34:57 2023
Response via : Initial Calibration

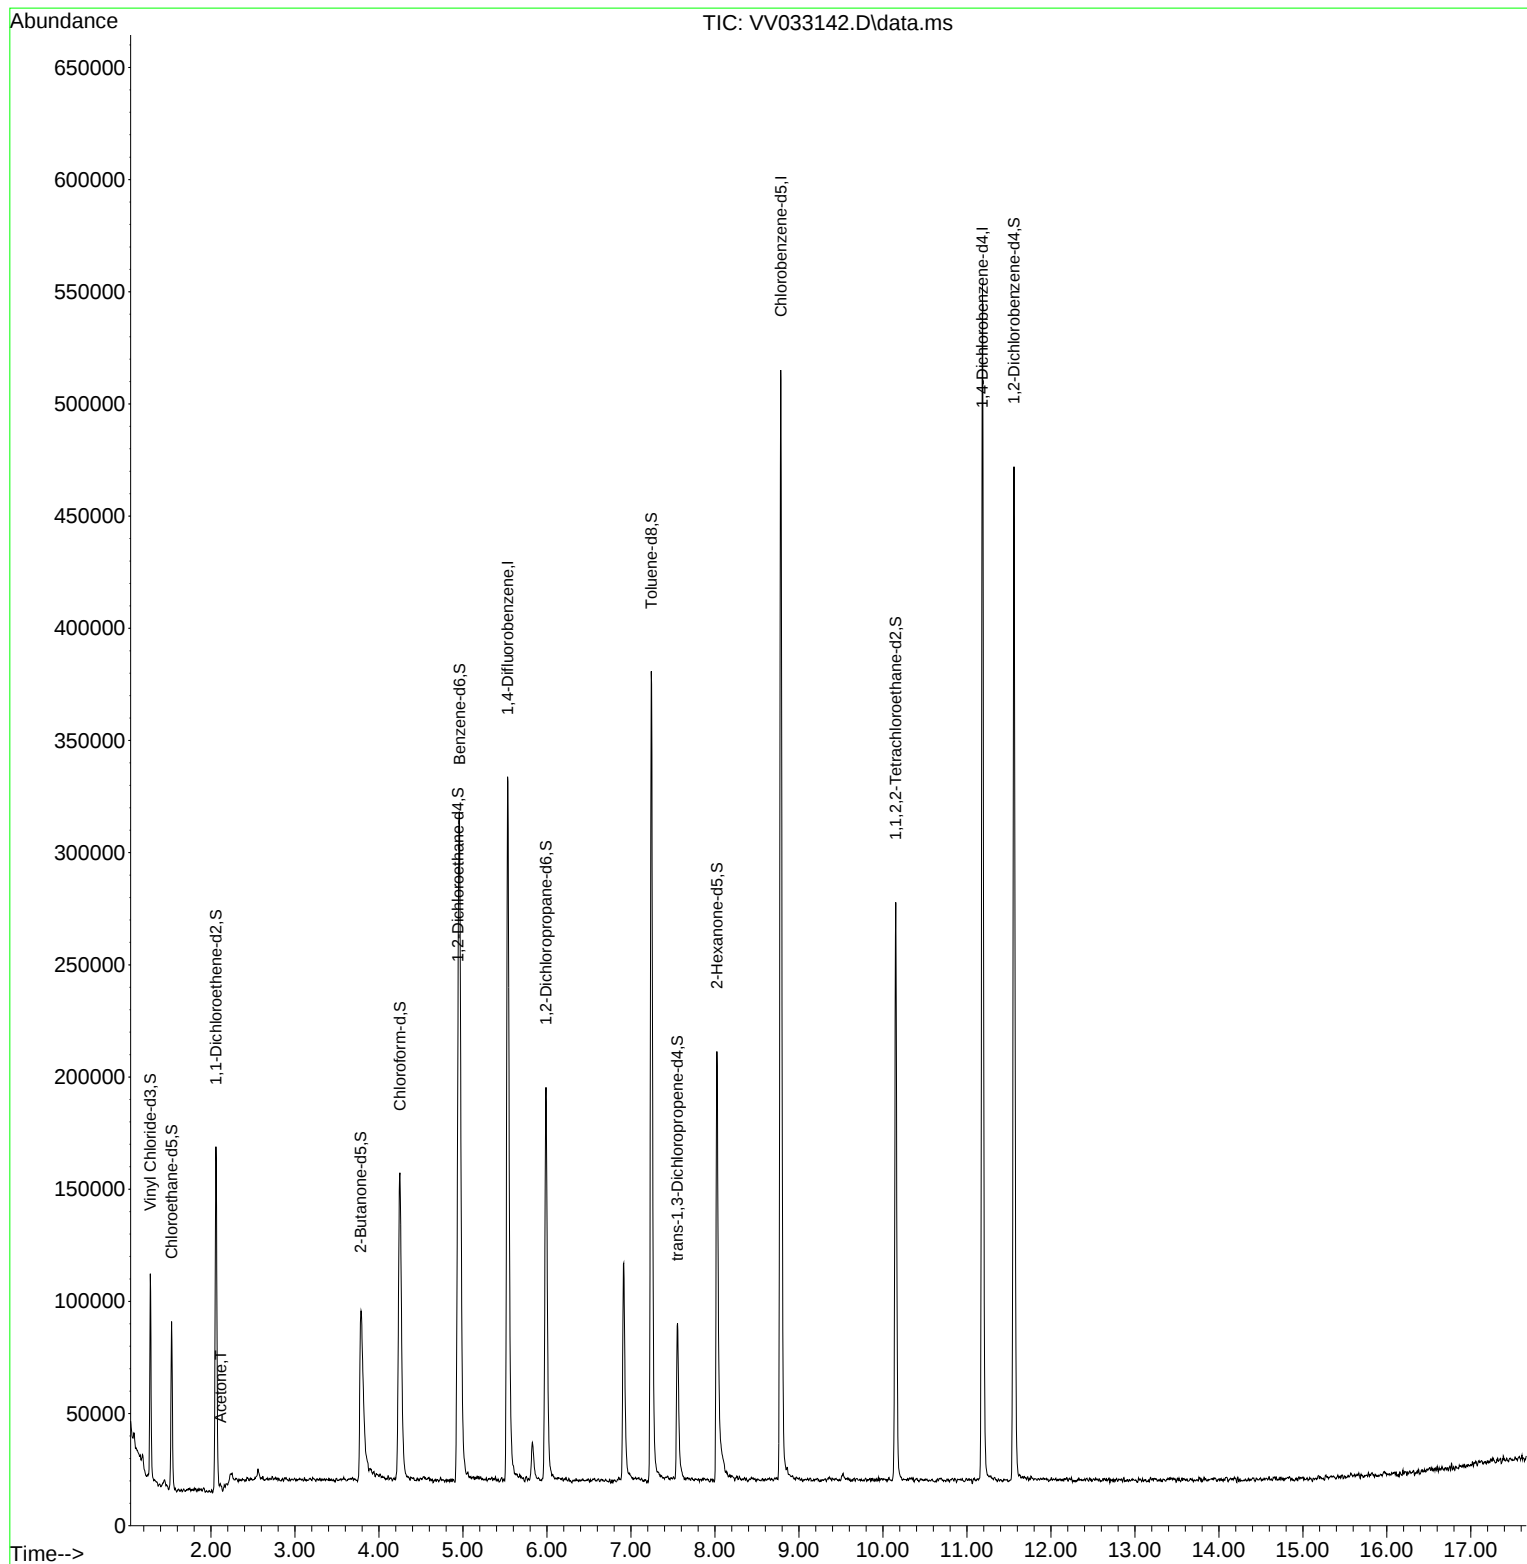

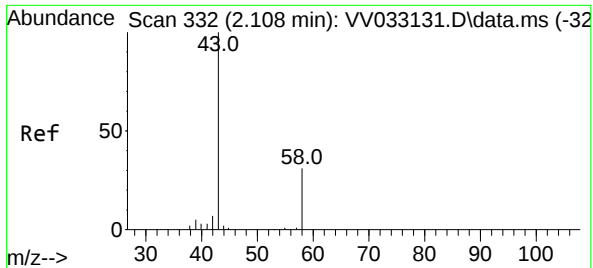

#13

Acetone

Concen: 3.824 ug/L

RT: 2.118 min Scan# 31

Delta R.T. 0.010 min

Lab File: VV033142.D

Acq: 07 Dec 2023 13:29

Instrument :

MSVOA_V

ClientSampleId :

C0G61

Tgt Ion: 43 Resp: 3125

Ion Ratio Lower Upper

43 100

58 30.6 0.0 62.8

