

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033144.D
 Acq On : 07 Dec 2023 14:16
 Operator : SY/MD
 Sample : 05673-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEJ1

Quant Time: Dec 08 01:38:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 01:34:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	299135	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	294338	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	155263	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	60403	33.778	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	67.560%		
7) Chloroethane-d5	1.532	69	48732	39.112	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	78.220%		
11) 1,1-Dichloroethene-d2	2.060	65	25129	36.939	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.880%		
21) 2-Butanone-d5	3.780	46	77221	86.943	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	86.940%		
24) Chloroform-d	4.249	84	157923	41.614	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.220%		
26) 1,2-Dichloroethane-d4	4.941	65	103342	43.799	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.600%		
32) Benzene-d6	4.960	84	285476	41.470	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.940%		
36) 1,2-Dichloropropane-d6	5.986	67	80175	43.316	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	86.640%		
41) Toluene-d8	7.243	98	263577	40.137	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	80.280%		
43) trans-1,3-Dichloroprop...	7.551	79	46931	40.098	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.200%		
47) 2-Hexanone-d5	8.021	63	63733	85.711	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	85.710%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	116040	44.102	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.200%		
66) 1,2-Dichlorobenzene-d4	11.561	152	129281	46.799	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.600%		
Target Compounds					Qvalue	
13) Acetone	2.111	43	3212	3.788	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033144.D
Acq On : 07 Dec 2023 14:16
Operator : SY/MD
Sample : 05673-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEJ1

Quant Time: Dec 08 01:38:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 01:34:57 2023
Response via : Initial Calibration

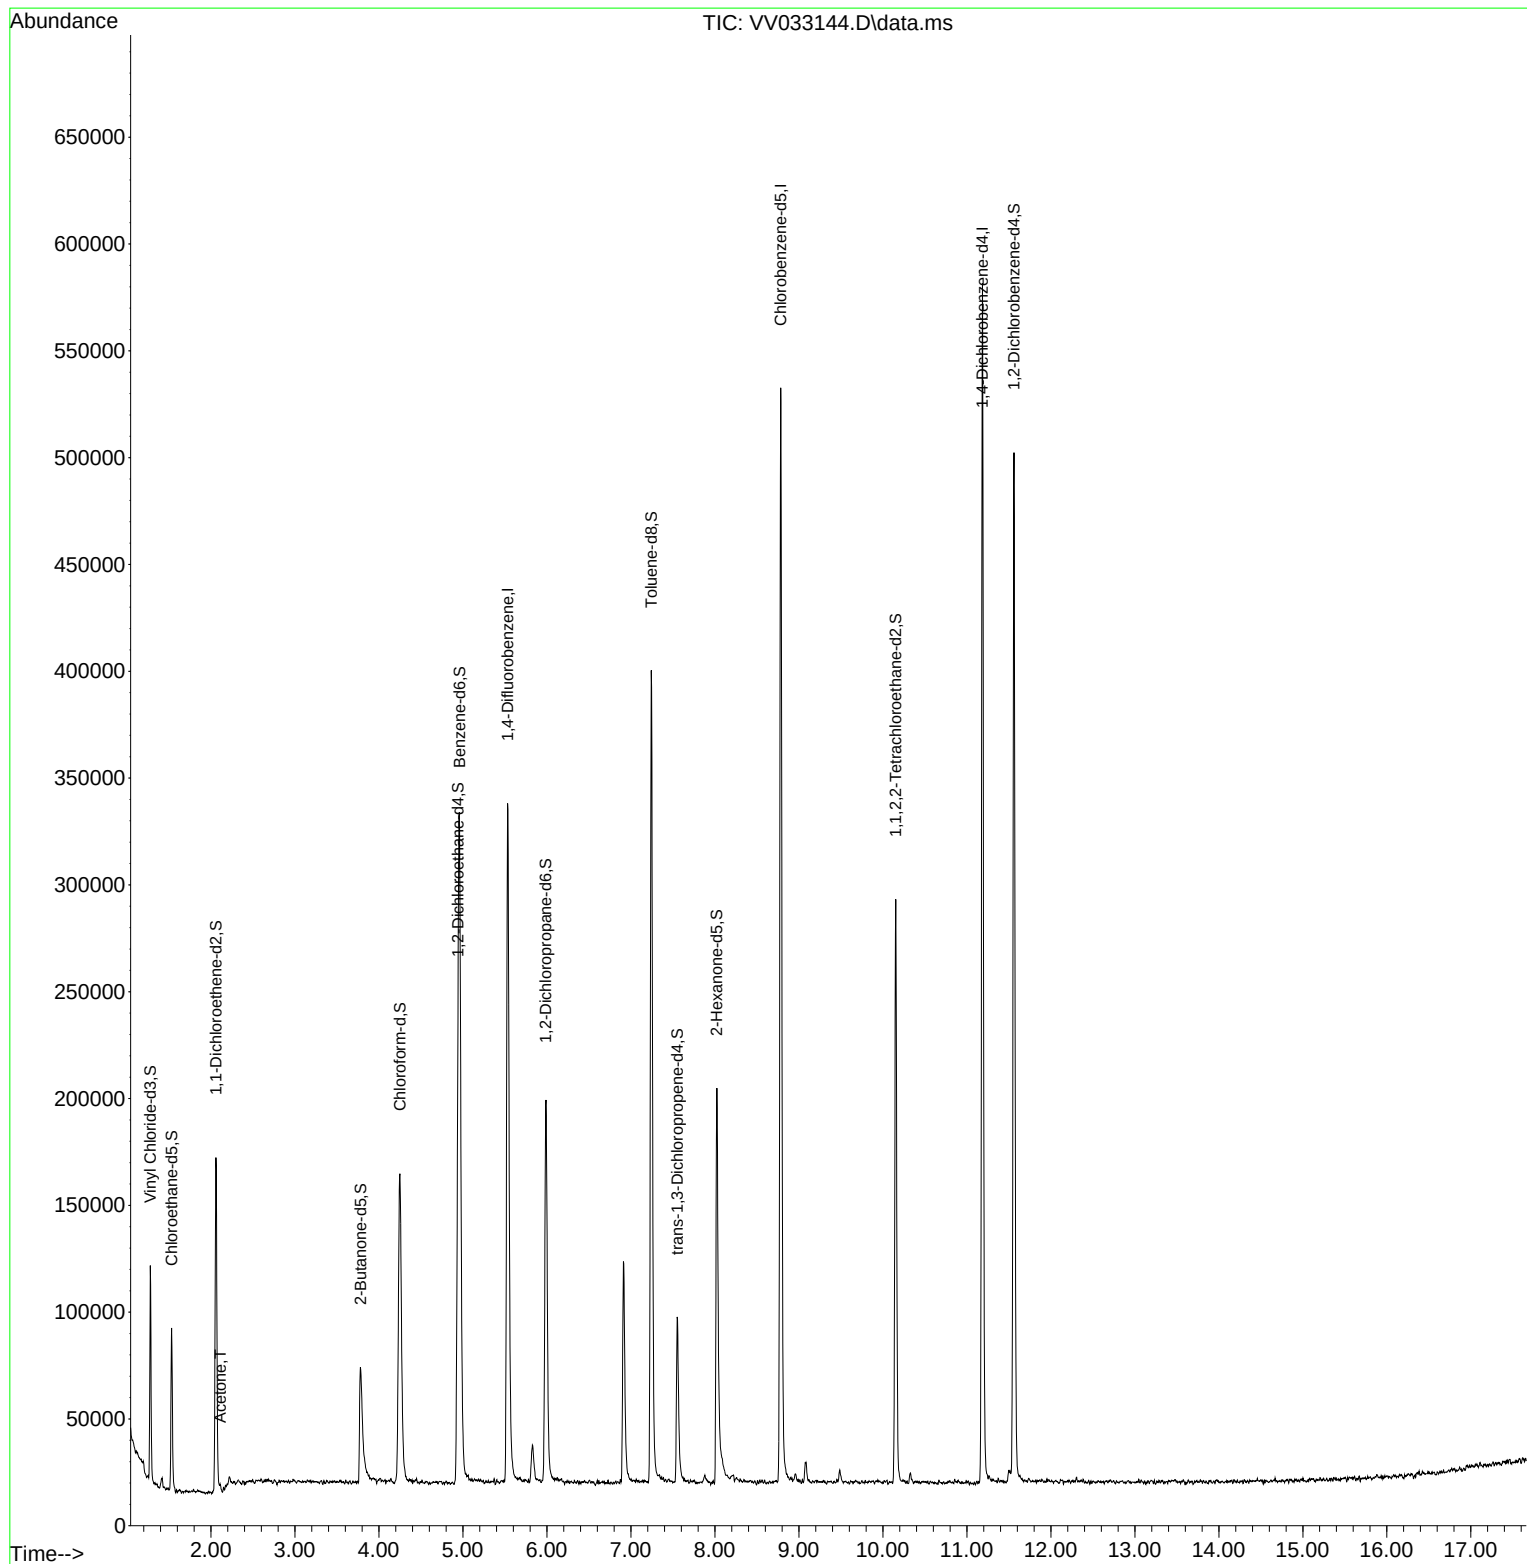

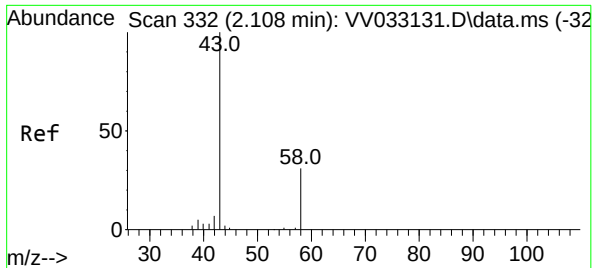

#13
 Acetone
 Concen: 3.788 ug/L
 RT: 2.111 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV033144.D
 Acq: 07 Dec 2023 14:16

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEJ1

Tgt Ion: 43 Resp: 3212
 Ion Ratio Lower Upper
 43 100
 58 34.2 0.0 62.8

