

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033166.D
 Acq On : 07 Dec 2023 23:10
 Operator : SY/MD
 Sample : 05689-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G85

Quant Time: Dec 08 04:18:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 04:15:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	276915	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	281620	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	144884	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	49192	29.716	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	59.440%#
7) Chloroethane-d5	1.532	69	40485	35.100	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	70.200%
11) 1,1-Dichloroethene-d2	2.060	65	21087	33.485	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.960%
21) 2-Butanone-d5	3.780	46	77989	94.854	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.850%
24) Chloroform-d	4.249	84	141326	40.229	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.460%
26) 1,2-Dichloroethane-d4	4.940	65	94956	43.475	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.940%
32) Benzene-d6	4.960	84	250409	38.019	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.040%
36) 1,2-Dichloropropane-d6	5.989	67	73605	41.563	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	83.120%
41) Toluene-d8	7.243	98	229528	36.531	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	73.060%#
43) trans-1,3-Dichloroprop...	7.554	79	41304	36.884	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.760%
47) 2-Hexanone-d5	8.024	63	65464	92.015	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.020%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	113496	45.083	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.160%
66) 1,2-Dichlorobenzene-d4	11.561	152	120057	46.573	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.140%
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.066	96	2763	1.990	ug/L #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033166.D
Acq On : 07 Dec 2023 23:10
Operator : SY/MD
Sample : 05689-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G85

Quant Time: Dec 08 04:18:12 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 04:15:58 2023
Response via : Initial Calibration

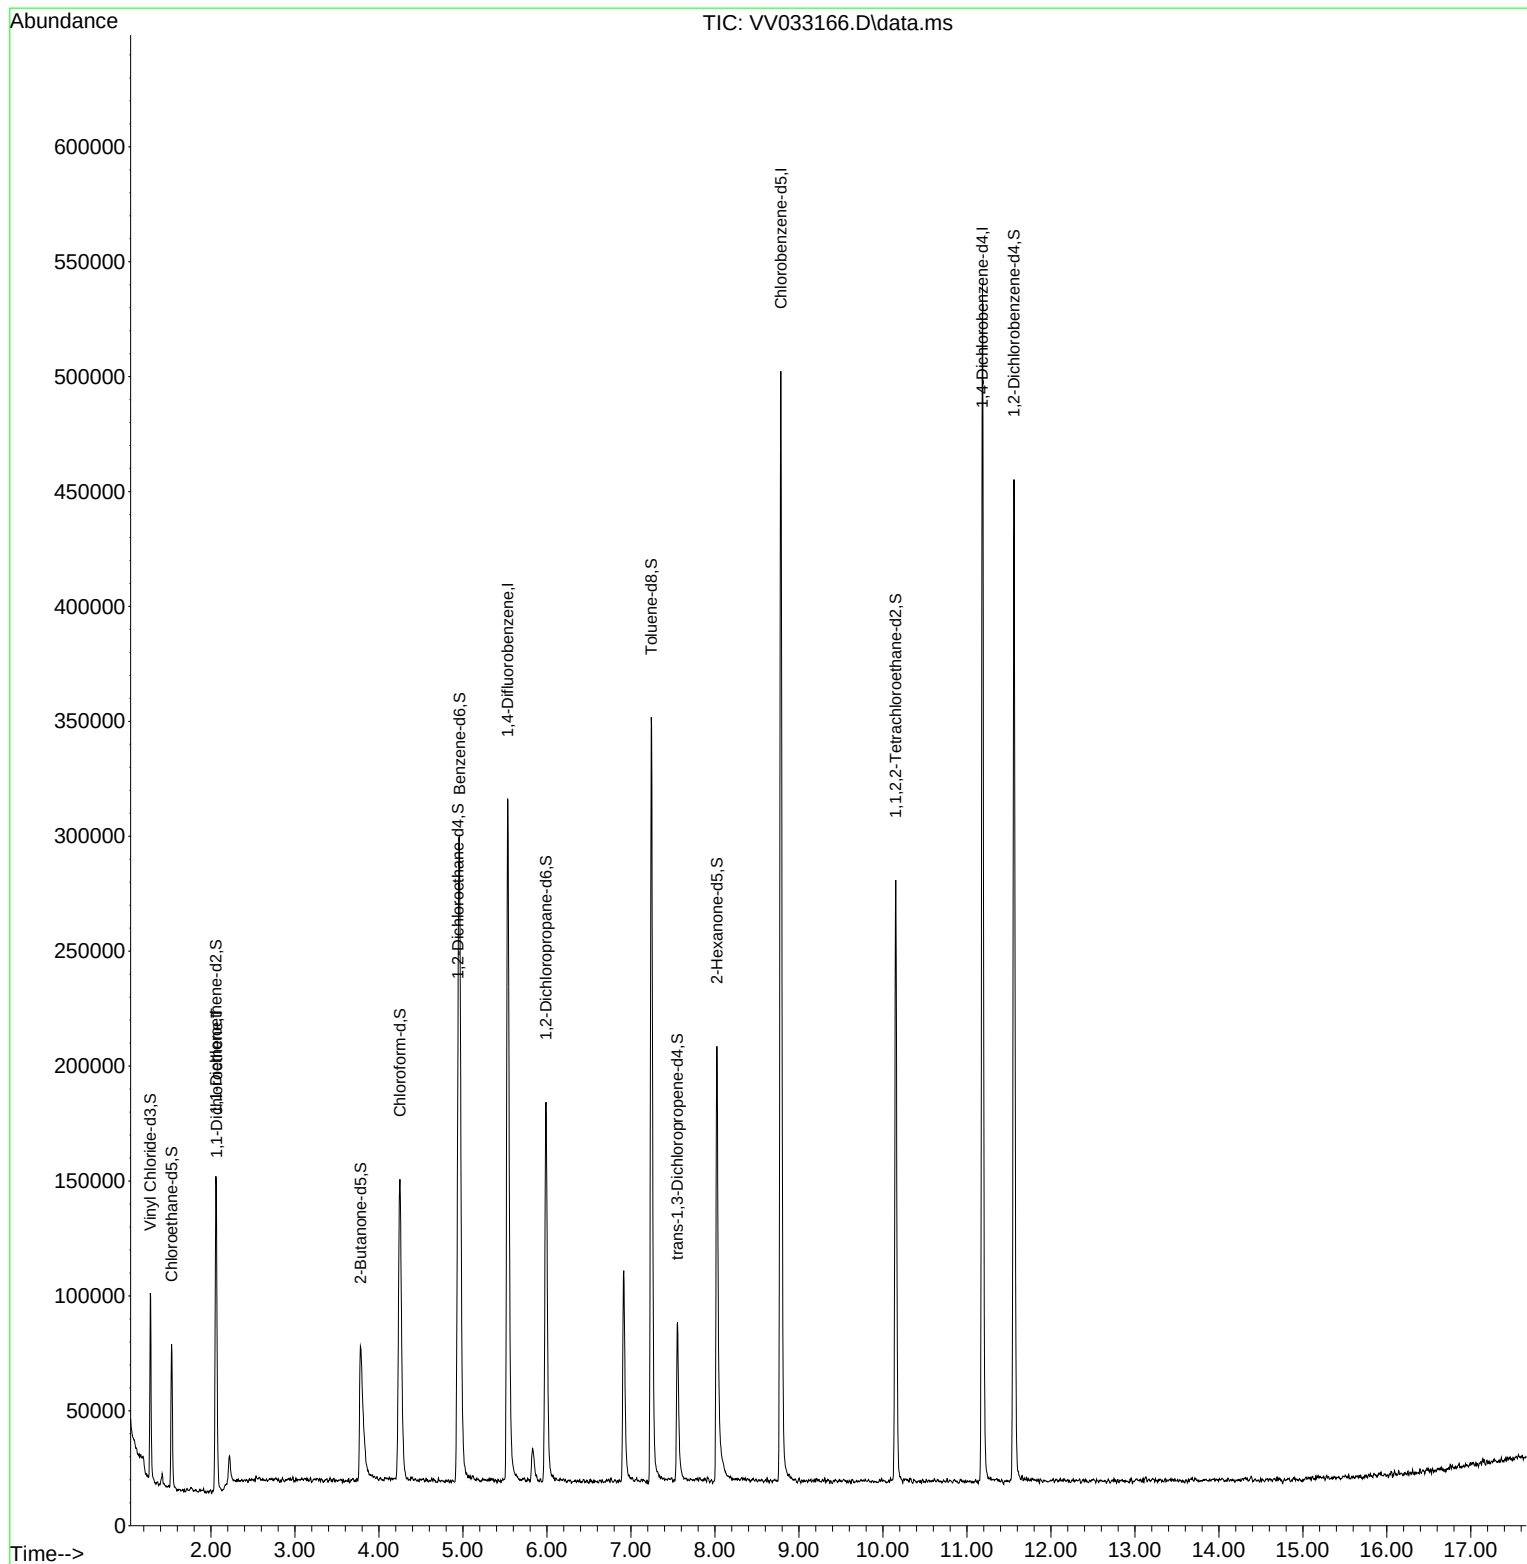

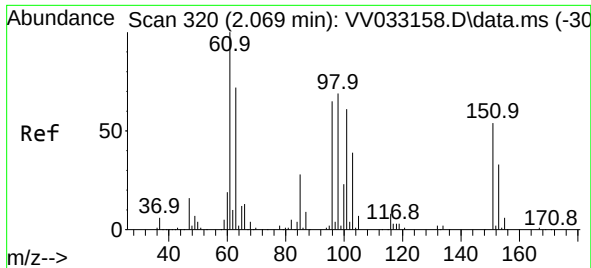

#12
 1,1-Dichloroethene
 Concen: 1.990 ug/L
 RT: 2.066 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VV033166.D
 Acq: 07 Dec 2023 23:10

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G85

Tgt Ion: 96 Resp: 2763
 Ion Ratio Lower Upper
 96 100
 61 449.8 109.1 202.7#
 63 2342.3 85.3 158.3#

