

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033172.D
 Acq On : 08 Dec 2023 01:29
 Operator : SY/MD
 Sample : 05689-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G98

Quant Time: Dec 08 04:19:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 04:15:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	266594	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	266863	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	138398	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	46378	29.101	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	58.200%#
7) Chloroethane-d5	1.532	69	40007	36.028	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	72.060%
11) 1,1-Dichloroethene-d2	2.060	65	20480	33.780	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.560%
21) 2-Butanone-d5	3.780	46	83585	105.595	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	105.600%
24) Chloroform-d	4.249	84	138161	40.850	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.700%
26) 1,2-Dichloroethane-d4	4.941	65	92219	43.856	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.720%
32) Benzene-d6	4.960	84	241737	38.732	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.460%
36) 1,2-Dichloropropane-d6	5.989	67	69352	41.327	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	82.660%
41) Toluene-d8	7.243	98	220797	37.085	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	74.160%#
43) trans-1,3-Dichloroprop...	7.555	79	39991	37.686	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.380%
47) 2-Hexanone-d5	8.021	63	61390	91.060	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.060%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	106006	44.437	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.880%
66) 1,2-Dichlorobenzene-d4	11.561	152	113313	46.017	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.040%
Target Compounds						
13) Acetone	2.108	43	2808	3.716	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033172.D
Acq On : 08 Dec 2023 01:29
Operator : SY/MD
Sample : 05689-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G98

Quant Time: Dec 08 04:19:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 04:15:58 2023
Response via : Initial Calibration

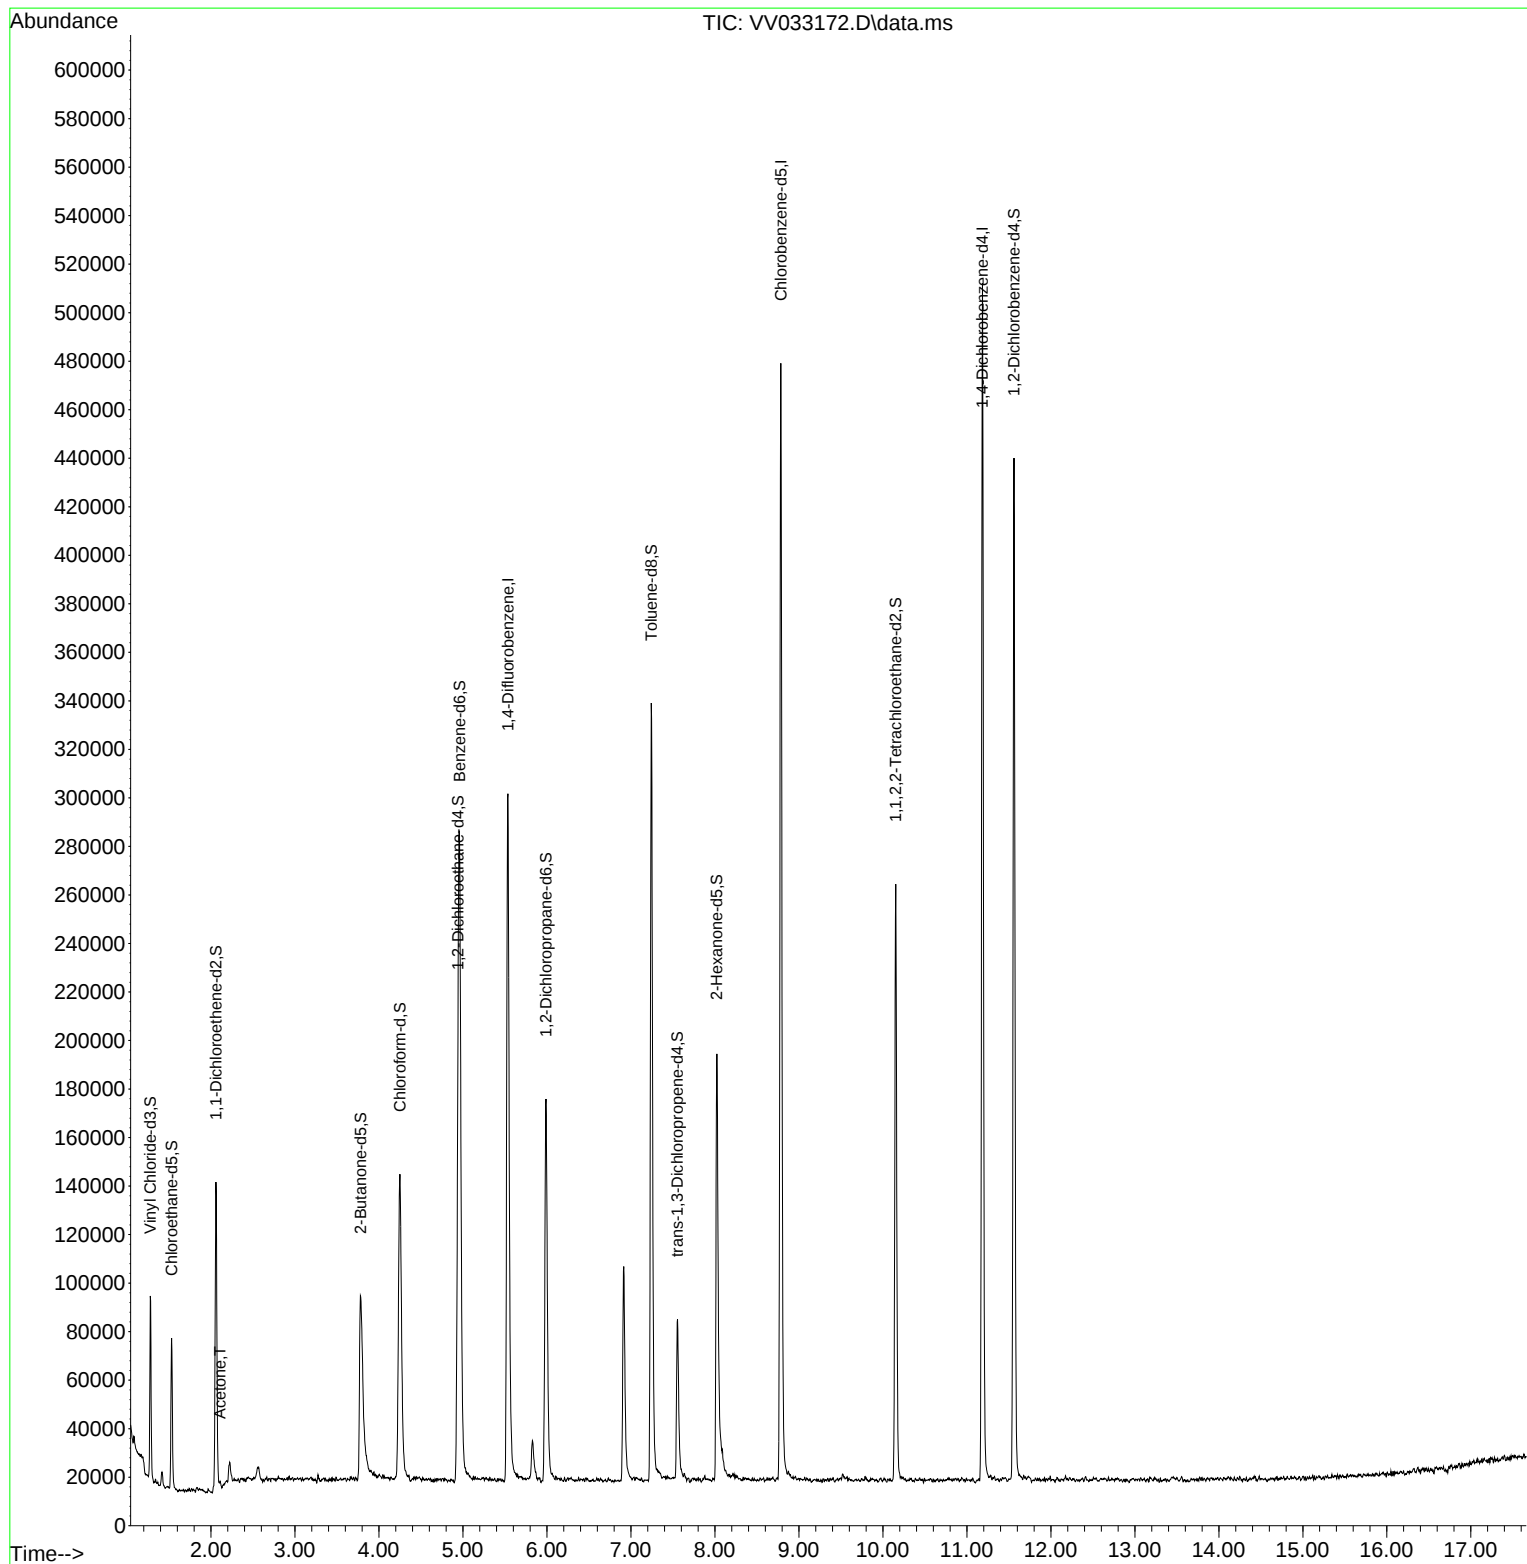

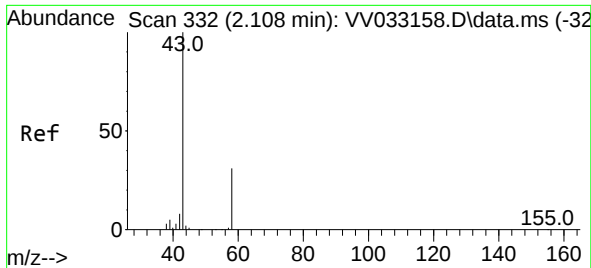

#13
 Acetone
 Concen: 3.716 ug/L
 RT: 2.108 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VV033172.D
 Acq: 08 Dec 2023 01:29

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G98

Tgt Ion: 43 Resp: 2808
 Ion Ratio Lower Upper
 43 100
 58 34.1 0.0 62.8

