

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033132.D
 Acq On : 07 Dec 2023 09:24
 Operator : SY/MD
 Sample : VV1207WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033132.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	117135	126236	13.79%	1.655%
2	1.429	110	121	132	rVV4	9731	19135	2.09%	0.251%
3	1.484	134	138	144	rVV4	1833	2403	0.26%	0.032%
4	1.529	144	152	167	rVB	87775	104840	11.45%	1.375%
5	1.603	172	175	179	rVB	1552	1288	0.14%	0.017%
6	1.632	179	184	186	rBV2	1510	1284	0.14%	0.017%
7	1.645	186	188	196	rVB2	1823	1755	0.19%	0.023%
8	1.680	196	199	203	rBV3	1176	1046	0.11%	0.014%
9	1.764	221	225	232	rVB3	2034	2568	0.28%	0.034%
10	1.806	232	238	239	rBV2	1288	1140	0.12%	0.015%
11	1.905	267	269	275	rVB3	1055	963	0.11%	0.013%
12	2.060	304	317	331	rBV	176868	258388	28.22%	3.388%
13	2.156	341	347	348	rBV	2053	1588	0.17%	0.021%
14	2.188	349	357	362	rBV	3042	4574	0.50%	0.060%
15	2.224	362	368	370	rBV	1544	1560	0.17%	0.020%
16	2.249	370	376	379	rBV3	1781	2135	0.23%	0.028%
17	2.400	420	423	429	rBV	1689	1496	0.16%	0.020%
18	3.108	638	643	648	rBV	1741	2100	0.23%	0.028%
19	3.336	711	714	717	rBV	1721	1249	0.14%	0.016%
20	3.699	824	827	829	rBV	1488	886	0.10%	0.012%
21	3.780	843	852	874	rBV	56422	147667	16.13%	1.936%
22	4.085	945	947	951	rVB	1593	945	0.10%	0.012%
23	4.246	978	997	1024	rBV2	153796	402544	43.97%	5.278%
24	4.413	1046	1049	1050	rBV2	1390	834	0.09%	0.011%
25	4.503	1074	1077	1081	rBV	1597	1419	0.15%	0.019%
26	4.590	1101	1104	1108	rBV	1760	1488	0.16%	0.020%
27	4.744	1148	1152	1156	rBV	1455	1388	0.15%	0.018%
28	4.767	1157	1159	1162	rBV	1236	778	0.08%	0.010%
29	4.857	1184	1187	1190	rBV	1350	1136	0.12%	0.015%
30	4.953	1201	1217	1242	rBV2	341697	915542	100.00%	12.004%
31	5.368	1343	1346	1348	rBV	1416	833	0.09%	0.011%
32	5.410	1357	1359	1364	rBV2	1165	1259	0.14%	0.017%
33	5.532	1386	1397	1423	rBV	338550	693495	75.75%	9.093%
34	5.828	1479	1489	1490	rBV6	12041	14671	1.60%	0.192%
35	5.902	1509	1512	1518	rVB	1754	1740	0.19%	0.023%
36	5.986	1525	1538	1561	rBV2	189808	398458	43.52%	5.224%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033132.D
 Acq On : 07 Dec 2023 09:24
 Operator : SY/MD
 Sample : VV1207WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.233	1612	1615	1622	rBV	1681	1796	0.20%	0.024%
38	6.490	1692	1695	1700	rVB	1910	1684	0.18%	0.022%
39	6.535	1706	1709	1712	rBV	1606	1130	0.12%	0.015%
40	6.632	1735	1739	1743	rBV	1522	1710	0.19%	0.022%
41	6.912	1815	1826	1856	rBV	108856	212635	23.23%	2.788%
42	7.191	1908	1913	1918	rBV	1532	1621	0.18%	0.021%
43	7.243	1918	1929	1952	rBV	403898	725147	79.20%	9.508%
44	7.551	2016	2025	2044	rBV	79390	139459	15.23%	1.829%
45	8.021	2162	2171	2203	rBV	191723	371983	40.63%	4.877%
46	8.275	2247	2250	2252	rBV3	1289	862	0.09%	0.011%
47	8.397	2285	2288	2295	rBV	1797	1537	0.17%	0.020%
48	8.783	2398	2408	2425	rBV	530210	854975	93.38%	11.210%
49	9.085	2499	2502	2504	rBV	2202	1551	0.17%	0.020%
50	9.175	2527	2530	2536	rVB	1423	1508	0.16%	0.020%
51	9.233	2545	2548	2550	rBV2	1171	915	0.10%	0.012%
52	9.686	2686	2689	2692	rBV	1001	822	0.09%	0.011%
53	9.764	2710	2713	2718	rBV	1175	1145	0.13%	0.015%
54	10.153	2823	2834	2848	rBV	281182	440231	48.08%	5.772%
55	10.760	3020	3023	3025	rBV2	1348	910	0.10%	0.012%
56	11.130	3133	3138	3143	rVB6	2206	2382	0.26%	0.031%
57	11.185	3144	3155	3171	rBV	548422	842966	92.07%	11.052%
58	11.423	3226	3229	3236	rBV	1715	1697	0.19%	0.022%
59	11.561	3259	3272	3294	rBV	481800	763518	83.40%	10.011%
60	11.709	3314	3318	3322	rVV2	1536	1229	0.13%	0.016%
61	11.731	3322	3325	3329	rVV	1701	1178	0.13%	0.015%
62	11.754	3329	3332	3337	rVB	2148	1845	0.20%	0.024%
63	11.812	3348	3350	3358	rVB2	1752	1790	0.20%	0.023%
64	11.963	3394	3397	3399	rBV	1666	1280	0.14%	0.017%
65	12.037	3417	3420	3422	rBV	1101	824	0.09%	0.011%
66	12.069	3427	3430	3431	rBV	1442	825	0.09%	0.011%
67	12.172	3459	3462	3469	rBV	1197	1514	0.17%	0.020%
68	12.204	3469	3472	3478	rVV	1491	1699	0.19%	0.022%
69	12.233	3478	3481	3488	rVB	2163	2288	0.25%	0.030%
70	12.265	3488	3491	3495	rBV	1949	1473	0.16%	0.019%
71	12.548	3574	3579	3585	rBV	2162	3086	0.34%	0.040%
72	12.590	3585	3592	3599	rVV3	4737	7322	0.80%	0.096%
73	12.821	3660	3664	3668	rBV	1524	1446	0.16%	0.019%
74	12.969	3706	3710	3714	rBV	1427	1295	0.14%	0.017%
75	13.066	3737	3740	3743	rVB	1908	1267	0.14%	0.017%
76	13.127	3755	3759	3763	rBV	1670	1519	0.17%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033132.D
 Acq On : 07 Dec 2023 09:24
 Operator : SY/MD
 Sample : VV1207WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	13.207	3777	3784	3794	rVB3	7035	11017	1.20%	0.144%
78	13.371	3831	3835	3836	rBV	1663	1162	0.13%	0.015%
79	13.445	3849	3858	3869	rBV	26696	45026	4.92%	0.590%
80	13.625	3911	3914	3917	rBV	1540	1251	0.14%	0.016%
81	13.686	3924	3933	3943	rBV5	11546	17538	1.92%	0.230%
82	13.889	3992	3996	3997	rBV	1596	1114	0.12%	0.015%
83	13.976	4021	4023	4029	rVB2	1439	1365	0.15%	0.018%
84	14.316	4123	4129	4131	rBV3	1851	2029	0.22%	0.027%
85	14.429	4161	4164	4167	rBV2	1300	1042	0.11%	0.014%
86	14.564	4202	4206	4207	rBV	1598	1182	0.13%	0.015%
87	14.593	4213	4215	4219	rVB3	1558	1037	0.11%	0.014%
88	14.889	4303	4307	4310	rBV	2085	1681	0.18%	0.022%
89	15.207	4403	4406	4410	rBV3	1411	1290	0.14%	0.017%
90	15.394	4461	4464	4467	rBV	1466	1003	0.11%	0.013%
91	15.554	4512	4514	4517	rBV3	1133	797	0.09%	0.010%
92	15.676	4549	4552	4554	rBV	1874	1293	0.14%	0.017%
93	15.725	4564	4567	4573	rBV4	1558	1694	0.19%	0.022%
94	15.818	4593	4596	4600	rBV3	1655	1199	0.13%	0.016%
95	16.175	4703	4707	4711	rBV3	2147	1864	0.20%	0.024%
96	16.358	4760	4764	4770	rBV5	2001	1684	0.18%	0.022%
97	16.397	4773	4776	4778	rBV4	1422	950	0.10%	0.012%
98	16.551	4821	4824	4827	rBV2	1998	1335	0.15%	0.018%
99	16.760	4886	4889	4891	rBV2	3014	2243	0.24%	0.029%
100	16.995	4960	4962	4964	rBV3	2262	1255	0.14%	0.016%


Sum of corrected areas: 7626946

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033132.D
Acq On : 07 Dec 2023 09:24
Operator : SY/MD
Sample : VV1207WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

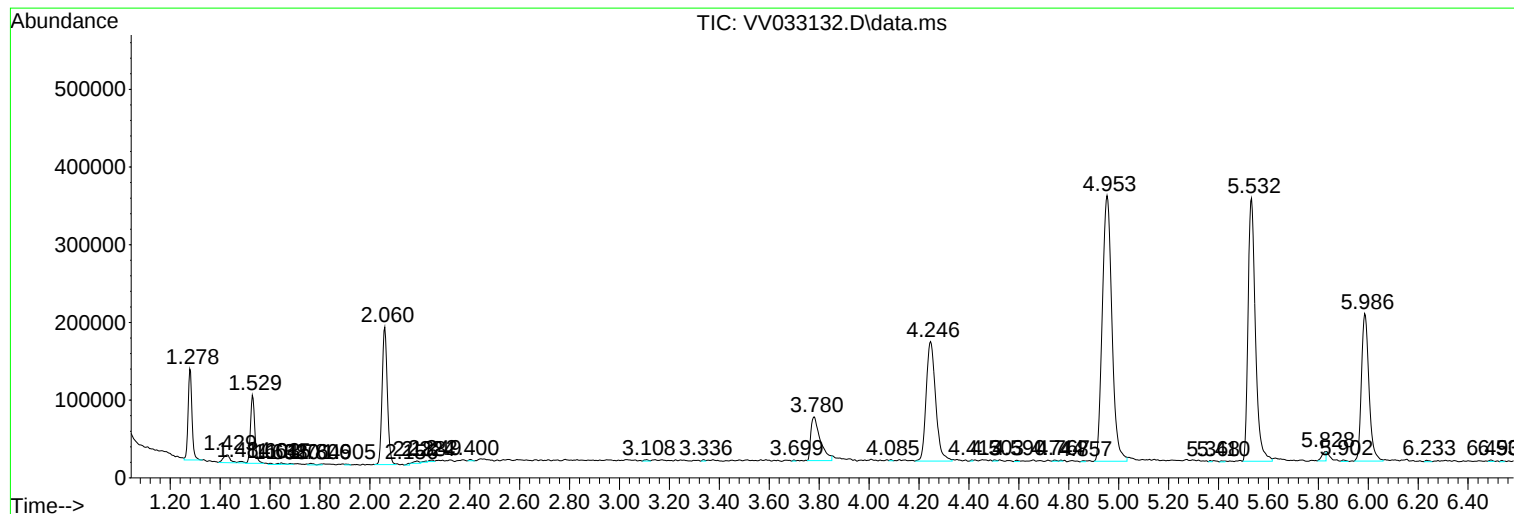

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033132.D
Acq On : 07 Dec 2023 09:24
Operator : SY/MD
Sample : VV1207WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033132.D
Acq On : 07 Dec 2023 09:24
Operator : SY/MD
Sample : VV1207WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc