

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033133.D
 Acq On : 07 Dec 2023 10:00
 Operator : SY/MD
 Sample : 05645-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	116035	127718	13.86%	1.653%
2	1.384	103	107	112	rBV	1462	1869	0.20%	0.024%
3	1.420	112	118	124	rVB5	5167	5757	0.62%	0.074%
4	1.532	144	153	164	rVB	89288	104823	11.37%	1.356%
5	1.577	164	167	173	rVB3	1265	1114	0.12%	0.014%
6	1.699	202	205	207	rBV2	1386	958	0.10%	0.012%
7	1.716	207	210	214	rVB3	1670	1311	0.14%	0.017%
8	1.835	244	247	257	rVB4	1711	1880	0.20%	0.024%
9	1.886	261	263	269	rVB2	1205	1062	0.12%	0.014%
10	1.963	283	287	290	rBV2	1297	1046	0.11%	0.014%
11	2.060	304	317	331	rBV	178355	264101	28.65%	3.417%
12	2.182	343	355	357	rBV	3077	5497	0.60%	0.071%
13	2.217	357	366	368	rVV3	3498	5793	0.63%	0.075%
14	2.230	368	370	381	rVB2	3202	4574	0.50%	0.059%
15	2.343	401	405	409	rBV4	1878	2131	0.23%	0.028%
16	2.597	481	484	488	rVB	2262	1689	0.18%	0.022%
17	2.925	583	586	590	rBV	1887	1202	0.13%	0.016%
18	3.252	685	688	690	rBV	1429	936	0.10%	0.012%
19	3.349	715	718	721	rBV	1391	1038	0.11%	0.013%
20	3.478	754	758	760	rBV	1964	1101	0.12%	0.014%
21	3.494	760	763	765	rBV	1628	1140	0.12%	0.015%
22	3.548	778	780	790	rVV	1233	1520	0.16%	0.020%
23	3.638	805	808	814	rBV	1761	1880	0.20%	0.024%
24	3.777	844	851	875	rBV	51468	132986	14.43%	1.721%
25	4.002	918	921	925	rVB	1565	1129	0.12%	0.015%
26	4.246	982	997	1020	rBV	159018	403480	43.77%	5.221%
27	4.432	1053	1055	1062	rVB2	1486	1780	0.19%	0.023%
28	4.551	1089	1092	1094	rBV2	1548	1127	0.12%	0.015%
29	4.818	1172	1175	1181	rBV2	1108	1403	0.15%	0.018%
30	4.953	1201	1217	1246	rBV2	339581	921759	100.00%	11.927%
31	5.532	1385	1397	1423	rBV	343138	714388	77.50%	9.244%
32	5.838	1478	1492	1507	rBV6	29005	73355	7.96%	0.949%
33	5.985	1525	1538	1561	rBV	193757	402075	43.62%	5.203%
34	6.149	1585	1589	1592	rBV	2461	2217	0.24%	0.029%
35	6.365	1649	1656	1659	rBV2	1608	2190	0.24%	0.028%
36	6.442	1673	1680	1690	rVB	2462	4372	0.47%	0.057%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033133.D
 Acq On : 07 Dec 2023 10:00
 Operator : SY/MD
 Sample : 05645-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.484	1690	1693	1695	rBV	1759	1147	0.12%	0.015%
38	6.516	1700	1703	1713	rVB	1943	2928	0.32%	0.038%
39	6.911	1816	1826	1848	rBV	112692	207662	22.53%	2.687%
40	7.175	1905	1908	1911	rBV3	1257	1228	0.13%	0.016%
41	7.243	1918	1929	1947	rBV	415902	732690	79.49%	9.481%
42	7.506	2008	2011	2012	rBV2	1551	952	0.10%	0.012%
43	7.551	2016	2025	2040	rVV	82978	140759	15.27%	1.821%
44	8.021	2163	2171	2198	rBV	180894	335975	36.45%	4.347%
45	8.233	2233	2237	2239	rBV2	1515	1354	0.15%	0.018%
46	8.284	2251	2253	2259	rVB	1722	1156	0.13%	0.015%
47	8.571	2339	2342	2345	rBV	1320	930	0.10%	0.012%
48	8.783	2397	2408	2433	rBV	545613	890280	96.58%	11.520%
49	9.255	2552	2555	2558	rBV	1841	1192	0.13%	0.015%
50	9.384	2590	2595	2599	rBV	1926	2146	0.23%	0.028%
51	9.468	2618	2621	2624	rBV	1614	1066	0.12%	0.014%
52	9.616	2664	2667	2670	rBV	1634	997	0.11%	0.013%
53	9.834	2730	2735	2743	rBV	2371	4061	0.44%	0.053%
54	9.927	2761	2764	2768	rBV2	1347	1380	0.15%	0.018%
55	10.153	2823	2834	2853	rBV	273942	437674	47.48%	5.663%
56	10.323	2881	2887	2899	rVB3	5423	9452	1.03%	0.122%
57	10.371	2899	2902	2905	rBV	2169	1721	0.19%	0.022%
58	10.773	3023	3027	3029	rBV2	1173	956	0.10%	0.012%
59	10.792	3030	3033	3038	rVB	1387	1216	0.13%	0.016%
60	10.831	3042	3045	3047	rBV	1630	1115	0.12%	0.014%
61	10.905	3065	3068	3072	rVB2	1541	1242	0.13%	0.016%
62	10.934	3072	3077	3078	rBV	1655	1617	0.18%	0.021%
63	11.124	3133	3136	3142	rBV3	1629	2250	0.24%	0.029%
64	11.185	3144	3155	3171	rBV	580509	892799	96.86%	11.552%
65	11.288	3184	3187	3192	rVB	3105	2913	0.32%	0.038%
66	11.313	3192	3195	3199	rBV	1888	1480	0.16%	0.019%
67	11.333	3199	3201	3206	rBV	1317	939	0.10%	0.012%
68	11.561	3260	3272	3293	rVV	495460	786612	85.34%	10.178%
69	11.895	3373	3376	3379	rBV	1759	1120	0.12%	0.014%
70	11.963	3395	3397	3403	rVB2	1646	1544	0.17%	0.020%
71	12.008	3403	3411	3414	rBV	1869	2688	0.29%	0.035%
72	12.152	3453	3456	3460	rBV	1310	1128	0.12%	0.015%
73	12.223	3475	3478	3481	rBV2	1537	1100	0.12%	0.014%
74	12.297	3499	3501	3508	rVB	1853	1804	0.20%	0.023%
75	12.680	3617	3620	3622	rBV	1299	948	0.10%	0.012%
76	12.808	3658	3660	3667	rVB	1182	1000	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033133.D
 Acq On : 07 Dec 2023 10:00
 Operator : SY/MD
 Sample : 05645-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.873	3677	3680	3683	rBV	2130	2080	0.23%	0.027%
78	13.066	3737	3740	3743	rBV	1358	974	0.11%	0.013%
79	13.098	3747	3750	3756	rVB	2162	1636	0.18%	0.021%
80	13.130	3756	3760	3762	rBV	2022	1514	0.16%	0.020%
81	13.201	3778	3782	3783	rBV2	2561	1797	0.19%	0.023%
82	13.448	3852	3859	3868	rVB2	6650	10766	1.17%	0.139%
83	13.676	3927	3930	3932	rBV2	1663	1137	0.12%	0.015%
84	13.818	3970	3974	3978	rBV	2221	2500	0.27%	0.032%
85	13.879	3990	3993	3995	rBV2	1535	936	0.10%	0.012%
86	14.069	4049	4052	4056	rBV	1099	1132	0.12%	0.015%
87	14.268	4111	4114	4119	rBV3	1451	1355	0.15%	0.018%
88	14.297	4119	4123	4127	rVV	1920	1562	0.17%	0.020%
89	14.435	4162	4166	4170	rBV3	1374	1644	0.18%	0.021%
90	14.541	4196	4199	4204	rBV	1889	1684	0.18%	0.022%
91	14.673	4237	4240	4242	rBV	1433	964	0.10%	0.012%
92	14.741	4257	4261	4265	rBV3	1387	1523	0.17%	0.020%
93	14.776	4269	4272	4278	rVB	1976	1630	0.18%	0.021%
94	14.805	4278	4281	4284	rBV2	1681	1380	0.15%	0.018%
95	14.889	4304	4307	4311	rBV2	1830	1942	0.21%	0.025%
96	15.020	4346	4348	4352	rVB2	2083	1349	0.15%	0.017%
97	15.043	4352	4355	4358	rBV	1617	1223	0.13%	0.016%
98	15.348	4448	4450	4455	rBV	1274	1229	0.13%	0.016%
99	15.982	4645	4647	4649	rBV2	1882	1123	0.12%	0.015%
100	16.303	4744	4747	4749	rBV2	2294	1533	0.17%	0.020%




Sum of corrected areas: 7728235

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033133.D
Acq On : 07 Dec 2023 10:00
Operator : SY/MD
Sample : 05645-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

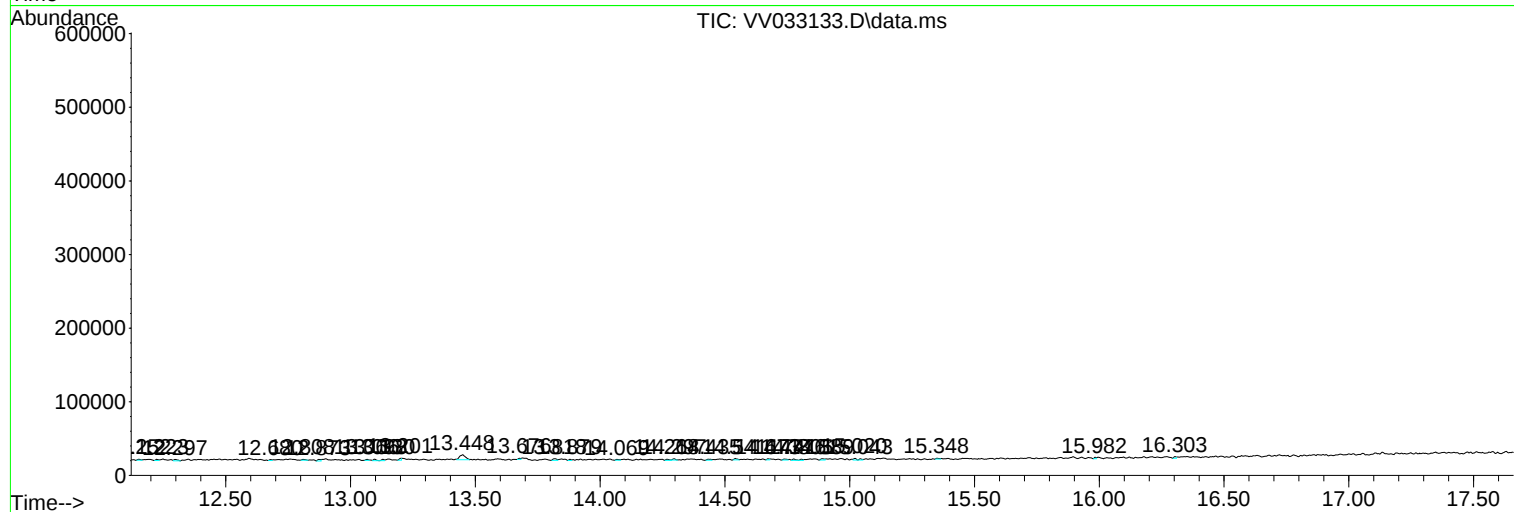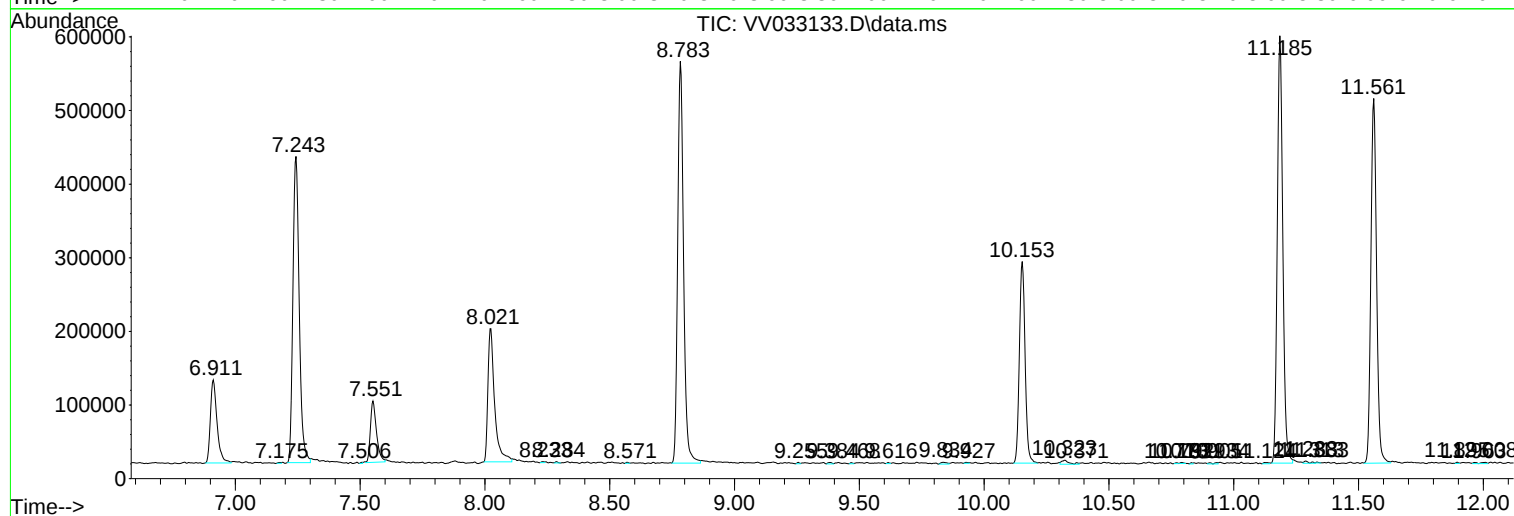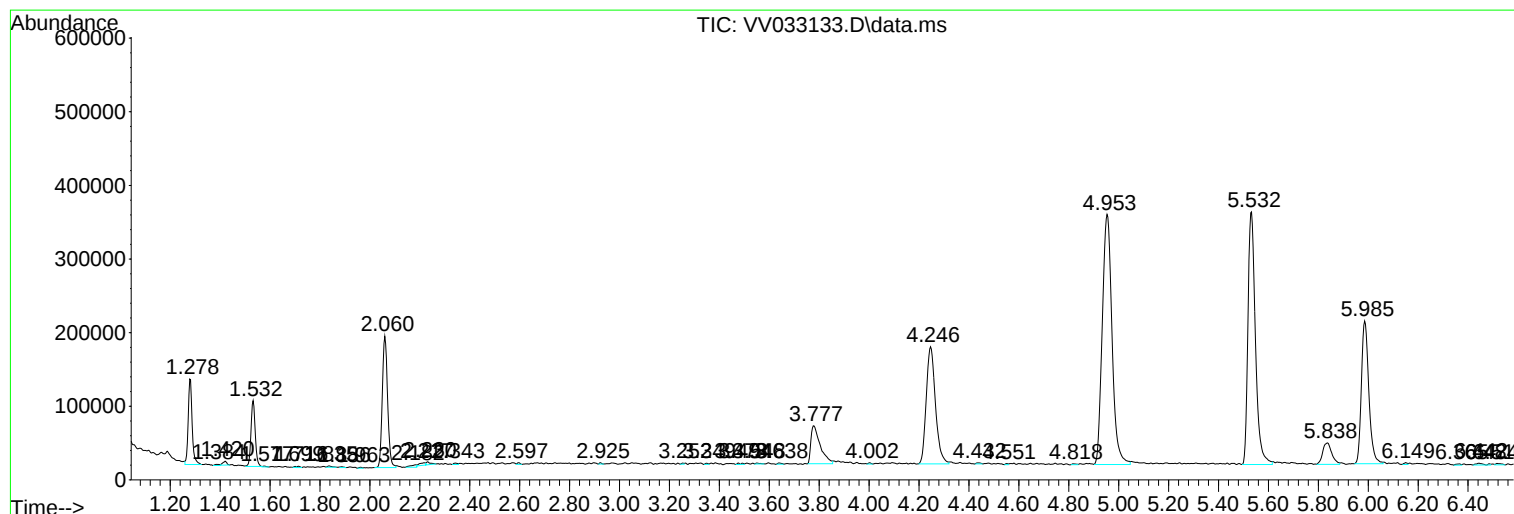

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033133.D
Acq On : 07 Dec 2023 10:00
Operator : SY/MD
Sample : 05645-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033133.D
Acq On : 07 Dec 2023 10:00
Operator : SY/MD
Sample : 05645-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc