

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033135.D
 Acq On : 07 Dec 2023 10:47
 Operator : SY/MD
 Sample : 05645-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033135.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rVB	103466	113151	13.16%	1.562%
2	1.387	105	108	110	rBV	886	556	0.06%	0.008%
3	1.420	112	118	127	rVB4	5120	7081	0.82%	0.098%
4	1.490	132	140	144	rBV2	1548	1844	0.21%	0.025%
5	1.535	144	154	165	rVV	79222	94934	11.05%	1.311%
6	1.590	169	171	175	rVB2	1547	975	0.11%	0.013%
7	1.629	180	183	185	rBV	1296	800	0.09%	0.011%
8	1.683	197	200	203	rVB2	1105	598	0.07%	0.008%
9	1.715	203	210	214	rBV3	1316	1601	0.19%	0.022%
10	1.780	224	230	239	rBV2	1455	2799	0.33%	0.039%
11	1.838	244	248	251	rVV3	1755	1256	0.15%	0.017%
12	1.902	265	268	271	rVV	1061	818	0.10%	0.011%
13	1.918	271	273	278	rVB3	1179	721	0.08%	0.010%
14	1.963	284	287	293	rVB	1512	1417	0.16%	0.020%
15	2.063	307	318	331	rBV	159723	237308	27.61%	3.276%
16	2.185	344	356	359	rBV	3619	7184	0.84%	0.099%
17	2.207	360	363	365	rBV	1354	925	0.11%	0.013%
18	2.243	370	374	379	rVV3	1406	2095	0.24%	0.029%
19	2.551	467	470	473	rBV	1765	1407	0.16%	0.019%
20	2.658	498	503	505	rBV	1486	1481	0.17%	0.020%
21	3.285	693	698	704	rBV	2052	2869	0.33%	0.040%
22	3.317	705	708	712	rVV	1581	1286	0.15%	0.018%
23	3.407	733	736	738	rVB2	1230	588	0.07%	0.008%
24	3.532	772	775	777	rBV	1404	901	0.10%	0.012%
25	3.783	845	853	873	rBV2	52753	130746	15.21%	1.805%
26	4.014	922	925	926	rBV2	1389	739	0.09%	0.010%
27	4.127	957	960	964	rVB2	1634	1324	0.15%	0.018%
28	4.249	983	998	1021	rBV2	147363	372122	43.30%	5.137%
29	4.487	1068	1072	1074	rBV2	1817	1473	0.17%	0.020%
30	4.751	1151	1154	1156	rBV2	983	677	0.08%	0.009%
31	4.956	1202	1218	1242	rBV2	321908	859492	100.00%	11.866%
32	5.410	1355	1359	1361	rBV	2166	1766	0.21%	0.024%
33	5.445	1368	1370	1377	rVB	1343	854	0.10%	0.012%
34	5.535	1386	1398	1421	rBV	326069	669126	77.85%	9.238%
35	5.673	1439	1441	1444	rVB3	1240	591	0.07%	0.008%
36	5.773	1468	1472	1475	rBV	1652	1225	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033135.D
 Acq On : 07 Dec 2023 10:47
 Operator : SY/MD
 Sample : 05645-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.831	1480	1490	1501	rVV7	13806	29933	3.48%	0.413%
38	5.989	1526	1539	1561	rBV	185765	381566	44.39%	5.268%
39	6.146	1584	1588	1597	rVB	2619	2734	0.32%	0.038%
40	6.310	1636	1639	1642	rBV2	1254	863	0.10%	0.012%
41	6.429	1673	1676	1680	rVB	1730	1124	0.13%	0.016%
42	6.490	1692	1695	1699	rBV	1382	940	0.11%	0.013%
43	6.596	1726	1728	1731	rBV	1283	749	0.09%	0.010%
44	6.818	1793	1797	1802	rBV	1538	1404	0.16%	0.019%
45	6.915	1817	1827	1847	rBV2	102602	189455	22.04%	2.616%
46	7.243	1919	1929	1958	rBV	390658	691182	80.42%	9.542%
47	7.342	1958	1960	1965	rVB3	1878	1548	0.18%	0.021%
48	7.468	1996	1999	2002	rBV	1185	939	0.11%	0.013%
49	7.506	2008	2011	2016	rBV3	1850	2076	0.24%	0.029%
50	7.551	2017	2025	2039	rBV2	76529	134036	15.59%	1.850%
51	7.870	2118	2124	2128	rBV	1938	2490	0.29%	0.034%
52	7.963	2148	2153	2156	rBV2	1612	1866	0.22%	0.026%
53	8.024	2163	2172	2198	rBV	186009	357651	41.61%	4.938%
54	8.394	2285	2287	2294	rVB	1828	1231	0.14%	0.017%
55	8.464	2307	2309	2311	rBV	1139	713	0.08%	0.010%
56	8.577	2342	2344	2349	rVB	1945	1382	0.16%	0.019%
57	8.599	2349	2351	2353	rBV	1226	786	0.09%	0.011%
58	8.734	2390	2393	2395	rBV	1555	950	0.11%	0.013%
59	8.786	2396	2409	2430	rBV	513582	846764	98.52%	11.690%
60	8.876	2435	2437	2442	rVB2	2616	1961	0.23%	0.027%
61	9.349	2581	2584	2588	rBV	1493	1428	0.17%	0.020%
62	9.802	2721	2725	2729	rBV	1697	1593	0.19%	0.022%
63	9.921	2759	2762	2767	rBV2	1156	1036	0.12%	0.014%
64	10.008	2786	2789	2793	rVB	1655	1079	0.13%	0.015%
65	10.046	2793	2801	2806	rBV	2206	3714	0.43%	0.051%
66	10.152	2824	2834	2852	rBV	264798	424289	49.37%	5.858%
67	10.484	2935	2937	2940	rVB	1632	815	0.09%	0.011%
68	10.525	2947	2950	2953	rVB	1157	719	0.08%	0.010%
69	10.586	2965	2969	2972	rBV	2058	1771	0.21%	0.024%
70	10.689	2998	3001	3003	rBV	903	613	0.07%	0.008%
71	10.860	3052	3054	3057	rBV	1128	769	0.09%	0.011%
72	11.021	3101	3104	3105	rBV	989	638	0.07%	0.009%
73	11.185	3144	3155	3178	rBV	538894	846896	98.53%	11.692%
74	11.561	3261	3272	3292	rBV	472905	747194	86.93%	10.316%
75	11.689	3308	3312	3314	rBV2	1303	1196	0.14%	0.017%
76	11.763	3332	3335	3338	rBV	1716	1249	0.15%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033135.D
 Acq On : 07 Dec 2023 10:47
 Operator : SY/MD
 Sample : 05645-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.837	3354	3358	3360	rBV2	1673	1439	0.17%	0.020%
78	12.300	3499	3502	3504	rBV	1042	814	0.09%	0.011%
79	12.541	3574	3577	3583	rVB	1587	1397	0.16%	0.019%
80	12.850	3670	3673	3675	rBV	1503	866	0.10%	0.012%
81	12.972	3708	3711	3715	rBV	1535	1037	0.12%	0.014%
82	12.995	3715	3718	3721	rBV	1511	1216	0.14%	0.017%
83	13.438	3853	3856	3857	rBV	1354	828	0.10%	0.011%
84	13.451	3858	3860	3865	rVB4	2037	1505	0.18%	0.021%
85	13.570	3894	3897	3902	rVB	2154	1500	0.17%	0.021%
86	13.596	3902	3905	3909	rBV	1244	1013	0.12%	0.014%
87	13.660	3922	3925	3928	rBV2	1527	1102	0.13%	0.015%
88	13.844	3980	3982	3990	rBV	1207	1405	0.16%	0.019%
89	13.921	4000	4006	4010	rBV3	1660	2210	0.26%	0.031%
90	13.966	4017	4020	4022	rBV	1370	1027	0.12%	0.014%
91	14.274	4113	4116	4121	rBV3	1386	1274	0.15%	0.018%
92	14.445	4166	4169	4171	rBV2	1256	1031	0.12%	0.014%
93	14.499	4184	4186	4189	rBV	1027	794	0.09%	0.011%
94	14.567	4204	4207	4210	rBV	2441	1479	0.17%	0.020%
95	15.178	4394	4397	4400	rBV2	1282	734	0.09%	0.010%
96	15.236	4412	4415	4417	rBV2	1766	1398	0.16%	0.019%
97	15.487	4490	4493	4494	rBV3	1798	1054	0.12%	0.015%
98	15.535	4505	4508	4511	rBV2	2347	1815	0.21%	0.025%
99	15.966	4638	4642	4644	rBV2	1618	1422	0.17%	0.020%
100	16.020	4657	4659	4662	rBV2	1251	894	0.10%	0.012%




Sum of corrected areas: 7243326

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033135.D
Acq On : 07 Dec 2023 10:47
Operator : SY/MD
Sample : 05645-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

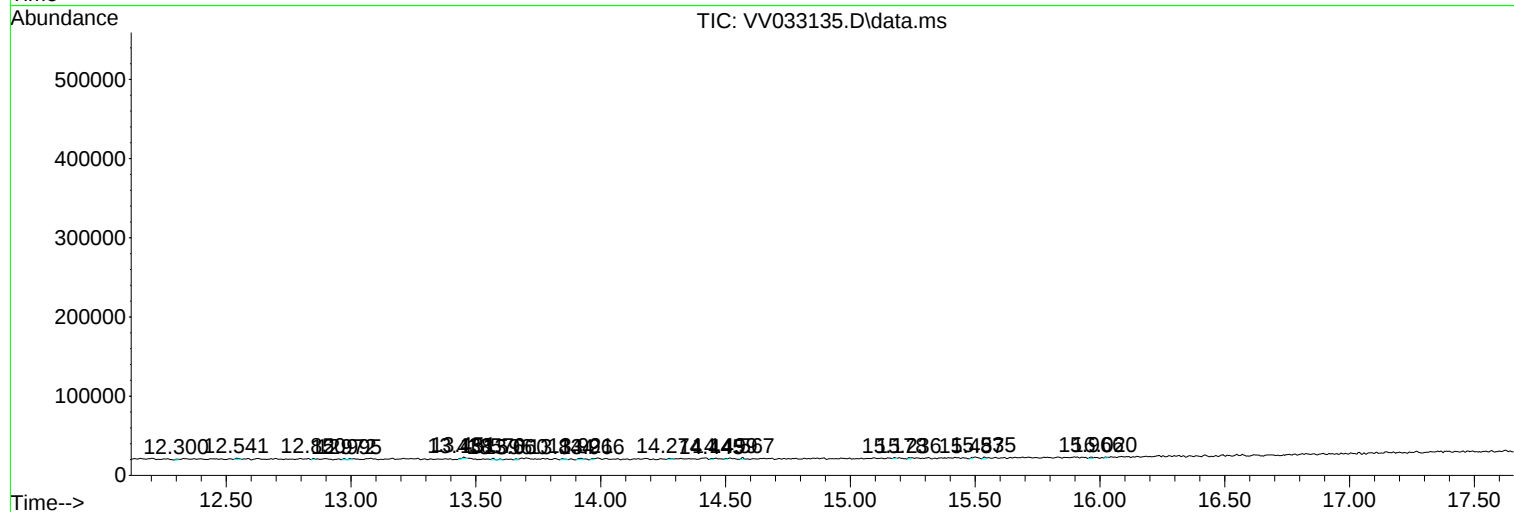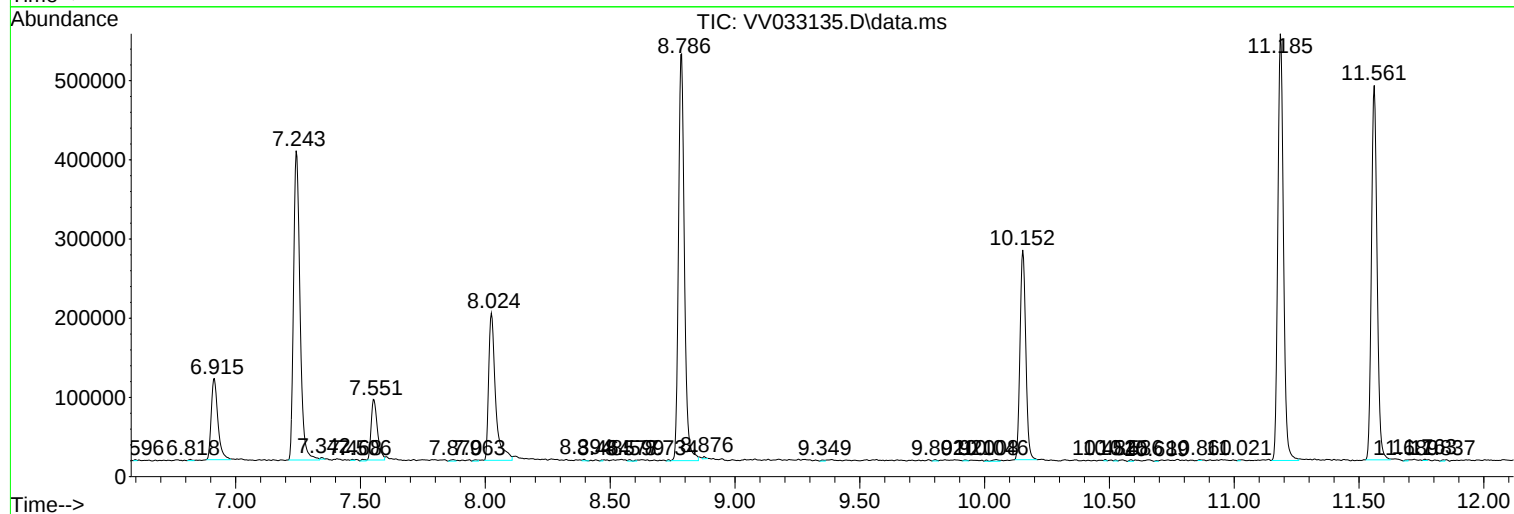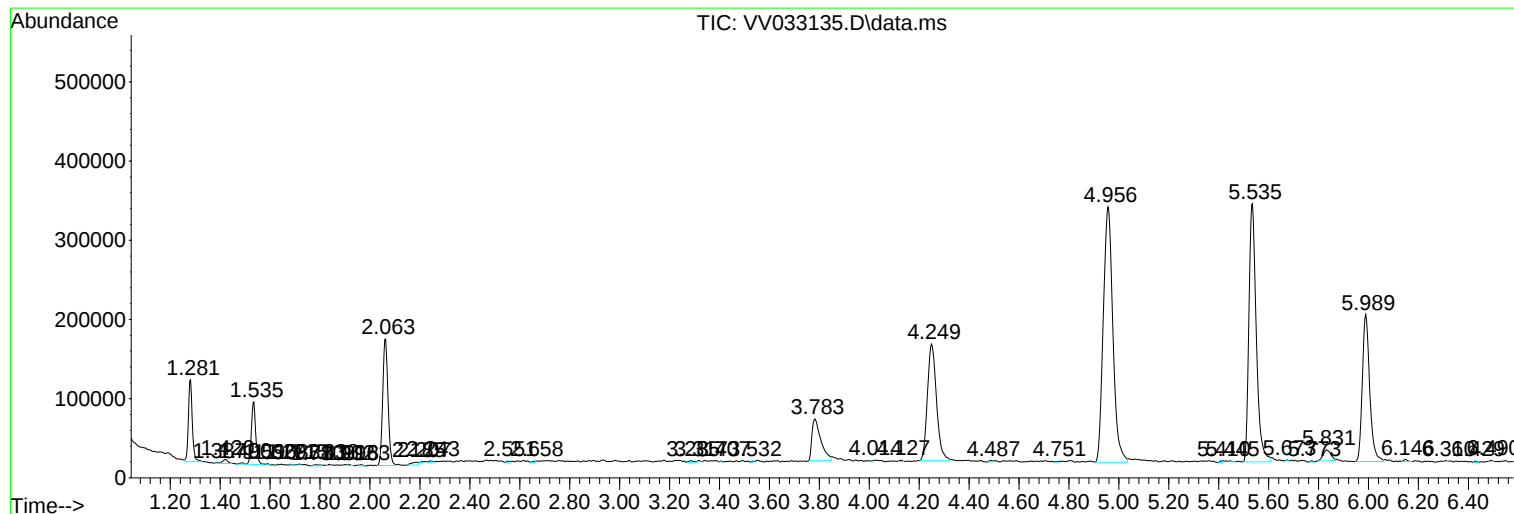

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033135.D
Acq On : 07 Dec 2023 10:47
Operator : SY/MD
Sample : 05645-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033135.D
Acq On : 07 Dec 2023 10:47
Operator : SY/MD
Sample : 05645-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc