

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033136.D
 Acq On : 07 Dec 2023 11:10
 Operator : SY/MD
 Sample : 05645-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033136.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	88	rVB	108854	115189	12.77%	1.578%
2	1.385	105	107	109	rBV2	755	359	0.04%	0.005%
3	1.420	109	118	128	rVB	5958	9477	1.05%	0.130%
4	1.458	128	130	134	rVB2	1700	1005	0.11%	0.014%
5	1.494	134	141	143	rBV3	1444	1660	0.18%	0.023%
6	1.532	144	153	165	rVB	80758	96719	10.73%	1.325%
7	1.600	172	174	176	rBV2	518	237	0.03%	0.003%
8	1.613	176	178	185	rVB2	1457	1228	0.14%	0.017%
9	1.642	185	187	189	rBV2	549	279	0.03%	0.004%
10	1.661	189	193	195	rBV3	800	657	0.07%	0.009%
11	1.677	196	198	203	rVB3	980	745	0.08%	0.010%
12	1.700	203	205	207	rVB	507	243	0.03%	0.003%
13	1.712	207	209	211	rBV2	737	385	0.04%	0.005%
14	1.738	214	217	221	rVB2	1537	1116	0.12%	0.015%
15	1.761	221	224	226	rBV2	1322	815	0.09%	0.011%
16	1.783	229	231	234	rVB2	924	467	0.05%	0.006%
17	1.809	237	239	241	rVB3	611	237	0.03%	0.003%
18	1.828	241	245	249	rVB3	1416	1098	0.12%	0.015%
19	1.854	250	253	255	rVB3	371	177	0.02%	0.002%
20	1.873	255	259	261	rBV	1139	1004	0.11%	0.014%
21	1.941	274	280	284	rBV	1649	2004	0.22%	0.027%
22	1.960	284	286	289	rVB	1015	466	0.05%	0.006%
23	1.976	289	291	292	rBV	906	428	0.05%	0.006%
24	1.989	292	295	301	rVB2	2179	2252	0.25%	0.031%
25	2.018	301	304	305	rBV	1722	1015	0.11%	0.014%
26	2.063	307	318	331	rBV	172595	253297	28.09%	3.470%
27	2.130	336	339	341	rBV2	929	680	0.08%	0.009%
28	2.147	341	344	347	rBV	1114	992	0.11%	0.014%
29	2.182	352	355	357	rBV	1192	837	0.09%	0.011%
30	2.220	359	367	374	rBV3	7398	12405	1.38%	0.170%
31	3.015	609	614	617	rBV	1890	2170	0.24%	0.030%
32	3.127	646	649	652	rBV	2206	1686	0.19%	0.023%
33	3.301	700	703	706	rBV	1973	1549	0.17%	0.021%
34	3.519	767	771	773	rBV	1495	1135	0.13%	0.016%
35	3.536	774	776	781	rVB	1490	1120	0.12%	0.015%
36	3.696	824	826	829	rVB	1311	569	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033136.D
 Acq On : 07 Dec 2023 11:10
 Operator : SY/MD
 Sample : 05645-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	3.716	829	832	837	rVB	1235	1027	0.11%	0.014%
38	3.783	844	853	882	rBV	62010	170129	18.87%	2.331%
39	4.249	984	998	1026	rBV2	151562	386125	42.82%	5.290%
40	4.468	1063	1066	1067	rBV	1136	714	0.08%	0.010%
41	4.609	1107	1110	1112	rBV	1231	780	0.09%	0.011%
42	4.857	1184	1187	1191	rBV2	1387	1168	0.13%	0.016%
43	4.957	1202	1218	1243	rBV2	339008	901715	100.00%	12.353%
44	5.111	1263	1266	1269	rBV	2008	1205	0.13%	0.017%
45	5.236	1302	1305	1310	rBV	1451	1442	0.16%	0.020%
46	5.423	1361	1363	1369	rBV	1246	1250	0.14%	0.017%
47	5.535	1383	1398	1422	rBV	296190	615716	68.28%	8.435%
48	5.706	1449	1451	1454	rBV	1245	620	0.07%	0.008%
49	5.828	1483	1489	1492	rBV6	10328	12834	1.42%	0.176%
50	5.989	1527	1539	1562	rBV	193806	402873	44.68%	5.519%
51	6.317	1637	1641	1643	rBV2	1357	1167	0.13%	0.016%
52	6.551	1712	1714	1717	rBV	1333	987	0.11%	0.014%
53	6.664	1746	1749	1753	rBV	1927	1347	0.15%	0.018%
54	6.863	1808	1811	1814	rBV2	1272	900	0.10%	0.012%
55	6.915	1817	1827	1848	rVV2	110270	208791	23.15%	2.860%
56	7.124	1889	1892	1895	rBV	1558	1258	0.14%	0.017%
57	7.166	1903	1905	1910	rVB	2063	1605	0.18%	0.022%
58	7.243	1919	1929	1952	rBV	415714	718889	79.72%	9.849%
59	7.551	2014	2025	2044	rBV	81320	149517	16.58%	2.048%
60	7.812	2103	2106	2111	rVB	1460	1191	0.13%	0.016%
61	8.024	2163	2172	2190	rBV	209107	376643	41.77%	5.160%
62	8.400	2287	2289	2296	rVB	2542	2445	0.27%	0.033%
63	8.432	2296	2299	2304	rBV	1853	1407	0.16%	0.019%
64	8.786	2399	2409	2433	rBV	462308	766058	84.96%	10.495%
65	9.227	2542	2546	2550	rVB	1671	1433	0.16%	0.020%
66	9.249	2550	2553	2554	rBV	1037	649	0.07%	0.009%
67	9.432	2607	2610	2613	rVB	1498	816	0.09%	0.011%
68	9.645	2674	2676	2678	rBV	1272	666	0.07%	0.009%
69	9.866	2742	2745	2749	rBV	1431	980	0.11%	0.013%
70	10.066	2805	2807	2810	rVB	1938	1202	0.13%	0.016%
71	10.153	2823	2834	2859	rBV	288956	457381	50.72%	6.266%
72	10.439	2921	2923	2928	rVB	1695	1239	0.14%	0.017%
73	10.715	3006	3009	3013	rVB	1710	1238	0.14%	0.017%
74	10.911	3068	3070	3074	rBV	1035	780	0.09%	0.011%
75	11.185	3145	3155	3175	rBV	503962	772924	85.72%	10.589%
76	11.288	3184	3187	3189	rBV	1593	1122	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033136.D
 Acq On : 07 Dec 2023 11:10
 Operator : SY/MD
 Sample : 05645-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.561	3260	3272	3292	rBV	508039	792311	87.87%	10.855%
78	12.175	3461	3463	3466	rBV	1316	737	0.08%	0.010%
79	12.313	3502	3506	3510	rBV	1913	1695	0.19%	0.023%
80	12.889	3682	3685	3689	rBV	1707	1692	0.19%	0.023%
81	12.908	3689	3691	3696	rVV	1716	1274	0.14%	0.017%
82	13.262	3798	3801	3808	rVB	1812	2226	0.25%	0.030%
83	13.397	3840	3843	3847	rBV	1987	1788	0.20%	0.024%
84	13.452	3857	3860	3867	rVB2	3013	3322	0.37%	0.046%
85	14.426	4160	4163	4165	rBV2	1408	964	0.11%	0.013%
86	14.551	4200	4202	4205	rBV	1660	1015	0.11%	0.014%
87	14.680	4240	4242	4245	rVB	1159	503	0.06%	0.007%
88	14.699	4245	4248	4251	rBV	1538	1176	0.13%	0.016%
89	15.175	4393	4396	4399	rBV2	1306	990	0.11%	0.014%
90	15.329	4442	4444	4448	rBV3	1534	1269	0.14%	0.017%
91	15.513	4498	4501	4504	rBV	1962	1334	0.15%	0.018%
92	15.943	4633	4635	4639	rVB3	1728	1082	0.12%	0.015%




Sum of corrected areas: 7299313

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033136.D
Acq On : 07 Dec 2023 11:10
Operator : SY/MD
Sample : 05645-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

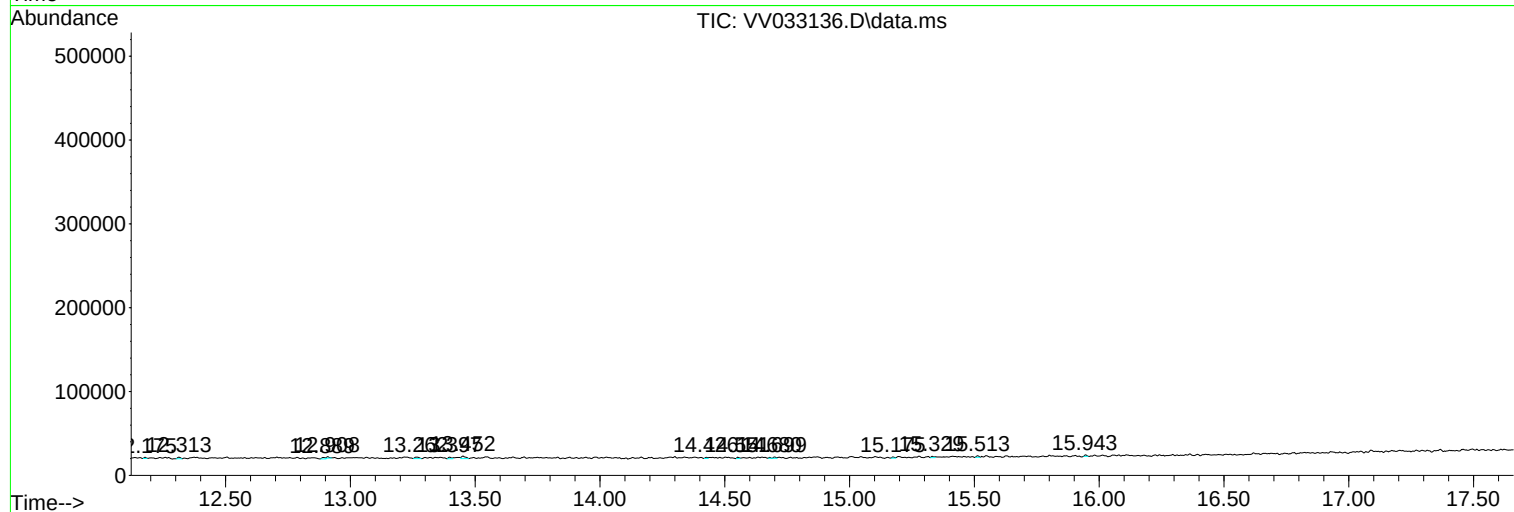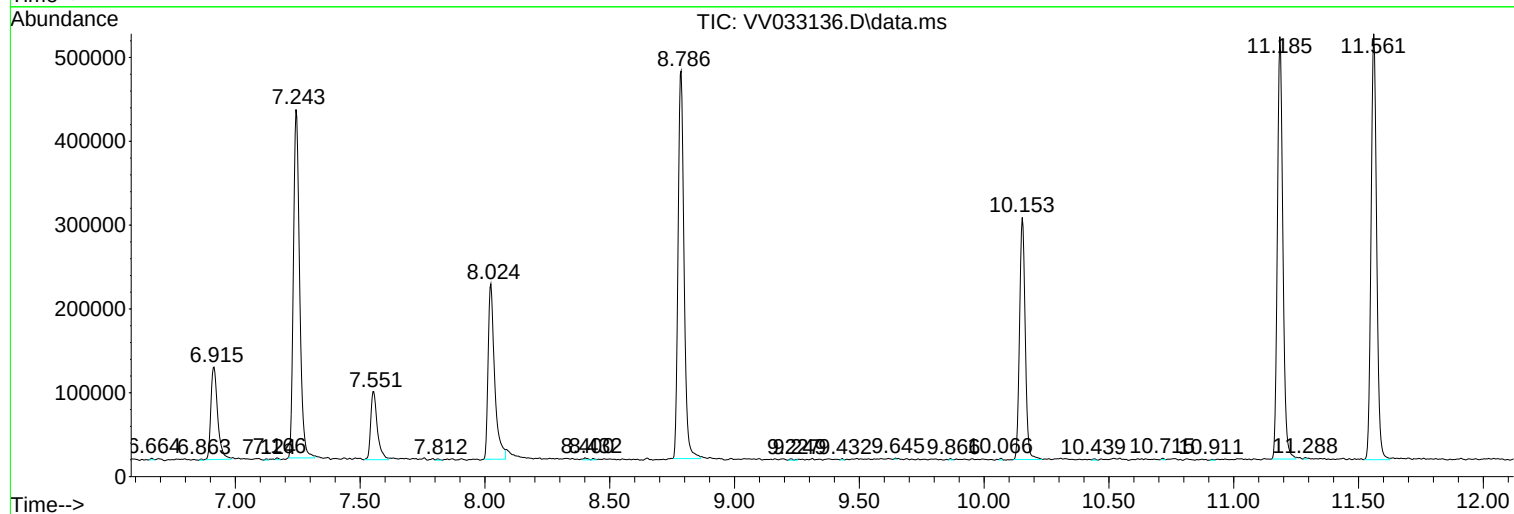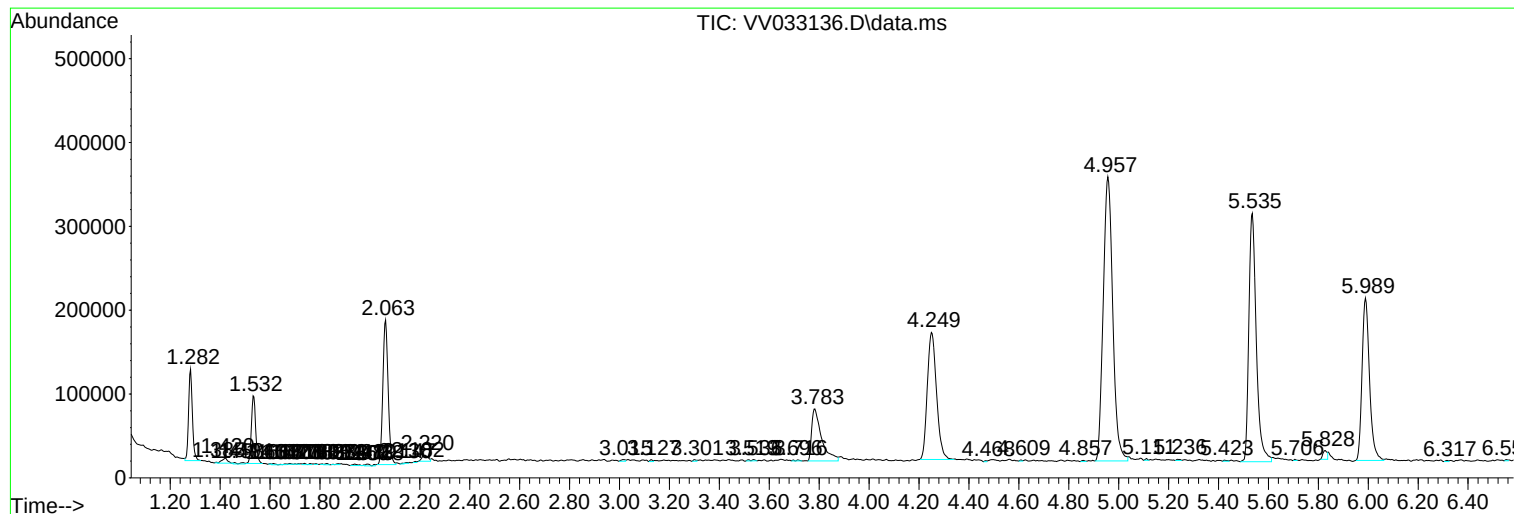

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033136.D
Acq On : 07 Dec 2023 11:10
Operator : SY/MD
Sample : 05645-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033136.D
Acq On : 07 Dec 2023 11:10
Operator : SY/MD
Sample : 05645-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc