

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033137.D
 Acq On : 07 Dec 2023 11:33
 Operator : SY/MD
 Sample : 05645-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	102729	111575	12.78%	1.513%
2	1.423	111	119	126	rVV5	4974	6752	0.77%	0.092%
3	1.452	126	128	133	rVB3	1623	1306	0.15%	0.018%
4	1.532	145	153	172	rVB	79990	97127	11.13%	1.317%
5	1.773	224	228	233	rBV	1201	997	0.11%	0.014%
6	1.802	233	237	242	rBV	1083	1111	0.13%	0.015%
7	1.863	252	256	259	rBV	1227	708	0.08%	0.010%
8	1.937	276	279	284	rVB2	1996	1342	0.15%	0.018%
9	2.060	308	317	332	rBV	162000	237731	27.23%	3.224%
10	2.185	346	356	359	rBV	2427	4136	0.47%	0.056%
11	2.220	359	367	375	rBV	9247	16819	1.93%	0.228%
12	2.288	384	388	390	rBV	1895	1376	0.16%	0.019%
13	2.535	462	465	466	rBV	1644	923	0.11%	0.013%
14	2.561	467	473	480	rVV2	3498	5901	0.68%	0.080%
15	2.645	495	499	501	rBV2	1394	1210	0.14%	0.016%
16	2.860	563	566	570	rBV	1510	1347	0.15%	0.018%
17	3.095	636	639	645	rVB	1723	1274	0.15%	0.017%
18	3.317	706	708	710	rBV	1361	867	0.10%	0.012%
19	3.506	764	767	770	rVB	1570	896	0.10%	0.012%
20	3.603	794	797	800	rBV	1406	781	0.09%	0.011%
21	3.690	820	824	825	rBV2	1896	1224	0.14%	0.017%
22	3.780	844	852	882	rBV	56398	151596	17.37%	2.056%
23	3.918	893	895	899	rBV2	1155	858	0.10%	0.012%
24	4.014	922	925	932	rVB	2248	2228	0.26%	0.030%
25	4.050	932	936	937	rBV2	1892	1361	0.16%	0.018%
26	4.249	982	998	1022	rBV2	146444	373565	42.80%	5.066%
27	4.442	1053	1058	1061	rBV3	1589	1846	0.21%	0.025%
28	4.590	1101	1104	1107	rVB2	1249	878	0.10%	0.012%
29	4.735	1146	1149	1155	rVB	1618	1437	0.16%	0.019%
30	4.957	1202	1218	1245	rBV2	319384	853401	97.77%	11.574%
31	5.114	1265	1267	1272	rVB2	1384	912	0.10%	0.012%
32	5.153	1277	1279	1287	rVB	1692	1557	0.18%	0.021%
33	5.313	1326	1329	1332	rBV2	1274	1028	0.12%	0.014%
34	5.413	1357	1360	1364	rBV2	1194	973	0.11%	0.013%
35	5.532	1384	1397	1425	rBV	330169	685519	78.53%	9.297%
36	5.722	1454	1456	1458	rBV2	1223	751	0.09%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033137.D
 Acq On : 07 Dec 2023 11:33
 Operator : SY/MD
 Sample : 05645-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.834	1480	1491	1510	rBV8	22229	52938	6.06%	0.718%
38	5.989	1526	1539	1566	rBV2	181165	374910	42.95%	5.085%
39	6.207	1604	1607	1608	rBV	1620	951	0.11%	0.013%
40	6.220	1609	1611	1613	rVV	1526	803	0.09%	0.011%
41	6.741	1770	1773	1780	rBV	1401	1610	0.18%	0.022%
42	6.825	1796	1799	1802	rBV	1215	916	0.10%	0.012%
43	6.870	1809	1813	1815	rBV2	1673	1532	0.18%	0.021%
44	6.915	1815	1827	1843	rVV	103423	191235	21.91%	2.594%
45	7.185	1908	1911	1913	rBV	1533	1007	0.12%	0.014%
46	7.243	1918	1929	1950	rBV	391523	684140	78.38%	9.278%
47	7.439	1987	1990	1996	rBV	1678	1917	0.22%	0.026%
48	7.554	2015	2026	2044	rBV	78761	141699	16.23%	1.922%
49	7.934	2140	2144	2151	rBV	2186	2678	0.31%	0.036%
50	8.024	2163	2172	2207	rBV	193675	368565	42.22%	4.999%
51	8.149	2207	2211	2214	rVB	2444	1886	0.22%	0.026%
52	8.278	2245	2251	2254	rBV	1753	1982	0.23%	0.027%
53	8.345	2266	2272	2278	rBV	2019	2852	0.33%	0.039%
54	8.480	2311	2314	2315	rBV2	1239	774	0.09%	0.010%
55	8.715	2384	2387	2392	rBV2	1621	1695	0.19%	0.023%
56	8.783	2398	2408	2433	rBV	517474	861730	98.72%	11.687%
57	8.947	2456	2459	2466	rVB	1784	1378	0.16%	0.019%
58	9.056	2490	2493	2497	rBV2	1152	1130	0.13%	0.015%
59	9.246	2548	2552	2557	rBV	1942	2224	0.25%	0.030%
60	9.397	2596	2599	2602	rVB	1666	883	0.10%	0.012%
61	9.567	2649	2652	2655	rBV	1632	1127	0.13%	0.015%
62	9.606	2661	2664	2666	rBV	1231	843	0.10%	0.011%
63	9.680	2685	2687	2692	rBV2	1101	951	0.11%	0.013%
64	9.744	2705	2707	2710	rBV	1476	988	0.11%	0.013%
65	9.789	2718	2721	2723	rBV	1651	1243	0.14%	0.017%
66	9.866	2742	2745	2748	rBV	1620	1001	0.11%	0.014%
67	10.001	2782	2787	2789	rBV	1758	1810	0.21%	0.025%
68	10.040	2796	2799	2803	rVB	1287	1178	0.13%	0.016%
69	10.152	2823	2834	2855	rVB	274924	435685	49.91%	5.909%
70	10.750	3016	3020	3022	rBV	1471	1279	0.15%	0.017%
71	10.934	3074	3077	3081	rBV	1469	1267	0.15%	0.017%
72	11.050	3110	3113	3116	rBV	1465	1009	0.12%	0.014%
73	11.185	3144	3155	3181	rBV	566462	872888	100.00%	11.838%
74	11.374	3211	3214	3217	rBV	1420	1121	0.13%	0.015%
75	11.416	3225	3227	3230	rBV	1020	829	0.09%	0.011%
76	11.461	3239	3241	3245	rVB	1909	1227	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033137.D
 Acq On : 07 Dec 2023 11:33
 Operator : SY/MD
 Sample : 05645-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.487	3245	3249	3251	rBV	1545	1128	0.13%	0.015%
78	11.500	3251	3253	3260	rVV3	1339	1212	0.14%	0.016%
79	11.561	3260	3272	3291	rBV	473865	745618	85.42%	10.112%
80	11.722	3318	3322	3325	rBV	1546	1457	0.17%	0.020%
81	12.194	3466	3469	3471	rBV	1545	1001	0.11%	0.014%
82	12.316	3504	3507	3511	rBV2	1283	1074	0.12%	0.015%
83	12.603	3593	3596	3605	rVB	2107	2758	0.32%	0.037%
84	12.747	3638	3641	3644	rBV	2267	1266	0.15%	0.017%
85	12.770	3644	3648	3650	rBV	1258	1005	0.12%	0.014%
86	12.995	3715	3718	3723	rVB3	1491	1311	0.15%	0.018%
87	13.024	3724	3727	3730	rVB	1664	1021	0.12%	0.014%
88	13.062	3737	3739	3743	rVB	1880	1108	0.13%	0.015%
89	13.127	3756	3759	3765	rBV2	1581	1803	0.21%	0.024%
90	13.541	3885	3888	3891	rBV	1758	1027	0.12%	0.014%
91	13.689	3930	3934	3937	rBV3	1669	1555	0.18%	0.021%
92	13.754	3952	3954	3959	rVB2	1726	1190	0.14%	0.016%
93	14.455	4169	4172	4175	rBV	1657	1094	0.13%	0.015%
94	14.474	4176	4178	4183	rVB3	1755	1023	0.12%	0.014%
95	14.567	4204	4207	4209	rBV2	1639	1155	0.13%	0.016%
96	15.011	4342	4345	4348	rBV2	1612	1205	0.14%	0.016%
97	15.390	4460	4463	4466	rBV	1621	1110	0.13%	0.015%
98	15.509	4498	4500	4503	rBV	1719	889	0.10%	0.012%
99	15.750	4572	4575	4579	rBV	1713	1125	0.13%	0.015%
100	16.081	4676	4678	4682	rBV4	1383	1081	0.12%	0.015%



Sum of corrected areas: 7373410

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033137.D
Acq On : 07 Dec 2023 11:33
Operator : SY/MD
Sample : 05645-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

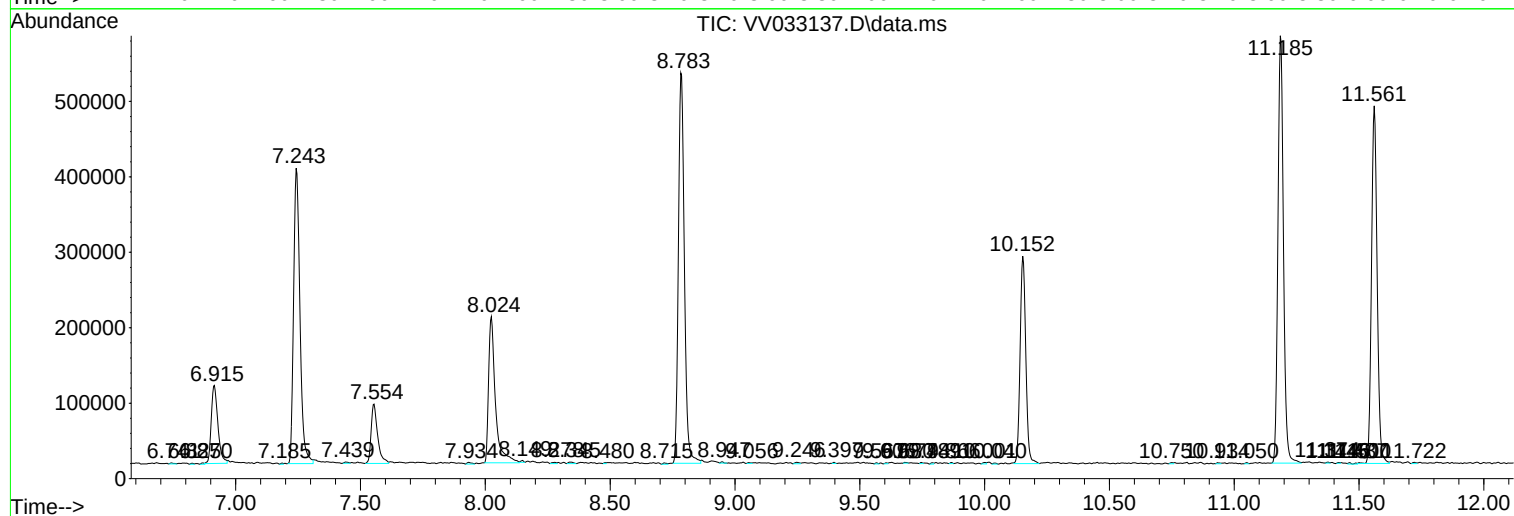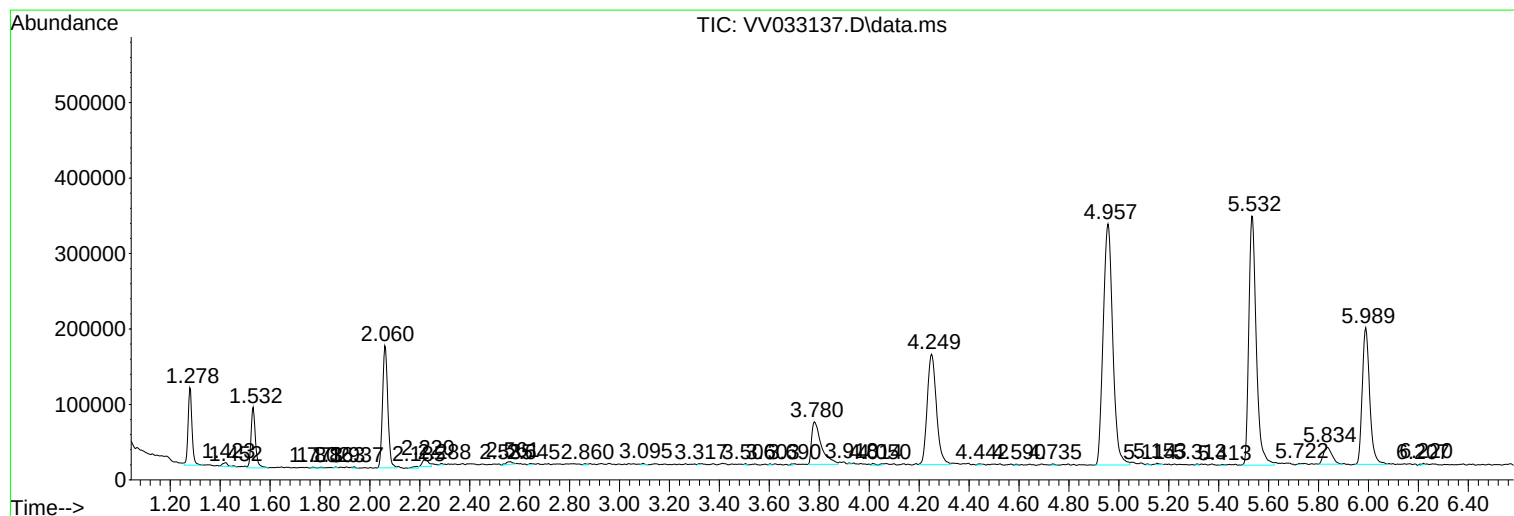

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033137.D
Acq On : 07 Dec 2023 11:33
Operator : SY/MD
Sample : 05645-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033137.D
Acq On : 07 Dec 2023 11:33
Operator : SY/MD
Sample : 05645-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc