

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033138.D
 Acq On : 07 Dec 2023 11:57
 Operator : SY/MD
 Sample : 05645-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033138.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rVB	100775	110424	13.35%	1.555%
2	1.417	111	117	127	rVB3	4706	7053	0.85%	0.099%
3	1.462	127	131	138	rVB2	1223	1247	0.15%	0.018%
4	1.532	144	153	166	rVB	78275	94390	11.41%	1.329%
5	1.629	180	183	186	rBV3	1091	732	0.09%	0.010%
6	1.851	248	252	258	rBV2	1057	1178	0.14%	0.017%
7	1.883	258	262	265	rVV2	1017	966	0.12%	0.014%
8	1.902	265	268	274	rVB4	1128	918	0.11%	0.013%
9	2.011	298	302	307	rBV	1126	903	0.11%	0.013%
10	2.060	307	317	330	rBV	158071	236340	28.56%	3.328%
11	2.111	330	333	338	rVB2	2180	2296	0.28%	0.032%
12	2.156	342	347	350	rBV	1957	1698	0.21%	0.024%
13	2.195	350	359	360	rBV2	3013	3225	0.39%	0.045%
14	2.217	362	366	369	rBV4	4197	3866	0.47%	0.054%
15	2.349	404	407	411	rBV	1783	1767	0.21%	0.025%
16	2.690	510	513	516	rBV	1693	1375	0.17%	0.019%
17	2.777	537	540	543	rBV	1263	998	0.12%	0.014%
18	2.815	548	552	555	rBV	2082	1832	0.22%	0.026%
19	2.909	579	581	587	rVB	1271	1311	0.16%	0.018%
20	3.095	636	639	640	rBV	1484	839	0.10%	0.012%
21	3.307	700	705	709	rBV	1479	1842	0.22%	0.026%
22	3.783	844	853	881	rBV	51195	134759	16.29%	1.898%
23	4.150	963	967	972	rBV	1995	2540	0.31%	0.036%
24	4.249	980	998	1025	rBV2	142841	371363	44.88%	5.229%
25	4.404	1043	1046	1052	rBV2	2020	1674	0.20%	0.024%
26	4.616	1109	1112	1115	rBV2	1479	1097	0.13%	0.015%
27	4.744	1149	1152	1160	rVB	1655	1750	0.21%	0.025%
28	4.783	1161	1164	1166	rBV2	1370	1037	0.13%	0.015%
29	4.957	1202	1218	1246	rBV3	312391	825257	99.73%	11.621%
30	5.304	1324	1326	1329	rVB	1795	1021	0.12%	0.014%
31	5.413	1358	1360	1363	rBV	1309	712	0.09%	0.010%
32	5.535	1386	1398	1423	rBV	313699	652671	78.88%	9.191%
33	5.751	1463	1465	1467	rBV	1498	866	0.10%	0.012%
34	5.831	1481	1490	1503	rBV3	10879	20539	2.48%	0.289%
35	5.989	1527	1539	1562	rBV	176889	365878	44.22%	5.152%
36	6.133	1582	1584	1587	rBV4	1416	946	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033138.D
 Acq On : 07 Dec 2023 11:57
 Operator : SY/MD
 Sample : 05645-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.304	1634	1637	1641	rVB2	1099	712	0.09%	0.010%
38	6.416	1670	1672	1676	rVB2	1475	884	0.11%	0.012%
39	6.619	1732	1735	1738	rVV	1160	902	0.11%	0.013%
40	6.670	1748	1751	1756	rBV	1484	1332	0.16%	0.019%
41	6.728	1766	1769	1771	rVB	1496	790	0.10%	0.011%
42	6.912	1817	1826	1854	rBV	101034	194670	23.53%	2.741%
43	7.243	1918	1929	1952	rBV	377047	665404	80.42%	9.370%
44	7.387	1971	1974	1977	rVB	2036	1119	0.14%	0.016%
45	7.555	2016	2026	2040	rBV2	75795	133720	16.16%	1.883%
46	7.670	2059	2062	2064	rBV2	1506	908	0.11%	0.013%
47	7.838	2112	2114	2116	rBV	1097	666	0.08%	0.009%
48	7.879	2124	2127	2130	rBV	1702	926	0.11%	0.013%
49	7.940	2144	2146	2153	rBV	1234	1034	0.12%	0.015%
50	8.024	2163	2172	2199	rBV	172379	326931	39.51%	4.604%
51	8.506	2320	2322	2326	rVB	1279	751	0.09%	0.011%
52	8.783	2398	2408	2436	rBV	494506	816380	98.66%	11.496%
53	8.905	2443	2446	2449	rBV2	1605	1030	0.12%	0.015%
54	8.976	2464	2468	2472	rVB2	1421	1249	0.15%	0.018%
55	9.516	2633	2636	2638	rBV	1270	748	0.09%	0.011%
56	9.821	2728	2731	2733	rBV2	1117	832	0.10%	0.012%
57	9.899	2752	2755	2762	rVB4	2661	2431	0.29%	0.034%
58	9.940	2766	2768	2776	rVB3	1657	1815	0.22%	0.026%
59	9.976	2776	2779	2783	rBV	2025	2199	0.27%	0.031%
60	10.153	2815	2834	2855	rBV	266244	427056	51.61%	6.014%
61	10.490	2937	2939	2941	rBV	1211	778	0.09%	0.011%
62	10.503	2941	2943	2946	rVB	1568	942	0.11%	0.013%
63	10.632	2978	2983	2986	rBV	1218	1371	0.17%	0.019%
64	11.104	3128	3130	3133	rBV2	1059	874	0.11%	0.012%
65	11.185	3144	3155	3185	rBV	533184	827453	100.00%	11.652%
66	11.313	3192	3195	3199	rBV2	1579	1176	0.14%	0.017%
67	11.461	3238	3241	3243	rBV	1138	895	0.11%	0.013%
68	11.561	3260	3272	3287	rBV	463604	728099	87.99%	10.253%
69	11.651	3298	3300	3306	rVB	2431	1989	0.24%	0.028%
70	11.847	3357	3361	3364	rBV2	1241	1240	0.15%	0.017%
71	11.947	3384	3392	3403	rBV3	13657	23502	2.84%	0.331%
72	12.130	3444	3449	3452	rBV2	1629	1810	0.22%	0.025%
73	12.149	3452	3455	3458	rVV	1511	975	0.12%	0.014%
74	12.188	3462	3467	3477	rVV3	6777	10009	1.21%	0.141%
75	12.365	3520	3522	3529	rVB2	1821	1889	0.23%	0.027%
76	12.532	3570	3574	3578	rBV	1987	1906	0.23%	0.027%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033138.D
 Acq On : 07 Dec 2023 11:57
 Operator : SY/MD
 Sample : 05645-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.554	3579	3581	3585	rVV3	1191	853	0.10%	0.012%
78	12.844	3668	3671	3676	rVB	1598	1320	0.16%	0.019%
79	12.873	3677	3680	3682	rBV	1498	1069	0.13%	0.015%
80	12.982	3710	3714	3716	rBV	1420	1271	0.15%	0.018%
81	13.207	3781	3784	3787	rVB	1690	925	0.11%	0.013%
82	13.429	3849	3853	3854	rBV	2080	1433	0.17%	0.020%
83	13.728	3942	3946	3948	rBV	1581	1135	0.14%	0.016%
84	13.747	3948	3952	3955	rBV4	1186	1252	0.15%	0.018%
85	13.783	3960	3963	3965	rBV	1392	937	0.11%	0.013%
86	13.915	4001	4004	4009	rVB	1953	1450	0.18%	0.020%
87	14.005	4029	4032	4034	rBV	1488	1054	0.13%	0.015%
88	14.056	4045	4048	4050	rBV	1283	709	0.09%	0.010%
89	14.124	4067	4069	4074	rBV	1222	1023	0.12%	0.014%
90	14.349	4130	4139	4148	rVB8	15881	26089	3.15%	0.367%
91	14.448	4167	4170	4174	rBV	2274	2020	0.24%	0.028%
92	14.468	4174	4176	4178	rBV	1210	747	0.09%	0.011%
93	14.529	4193	4195	4202	rVB5	2167	2111	0.26%	0.030%
94	14.628	4223	4226	4230	rBV3	1428	1251	0.15%	0.018%
95	14.683	4240	4243	4245	rBV	1411	806	0.10%	0.011%
96	15.004	4341	4343	4345	rBV	1045	690	0.08%	0.010%
97	15.722	4563	4566	4570	rBV2	1320	1314	0.16%	0.019%
98	15.779	4579	4584	4588	rBV3	2193	2610	0.32%	0.037%
99	16.062	4670	4672	4675	rBV	1641	1132	0.14%	0.016%
100	16.278	4737	4739	4745	rBV	1809	1673	0.20%	0.024%


Sum of corrected areas: 7101581

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033138.D
Acq On : 07 Dec 2023 11:57
Operator : SY/MD
Sample : 05645-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

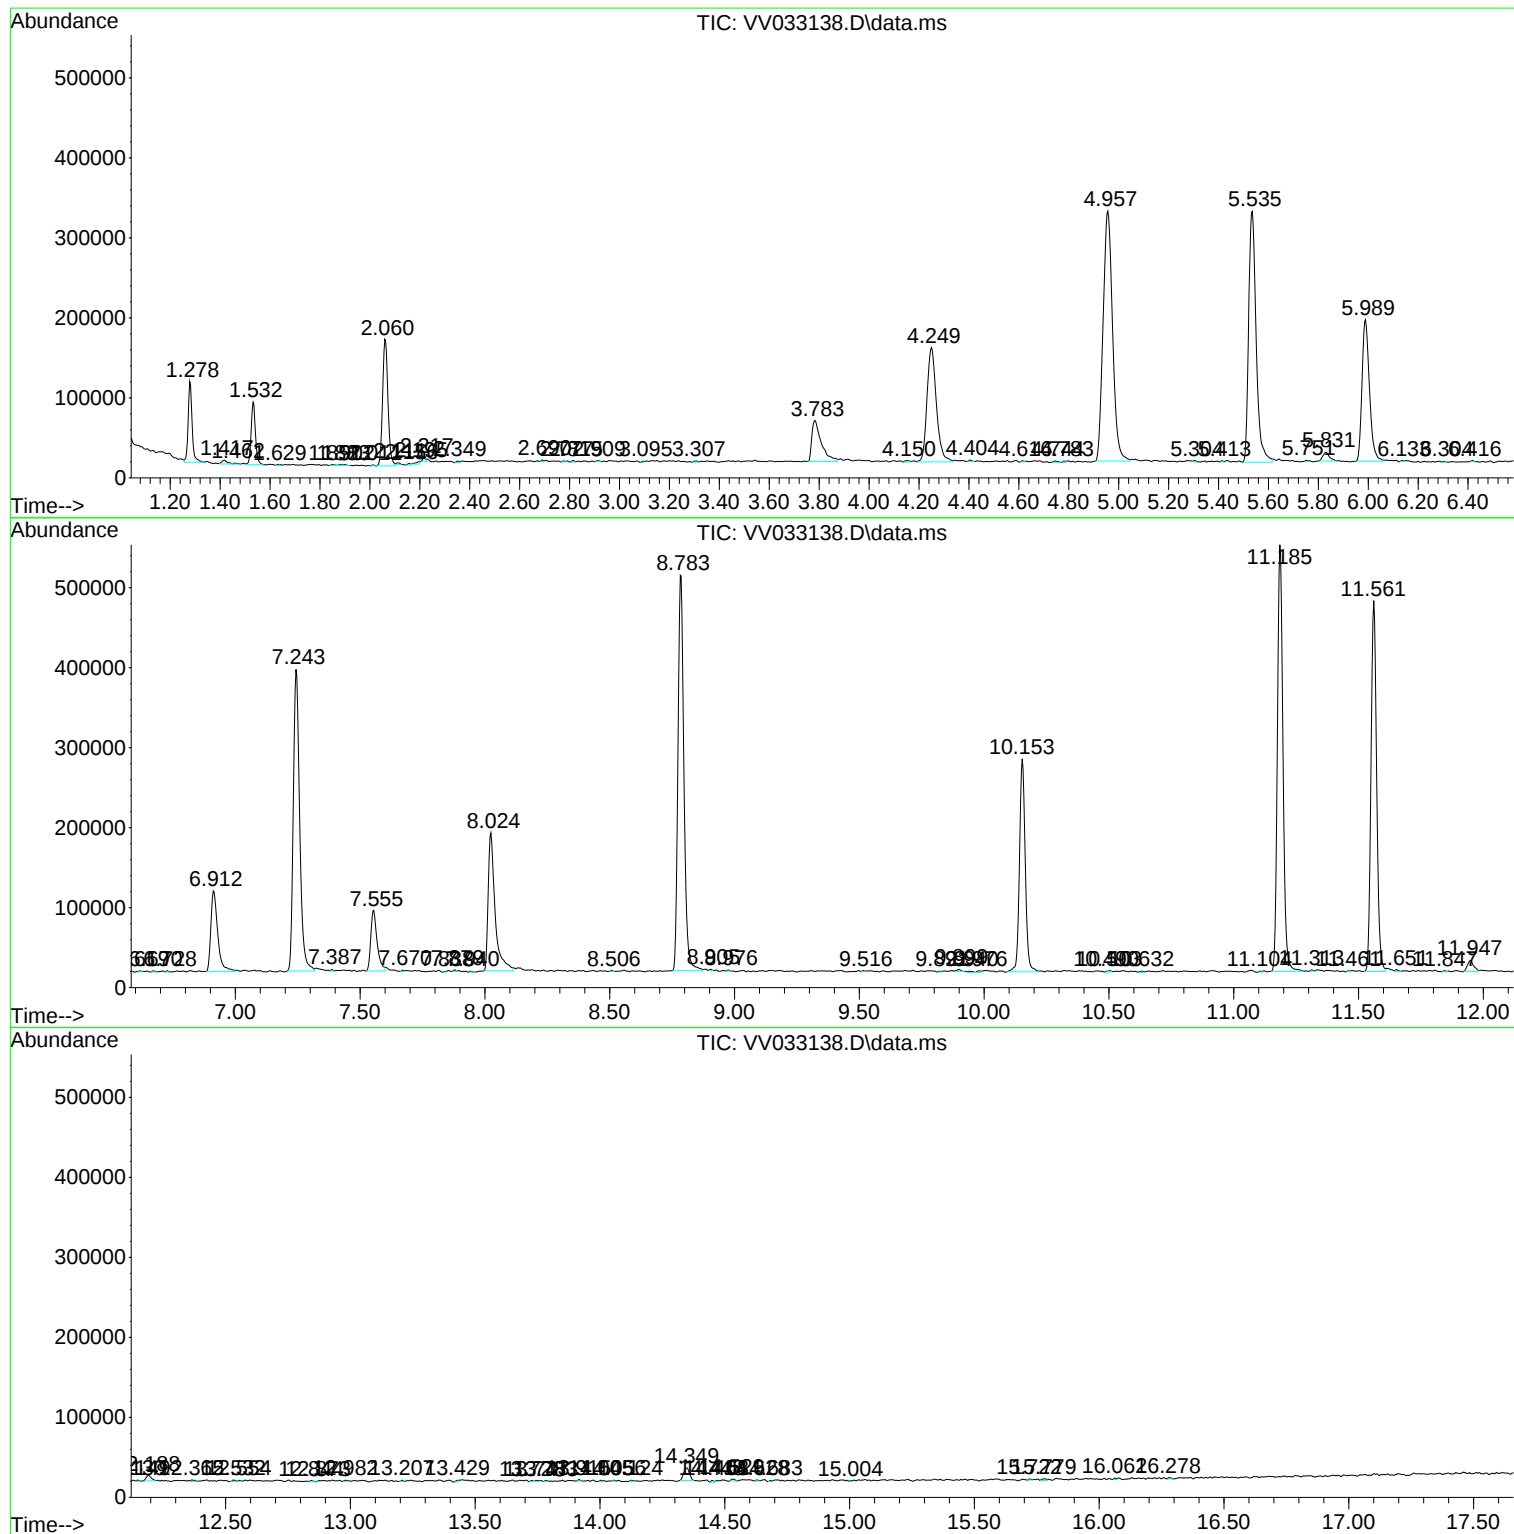

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033138.D
Acq On : 07 Dec 2023 11:57
Operator : SY/MD
Sample : 05645-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033138.D
Acq On : 07 Dec 2023 11:57
Operator : SY/MD
Sample : 05645-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------