

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033139.D
 Acq On : 07 Dec 2023 12:20
 Operator : SY/MD
 Sample : 05645-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033139.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rVB	102587	105311	12.42%	1.465%
2	1.417	110	117	125	rBV	4404	5636	0.66%	0.078%
3	1.500	140	143	145	rBV2	766	505	0.06%	0.007%
4	1.532	145	153	167	rVB	78069	94073	11.09%	1.309%
5	1.593	167	172	175	rVB2	1093	1081	0.13%	0.015%
6	1.642	184	187	188	rBV	740	366	0.04%	0.005%
7	1.651	188	190	193	rVB	1133	651	0.08%	0.009%
8	1.671	193	196	199	rBV2	989	651	0.08%	0.009%
9	1.761	221	224	227	rVB2	733	460	0.05%	0.006%
10	1.802	233	237	240	rBV	886	601	0.07%	0.008%
11	1.828	240	245	248	rBV2	1148	958	0.11%	0.013%
12	1.876	256	260	263	rVB2	717	586	0.07%	0.008%
13	1.892	263	265	268	rBV	589	399	0.05%	0.006%
14	1.918	270	273	277	rBV	1402	1143	0.13%	0.016%
15	1.937	277	279	281	rVB	895	411	0.05%	0.006%
16	1.960	284	286	289	rVB	1160	698	0.08%	0.010%
17	1.986	289	294	297	rBV2	800	773	0.09%	0.011%
18	2.005	297	300	302	rBV4	811	477	0.06%	0.007%
19	2.060	307	317	328	rBV	160122	234884	27.70%	3.268%
20	2.111	328	333	343	rVB2	8108	11315	1.33%	0.157%
21	2.172	343	352	355	rBV	2168	3213	0.38%	0.045%
22	2.198	355	360	361	rBV2	2336	1956	0.23%	0.027%
23	2.214	361	365	367	rBV2	2832	2375	0.28%	0.033%
24	2.272	379	383	385	rBV2	1934	1405	0.17%	0.020%
25	2.423	427	430	431	rBV	1116	685	0.08%	0.010%
26	2.449	436	438	441	rBV2	1065	626	0.07%	0.009%
27	2.519	457	460	462	rBV	1791	991	0.12%	0.014%
28	2.754	530	533	535	rBV	1116	721	0.09%	0.010%
29	3.783	844	853	881	rBV	49719	135600	15.99%	1.887%
30	4.249	983	998	1020	rBV	143083	365719	43.13%	5.088%
31	4.664	1124	1127	1129	rBV2	1140	801	0.09%	0.011%
32	4.754	1152	1155	1160	rBV	1419	1436	0.17%	0.020%
33	4.799	1167	1169	1170	rBV	1271	600	0.07%	0.008%
34	4.957	1202	1218	1241	rBV2	313125	835167	98.50%	11.619%
35	5.095	1258	1261	1268	rVB	2438	2893	0.34%	0.040%
36	5.416	1358	1361	1364	rBV	1331	786	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033139.D
 Acq On : 07 Dec 2023 12:20
 Operator : SY/MD
 Sample : 05645-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.439	1364	1368	1372	rBV	1673	1581	0.19%	0.022%
38	5.532	1387	1397	1428	rBV	321681	664158	78.33%	9.240%
39	5.667	1437	1439	1442	rBV	1054	675	0.08%	0.009%
40	5.796	1477	1479	1481	rBV	1255	821	0.10%	0.011%
41	5.834	1482	1491	1510	rVB8	19837	47782	5.64%	0.665%
42	5.989	1525	1539	1563	rBV	182828	383291	45.21%	5.333%
43	6.301	1633	1636	1639	rBV	1289	1015	0.12%	0.014%
44	6.403	1666	1668	1670	rBV	931	518	0.06%	0.007%
45	6.664	1746	1749	1751	rBV	1892	1194	0.14%	0.017%
46	6.911	1814	1826	1847	rBV	103911	192851	22.74%	2.683%
47	6.985	1847	1849	1859	rVB	2659	3515	0.41%	0.049%
48	7.098	1881	1884	1887	rBV	1754	1189	0.14%	0.017%
49	7.133	1892	1895	1899	rBV2	1914	1638	0.19%	0.023%
50	7.243	1918	1929	1946	rBV	388735	677589	79.91%	9.427%
51	7.555	2017	2026	2041	rBV	74604	136081	16.05%	1.893%
52	7.805	2101	2104	2106	rBV	1327	822	0.10%	0.011%
53	7.850	2114	2118	2121	rVB2	1509	1314	0.15%	0.018%
54	8.024	2163	2172	2204	rBV	180036	348120	41.06%	4.843%
55	8.207	2227	2229	2233	rBV3	1420	758	0.09%	0.011%
56	8.661	2368	2370	2373	rBV	1049	640	0.08%	0.009%
57	8.741	2392	2395	2398	rBV2	1245	1030	0.12%	0.014%
58	8.783	2398	2408	2428	rBV	504337	833698	98.33%	11.599%
59	9.127	2510	2515	2520	rBV2	1772	2601	0.31%	0.036%
60	9.278	2560	2562	2565	rBV	1341	1134	0.13%	0.016%
61	9.294	2565	2567	2571	rVB	1753	1184	0.14%	0.016%
62	9.487	2625	2627	2633	rVB	1989	1861	0.22%	0.026%
63	9.715	2695	2698	2701	rBV	1726	1451	0.17%	0.020%
64	9.780	2715	2718	2721	rBV	1222	797	0.09%	0.011%
65	10.153	2824	2834	2852	rVB	266002	423045	49.89%	5.886%
66	10.271	2868	2871	2875	rBV2	1850	1506	0.18%	0.021%
67	10.542	2953	2955	2961	rVB	1389	896	0.11%	0.012%
68	10.590	2967	2970	2972	rBV	1369	789	0.09%	0.011%
69	10.661	2989	2992	2995	rBV2	1562	1152	0.14%	0.016%
70	10.783	3027	3030	3032	rBV	1301	782	0.09%	0.011%
71	11.185	3145	3155	3174	rBV	555164	847891	100.00%	11.796%
72	11.455	3236	3239	3242	rBV	1136	911	0.11%	0.013%
73	11.561	3260	3272	3288	rBV	469942	742715	87.60%	10.333%
74	11.709	3315	3318	3319	rBV2	1793	981	0.12%	0.014%
75	11.738	3324	3327	3330	rBV2	1204	1132	0.13%	0.016%
76	11.879	3367	3371	3375	rBV	1339	1239	0.15%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033139.D
 Acq On : 07 Dec 2023 12:20
 Operator : SY/MD
 Sample : 05645-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.143	3450	3453	3456	rBV	1725	1271	0.15%	0.018%
78	12.191	3466	3468	3470	rBV	1030	611	0.07%	0.009%
79	12.300	3499	3502	3504	rVB	1473	801	0.09%	0.011%
80	12.513	3565	3568	3571	rVB	1565	1065	0.13%	0.015%
81	12.580	3587	3589	3595	rVB	1926	1296	0.15%	0.018%
82	12.641	3605	3608	3618	rVB	1732	2110	0.25%	0.029%
83	12.705	3625	3628	3631	rBV	1593	1268	0.15%	0.018%
84	12.831	3664	3667	3670	rBV	1568	1113	0.13%	0.015%
85	13.046	3732	3734	3739	rVB3	1055	553	0.07%	0.008%
86	13.201	3780	3782	3788	rBV3	1324	1381	0.16%	0.019%
87	13.464	3862	3864	3868	rBV	1209	983	0.12%	0.014%
88	13.612	3907	3910	3912	rBV	1228	713	0.08%	0.010%
89	13.654	3921	3923	3925	rBV2	1048	688	0.08%	0.010%
90	13.705	3937	3939	3942	rVB	1281	655	0.08%	0.009%
91	13.882	3991	3994	3999	rVB	1740	1367	0.16%	0.019%
92	13.908	3999	4002	4004	rBV	1361	879	0.10%	0.012%
93	14.162	4079	4081	4085	rBV2	1260	1094	0.13%	0.015%
94	14.345	4132	4138	4148	rBV8	9033	12959	1.53%	0.180%
95	14.606	4217	4219	4225	rBV	1412	1148	0.14%	0.016%
96	14.792	4274	4277	4279	rBV	1802	1203	0.14%	0.017%
97	14.963	4327	4330	4335	rVB	1927	1357	0.16%	0.019%
98	15.065	4359	4362	4365	rBV	2023	1473	0.17%	0.020%
99	15.538	4506	4509	4512	rBV	1617	1099	0.13%	0.015%
100	16.200	4709	4715	4717	rBV5	2144	2270	0.27%	0.032%




Sum of corrected areas: 7187657

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033139.D
Acq On : 07 Dec 2023 12:20
Operator : SY/MD
Sample : 05645-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

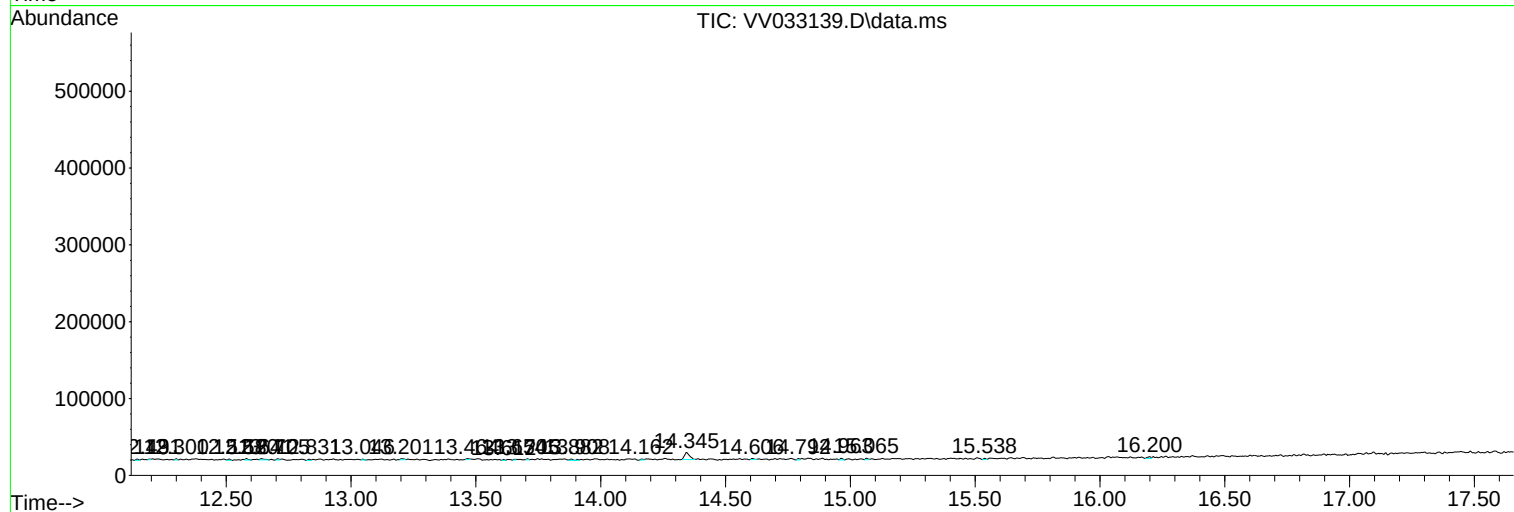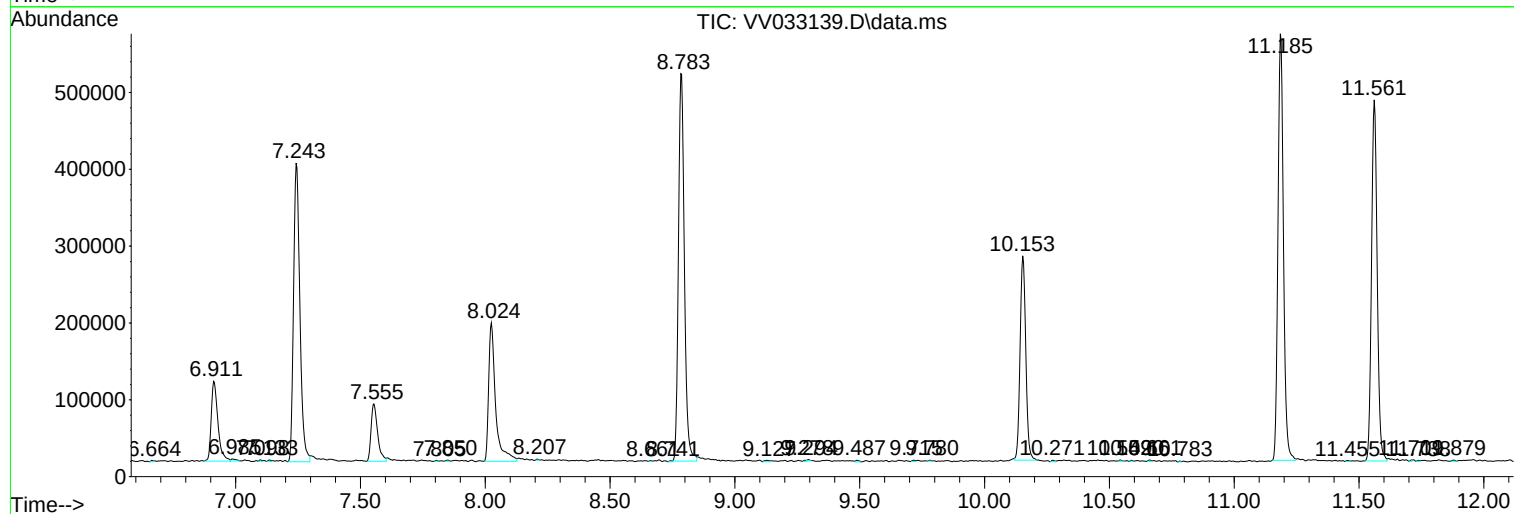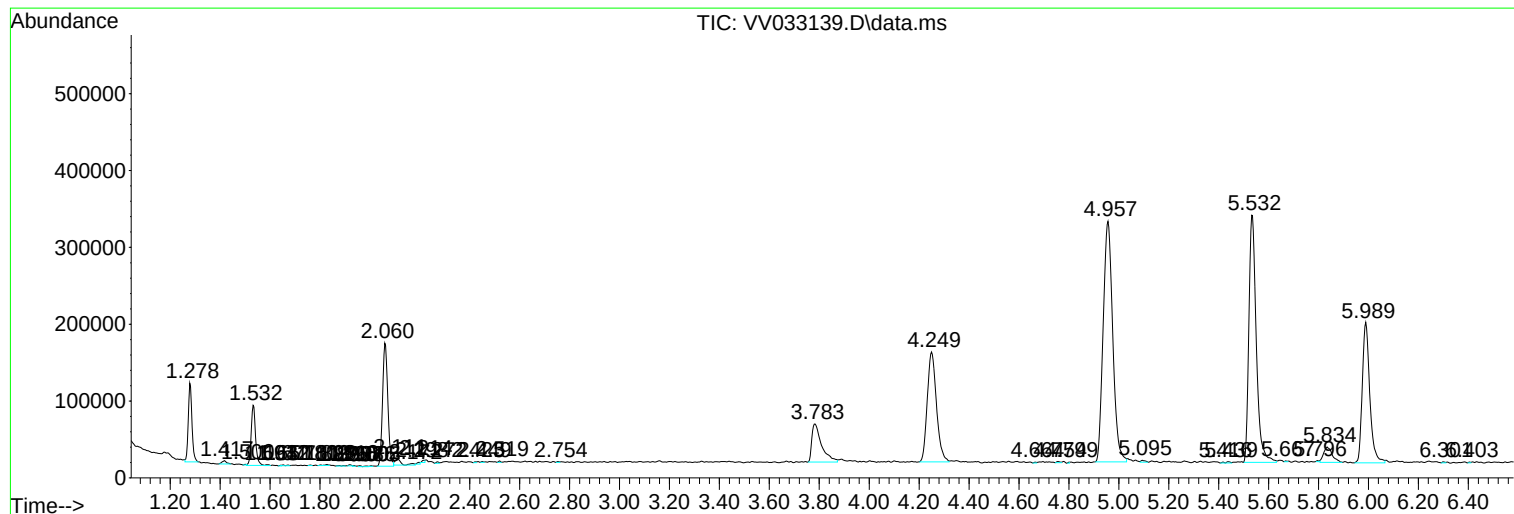

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033139.D
Acq On : 07 Dec 2023 12:20
Operator : SY/MD
Sample : 05645-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033139.D
Acq On : 07 Dec 2023 12:20
Operator : SY/MD
Sample : 05645-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc