

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033140.D
 Acq On : 07 Dec 2023 12:43
 Operator : SY/MD
 Sample : 05645-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033140.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	88	rVB	101209	108497	12.69%	1.495%
2	1.394	107	110	111	rBV	1940	1060	0.12%	0.015%
3	1.445	123	126	129	rVB	1455	945	0.11%	0.013%
4	1.468	129	133	134	rVV	1224	824	0.10%	0.011%
5	1.478	134	136	143	rVV4	1682	2143	0.25%	0.030%
6	1.532	143	153	166	rVB	78342	94174	11.02%	1.298%
7	1.635	180	185	190	rVB	1633	1979	0.23%	0.027%
8	1.677	194	198	200	rBV2	1145	962	0.11%	0.013%
9	1.757	221	223	229	rVB	1230	893	0.10%	0.012%
10	1.915	268	272	273	rBV	1273	791	0.09%	0.011%
11	1.924	273	275	279	rVB2	1565	1061	0.12%	0.015%
12	2.008	296	301	304	rBV2	882	665	0.08%	0.009%
13	2.060	304	317	331	rBV	161186	239830	28.05%	3.305%
14	2.111	331	333	339	rVB3	1134	1012	0.12%	0.014%
15	2.166	344	350	351	rBV	877	820	0.10%	0.011%
16	2.201	352	361	363	rBV	3771	4805	0.56%	0.066%
17	2.220	363	367	369	rBV2	1343	1113	0.13%	0.015%
18	2.301	389	392	397	rBV2	1649	1735	0.20%	0.024%
19	2.497	450	453	455	rBV	1283	945	0.11%	0.013%
20	2.741	526	529	532	rBV	1728	1420	0.17%	0.020%
21	2.777	537	540	542	rBV	1200	685	0.08%	0.009%
22	2.912	579	582	584	rBV	1649	1212	0.14%	0.017%
23	3.037	617	621	622	rBV	1488	1070	0.13%	0.015%
24	3.288	696	699	704	rBV2	1163	1187	0.14%	0.016%
25	3.310	704	706	710	rVB	1132	719	0.08%	0.010%
26	3.494	759	763	764	rBV	1815	1262	0.15%	0.017%
27	3.526	770	773	775	rBV	1649	1030	0.12%	0.014%
28	3.783	844	853	881	rBV	53514	145912	17.07%	2.011%
29	3.908	889	892	895	rBV2	1620	1048	0.12%	0.014%
30	4.101	949	952	955	rBV3	1010	754	0.09%	0.010%
31	4.249	984	998	1019	rBV	146159	369050	43.17%	5.086%
32	4.735	1146	1149	1152	rBV	1171	838	0.10%	0.012%
33	4.957	1201	1218	1240	rBV2	317074	854939	100.00%	11.782%
34	5.223	1299	1301	1305	rVB	1988	1195	0.14%	0.016%
35	5.246	1305	1308	1311	rBV	1679	1190	0.14%	0.016%
36	5.278	1315	1318	1321	rBV	1638	967	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033140.D
 Acq On : 07 Dec 2023 12:43
 Operator : SY/MD
 Sample : 05645-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.426	1361	1364	1367	rBV	1708	1507	0.18%	0.021%
38	5.532	1385	1397	1422	rBV	316641	660677	77.28%	9.105%
39	5.828	1479	1489	1505	rBV5	11789	28189	3.30%	0.388%
40	5.989	1527	1539	1558	rBV	183472	372949	43.62%	5.139%
41	6.510	1698	1701	1704	rBV	1355	1078	0.13%	0.015%
42	6.747	1772	1775	1777	rBV	1704	1090	0.13%	0.015%
43	6.911	1816	1826	1849	rBV	107043	200912	23.50%	2.769%
44	7.243	1919	1929	1951	rBV	384757	685599	80.19%	9.448%
45	7.554	2016	2026	2045	rBV	76186	138083	16.15%	1.903%
46	7.808	2102	2105	2109	rVB	1776	1087	0.13%	0.015%
47	8.024	2163	2172	2212	rBV	196880	380515	44.51%	5.244%
48	8.223	2232	2234	2239	rBV2	1479	884	0.10%	0.012%
49	8.352	2271	2274	2279	rBV	1552	1432	0.17%	0.020%
50	8.522	2322	2327	2330	rBV	1509	1920	0.22%	0.026%
51	8.667	2369	2372	2377	rBV	1291	1251	0.15%	0.017%
52	8.783	2397	2408	2427	rBV	511703	835806	97.76%	11.518%
53	9.249	2550	2553	2556	rBV	962	739	0.09%	0.010%
54	9.426	2606	2608	2611	rBV	1267	963	0.11%	0.013%
55	9.509	2631	2634	2638	rBV2	1469	1073	0.13%	0.015%
56	9.821	2729	2731	2733	rBV	1095	682	0.08%	0.009%
57	9.902	2752	2756	2760	rBV	1462	1517	0.18%	0.021%
58	10.021	2790	2793	2794	rBV	1328	768	0.09%	0.011%
59	10.152	2823	2834	2856	rBV	278267	440091	51.48%	6.065%
60	10.368	2898	2901	2906	rBV2	1120	1102	0.13%	0.015%
61	10.419	2914	2917	2920	rBV	1156	960	0.11%	0.013%
62	10.487	2935	2938	2943	rBV2	1467	1576	0.18%	0.022%
63	10.535	2948	2953	2957	rBV	2616	3113	0.36%	0.043%
64	10.667	2989	2994	2998	rVB2	1576	1683	0.20%	0.023%
65	10.693	2999	3002	3005	rBV	1340	1079	0.13%	0.015%
66	10.805	3033	3037	3040	rVB	1467	1187	0.14%	0.016%
67	10.834	3042	3046	3050	rBV	1701	1843	0.22%	0.025%
68	10.886	3059	3062	3063	rBV	1234	790	0.09%	0.011%
69	11.011	3098	3101	3103	rBV2	1259	1045	0.12%	0.014%
70	11.043	3109	3111	3114	rVB	1309	716	0.08%	0.010%
71	11.127	3134	3137	3140	rBV	1075	816	0.10%	0.011%
72	11.185	3145	3155	3173	rVV	547186	842655	98.56%	11.612%
73	11.271	3179	3182	3188	rVB	2190	1613	0.19%	0.022%
74	11.484	3245	3248	3254	rBV	2171	1712	0.20%	0.024%
75	11.561	3260	3272	3293	rBV	482057	758167	88.68%	10.448%
76	11.789	3339	3343	3346	rBV	1733	1281	0.15%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033140.D
 Acq On : 07 Dec 2023 12:43
 Operator : SY/MD
 Sample : 05645-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.217	3473	3476	3477	rBV	1209	748	0.09%	0.010%
78	12.252	3484	3487	3490	rBV	1603	1160	0.14%	0.016%
79	12.316	3504	3507	3512	rBV2	1174	742	0.09%	0.010%
80	12.381	3524	3527	3531	rBV2	1224	972	0.11%	0.013%
81	12.554	3578	3581	3584	rBV	1296	953	0.11%	0.013%
82	12.628	3601	3604	3608	rBV	1536	1121	0.13%	0.015%
83	12.654	3609	3612	3614	rBV	1532	997	0.12%	0.014%
84	12.709	3627	3629	3631	rBV2	1260	703	0.08%	0.010%
85	12.921	3693	3695	3700	rVB	1477	1256	0.15%	0.017%
86	12.959	3704	3707	3710	rBV	1893	1125	0.13%	0.016%
87	12.992	3715	3717	3719	rBV	1189	719	0.08%	0.010%
88	13.255	3795	3799	3806	rBV	2161	2391	0.28%	0.033%
89	13.291	3807	3810	3814	rVB	1479	1228	0.14%	0.017%
90	13.365	3830	3833	3835	rBV2	1468	1083	0.13%	0.015%
91	13.445	3856	3858	3860	rBV	1294	797	0.09%	0.011%
92	13.786	3961	3964	3967	rBV	1722	1345	0.16%	0.019%
93	14.072	4049	4053	4056	rBV3	1670	1661	0.19%	0.023%
94	14.274	4114	4116	4119	rBV	1282	801	0.09%	0.011%
95	14.660	4234	4236	4238	rBV2	1132	708	0.08%	0.010%
96	14.725	4254	4256	4262	rVB	1738	1258	0.15%	0.017%
97	15.278	4425	4428	4429	rBV3	1361	848	0.10%	0.012%
98	15.522	4501	4504	4506	rBV	1504	990	0.12%	0.014%
99	16.101	4681	4684	4688	rVB2	2501	1820	0.21%	0.025%
100	17.339	5067	5069	5075	rVB6	3312	2279	0.27%	0.031%




Sum of corrected areas: 7256587

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033140.D
Acq On : 07 Dec 2023 12:43
Operator : SY/MD
Sample : 05645-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

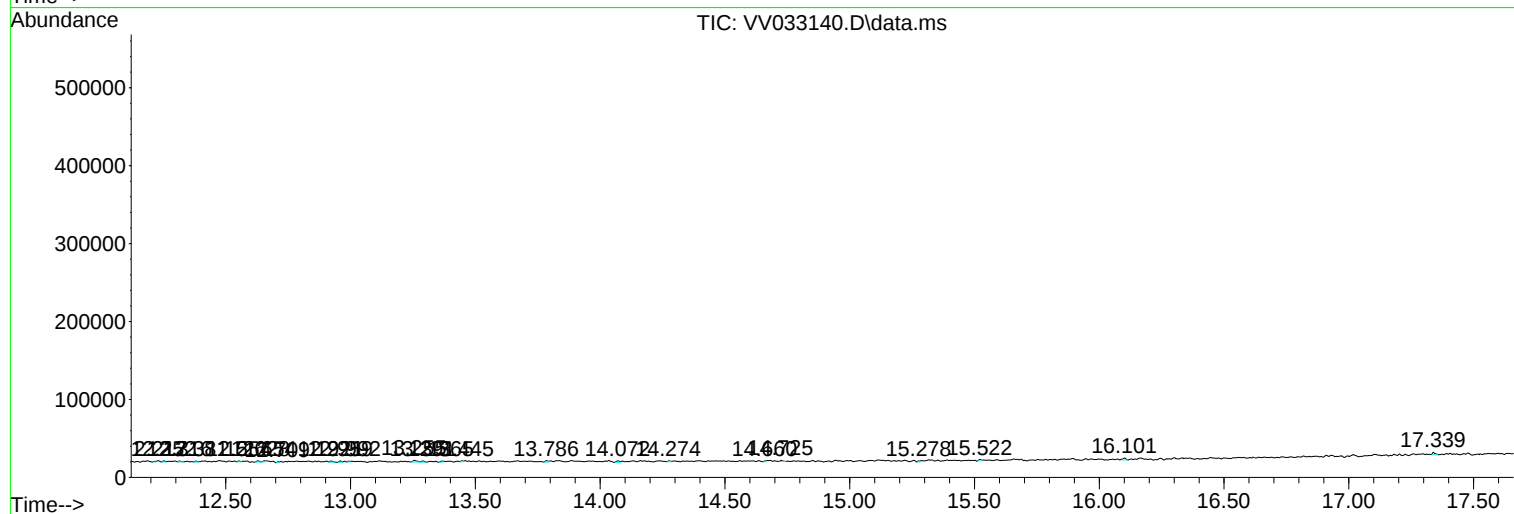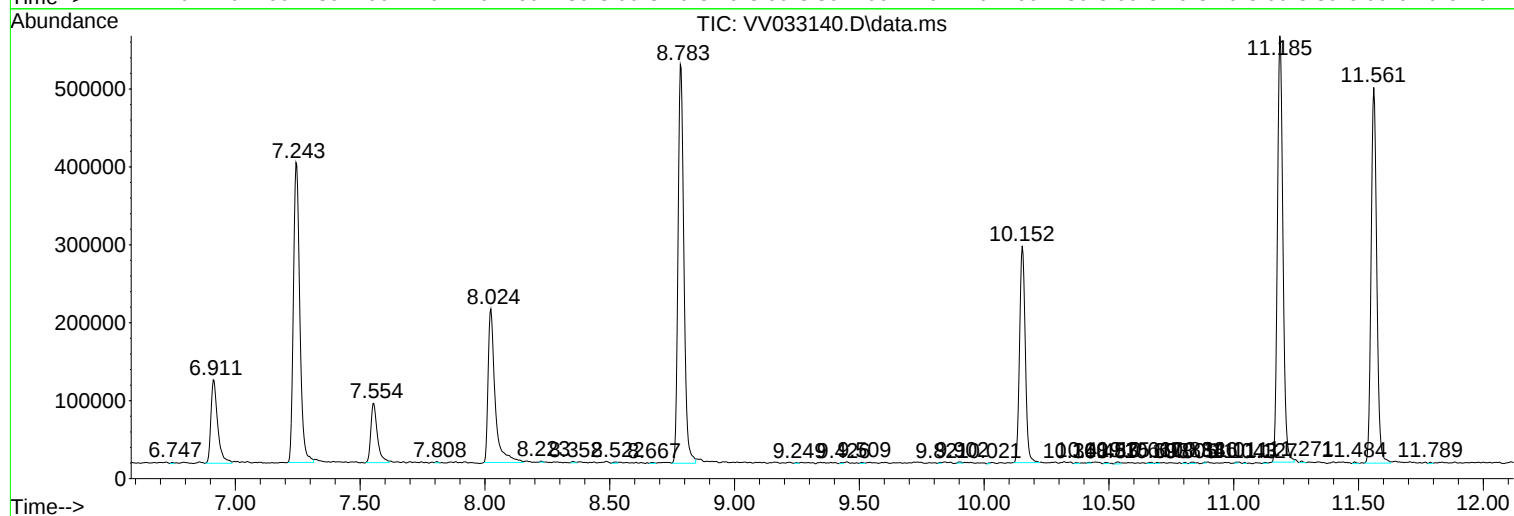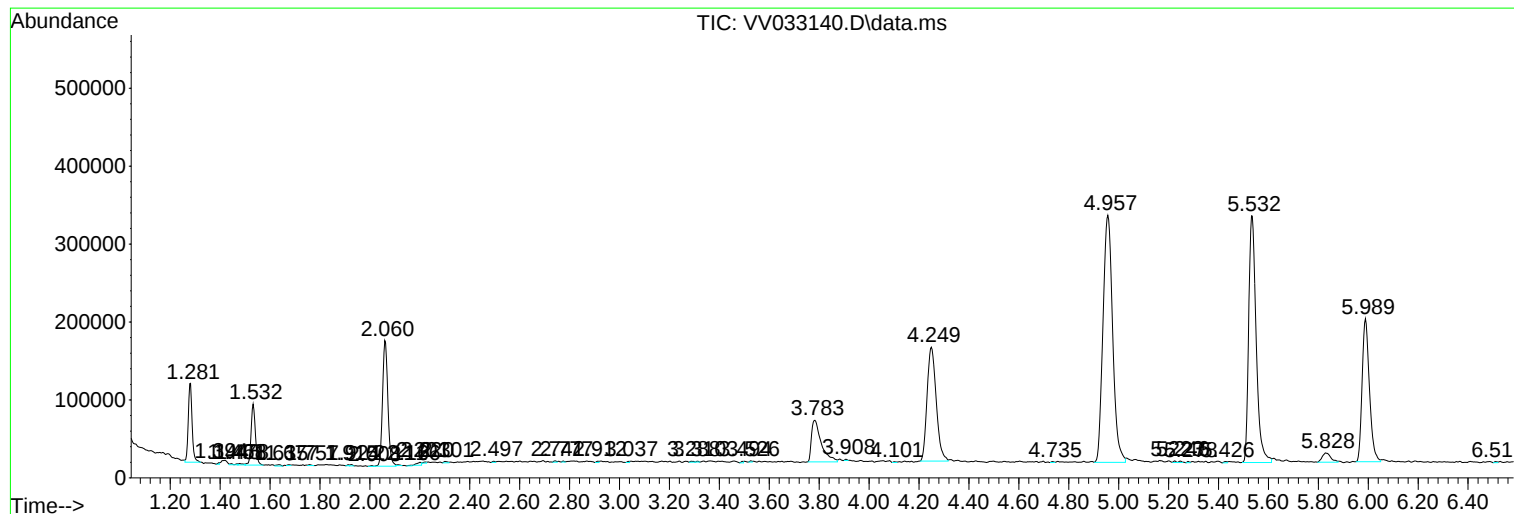

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033140.D
Acq On : 07 Dec 2023 12:43
Operator : SY/MD
Sample : 05645-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033140.D
Acq On : 07 Dec 2023 12:43
Operator : SY/MD
Sample : 05645-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------