

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033141.D
 Acq On : 07 Dec 2023 13:06
 Operator : SY/MD
 Sample : 05645-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

Signal : TIC: VV033141.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	100284	111903	13.22%	1.541%
2	1.416	108	117	124	rBV3	4483	6617	0.78%	0.091%
3	1.465	129	132	135	rVB	1144	690	0.08%	0.010%
4	1.490	138	140	142	rBV	678	298	0.04%	0.004%
5	1.532	146	153	162	rBV	74173	86963	10.27%	1.198%
6	1.616	177	179	181	rVB	691	256	0.03%	0.004%
7	1.642	181	187	190	rBV4	1030	1065	0.13%	0.015%
8	1.699	202	205	209	rBV	973	874	0.10%	0.012%
9	1.728	209	214	222	rVV	1312	1546	0.18%	0.021%
10	1.761	222	224	231	rVB4	929	717	0.08%	0.010%
11	1.806	233	238	241	rBV2	760	764	0.09%	0.011%
12	1.838	241	248	252	rVB3	1577	1968	0.23%	0.027%
13	1.860	252	255	256	rBV2	463	263	0.03%	0.004%
14	1.870	256	258	262	rVB2	730	455	0.05%	0.006%
15	1.889	262	264	266	rBV	447	238	0.03%	0.003%
16	1.905	266	269	276	rVB	1988	2376	0.28%	0.033%
17	1.937	276	279	281	rBV	737	467	0.06%	0.006%
18	1.953	281	284	285	rBV2	382	216	0.03%	0.003%
19	1.976	285	291	293	rVB2	1063	1084	0.13%	0.015%
20	1.995	293	297	303	rBV	1291	1291	0.15%	0.018%
21	2.060	303	317	330	rBV	160904	236058	27.88%	3.252%
22	2.121	334	336	337	rBV2	461	175	0.02%	0.002%
23	2.130	337	339	342	rVB	1151	568	0.07%	0.008%
24	2.150	342	345	347	rBV	1057	709	0.08%	0.010%
25	2.191	350	358	362	rBV2	2210	3255	0.38%	0.045%
26	2.224	365	368	371	rBV	2647	1823	0.22%	0.025%
27	2.461	440	442	445	rBV	1407	734	0.09%	0.010%
28	2.796	543	546	550	rBV	1737	1665	0.20%	0.023%
29	3.101	638	641	646	rBV	1717	1748	0.21%	0.024%
30	3.487	759	761	766	rBV	1208	1094	0.13%	0.015%
31	3.744	838	841	844	rBV	1620	1139	0.13%	0.016%
32	3.780	844	852	882	rVV2	52704	151326	17.87%	2.084%
33	4.011	919	924	927	rBV2	1561	1592	0.19%	0.022%
34	4.249	984	998	1021	rBV2	139318	359470	42.45%	4.952%
35	4.764	1155	1158	1161	rBV	1254	856	0.10%	0.012%
36	4.957	1202	1218	1244	rBV2	315355	846737	100.00%	11.663%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033141.D
 Acq On : 07 Dec 2023 13:06
 Operator : SY/MD
 Sample : 05645-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.262	1310	1313	1316	rBV2	2106	1580	0.19%	0.022%
38	5.313	1326	1329	1332	rBV2	1458	1072	0.13%	0.015%
39	5.346	1336	1339	1342	rBV	1265	884	0.10%	0.012%
40	5.535	1386	1398	1420	rBV	314723	646430	76.34%	8.904%
41	5.838	1479	1492	1510	rBV6	57126	125435	14.81%	1.728%
42	5.989	1526	1539	1560	rBV	183665	379679	44.84%	5.230%
43	6.384	1658	1662	1664	rBV	1494	1260	0.15%	0.017%
44	6.567	1716	1719	1722	rBV2	1545	1289	0.15%	0.018%
45	6.606	1728	1731	1735	rBV	1066	949	0.11%	0.013%
46	6.747	1773	1775	1780	rVB	1903	1227	0.14%	0.017%
47	6.850	1802	1807	1815	rVB	1385	1977	0.23%	0.027%
48	6.915	1815	1827	1846	rBV	101987	195475	23.09%	2.693%
49	7.098	1881	1884	1889	rVB	2057	1600	0.19%	0.022%
50	7.243	1919	1929	1949	rBV	380397	674097	79.61%	9.285%
51	7.551	2016	2025	2044	rBV	75607	136405	16.11%	1.879%
52	7.661	2056	2059	2063	rBV2	1429	1151	0.14%	0.016%
53	8.024	2163	2172	2212	rBV	191807	374599	44.24%	5.160%
54	8.255	2242	2244	2246	rBV	1185	677	0.08%	0.009%
55	8.323	2263	2265	2266	rBV	1012	412	0.05%	0.006%
56	8.786	2398	2409	2427	rBV	510563	831984	98.26%	11.460%
57	9.069	2494	2497	2499	rBV3	1209	943	0.11%	0.013%
58	9.561	2647	2650	2655	rVB	2222	1689	0.20%	0.023%
59	9.590	2656	2659	2661	rBV	1729	1295	0.15%	0.018%
60	9.734	2702	2704	2707	rBV	1061	555	0.07%	0.008%
61	10.152	2822	2834	2854	rBV	275969	434250	51.29%	5.982%
62	10.702	3002	3005	3007	rBV	1029	742	0.09%	0.010%
63	10.750	3017	3020	3021	rBV	1131	714	0.08%	0.010%
64	11.085	3121	3124	3130	rBV3	1212	1175	0.14%	0.016%
65	11.185	3144	3155	3174	rBV	544984	840575	99.27%	11.579%
66	11.307	3190	3193	3201	rVB	1827	2014	0.24%	0.028%
67	11.561	3261	3272	3294	rVB	474809	741133	87.53%	10.209%
68	11.731	3321	3325	3328	rBV	1933	1664	0.20%	0.023%
69	11.931	3381	3387	3389	rBV	2762	3014	0.36%	0.042%
70	12.172	3459	3462	3464	rBV2	1542	1076	0.13%	0.015%
71	12.349	3514	3517	3520	rVB	1484	865	0.10%	0.012%
72	12.480	3555	3558	3562	rVB	1499	1108	0.13%	0.015%
73	12.911	3690	3692	3694	rBV	1298	850	0.10%	0.012%
74	12.992	3714	3717	3719	rBV2	1749	1245	0.15%	0.017%
75	13.053	3733	3736	3739	rBV	1397	768	0.09%	0.011%
76	13.442	3854	3857	3862	rBV	1226	1147	0.14%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033141.D
 Acq On : 07 Dec 2023 13:06
 Operator : SY/MD
 Sample : 05645-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	13.477	3865	3868	3873	rBV	1151	963	0.11%	0.013%
78	13.516	3878	3880	3883	rBV	1099	656	0.08%	0.009%
79	13.696	3934	3936	3939	rVB	1174	620	0.07%	0.009%
80	14.065	4049	4051	4053	rBV2	1227	706	0.08%	0.010%
81	14.098	4058	4061	4064	rBV2	1576	1149	0.14%	0.016%
82	14.194	4089	4091	4094	rBV2	1134	732	0.09%	0.010%
83	14.371	4144	4146	4148	rBV3	1054	645	0.08%	0.009%
84	14.496	4183	4185	4187	rBV	1127	602	0.07%	0.008%
85	14.792	4274	4277	4281	rBV	1663	1390	0.16%	0.019%
86	15.332	4440	4445	4449	rBV	1797	1853	0.22%	0.026%
87	15.368	4454	4456	4460	rBV2	1732	1174	0.14%	0.016%
88	15.426	4471	4474	4476	rBV3	1946	1349	0.16%	0.019%
89	15.593	4523	4526	4531	rVB	2408	1973	0.23%	0.027%
90	15.622	4533	4535	4538	rBV	1252	741	0.09%	0.010%
91	15.827	4596	4599	4603	rVB2	1915	1226	0.14%	0.017%




Sum of corrected areas: 7259783

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033141.D
Acq On : 07 Dec 2023 13:06
Operator : SY/MD
Sample : 05645-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

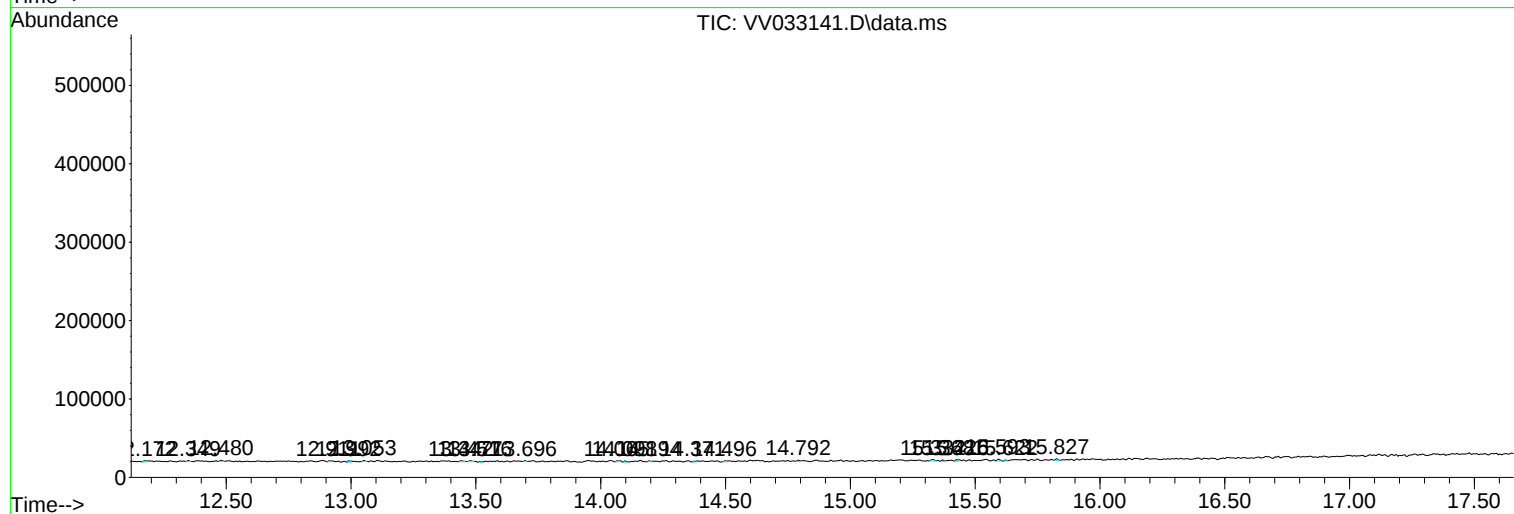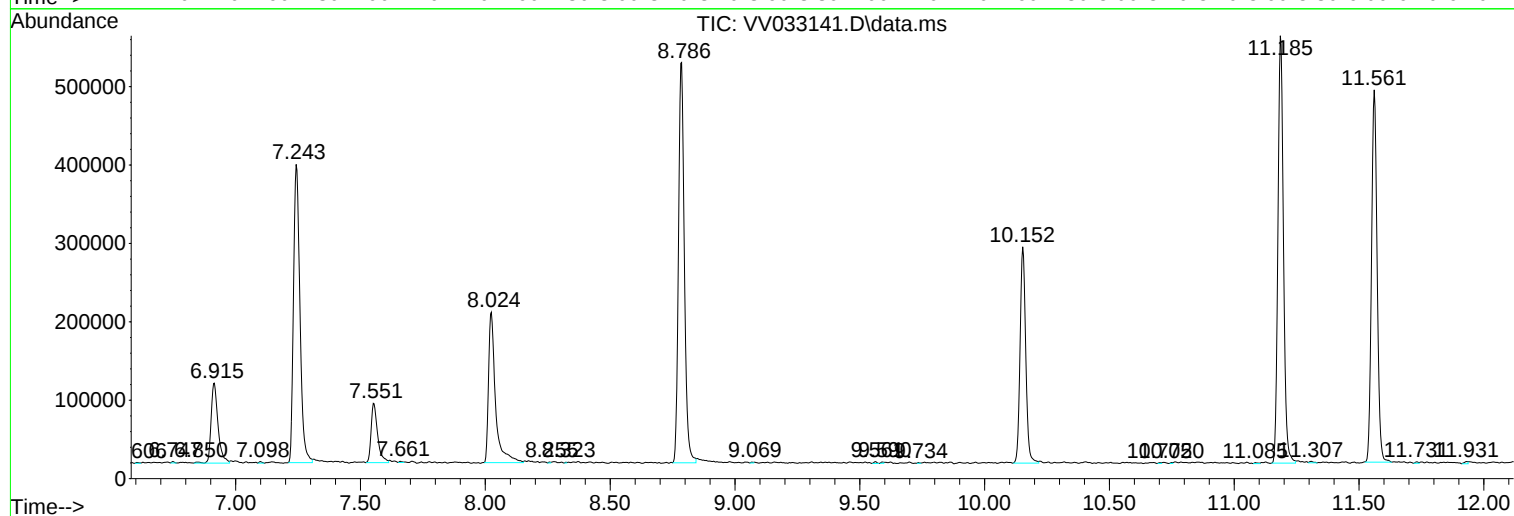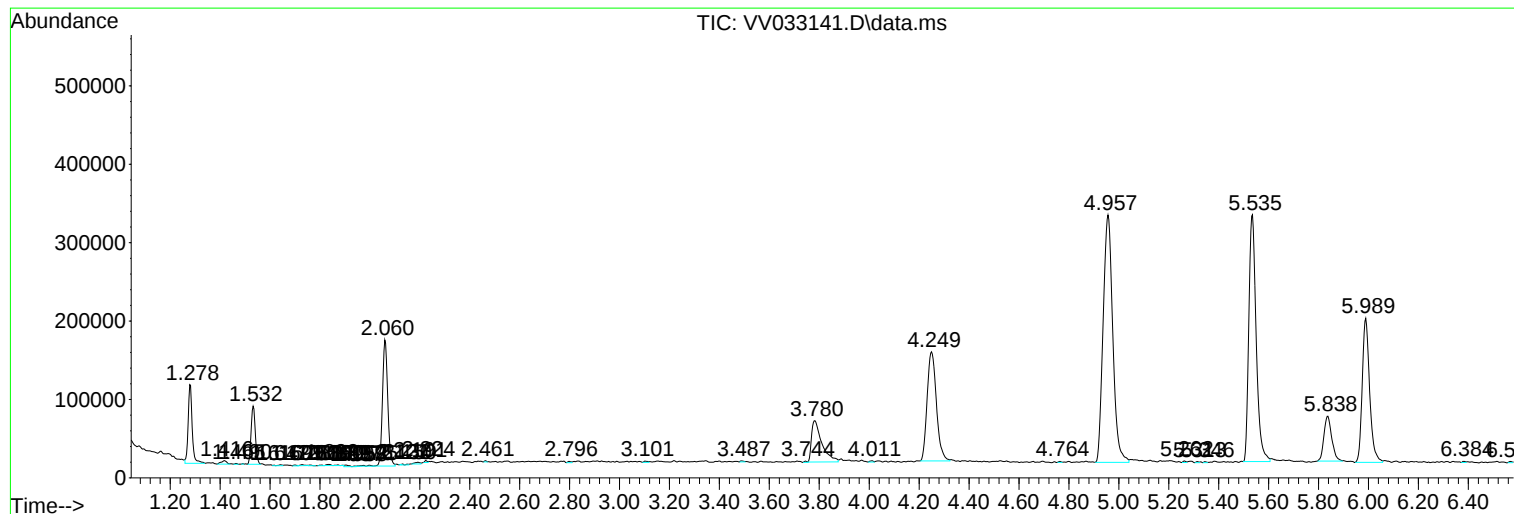

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033141.D
Acq On : 07 Dec 2023 13:06
Operator : SY/MD
Sample : 05645-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033141.D
Acq On : 07 Dec 2023 13:06
Operator : SY/MD
Sample : 05645-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc