

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033142.D
 Acq On : 07 Dec 2023 13:29
 Operator : SY/MD
 Sample : 05644-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033142.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	92234	96898	11.83%	1.383%
2	1.417	114	117	118	rBV	754	438	0.05%	0.006%
3	1.426	118	120	122	rBV2	920	619	0.08%	0.009%
4	1.532	142	153	164	rBV	74912	89208	10.89%	1.273%
5	1.574	164	166	172	rVB3	1657	1238	0.15%	0.018%
6	1.603	172	175	176	rBV	911	480	0.06%	0.007%
7	1.616	176	179	182	rVB	945	638	0.08%	0.009%
8	1.645	186	188	192	rVB2	1132	748	0.09%	0.011%
9	1.674	192	197	203	rBV4	1290	1408	0.17%	0.020%
10	1.712	207	209	212	rBV2	524	300	0.04%	0.004%
11	1.728	212	214	216	rBV2	698	297	0.04%	0.004%
12	1.748	216	220	223	rVB	1226	996	0.12%	0.014%
13	1.764	223	225	227	rBV	631	330	0.04%	0.005%
14	1.783	229	231	234	rVB3	615	307	0.04%	0.004%
15	1.802	234	237	239	rBV2	1162	579	0.07%	0.008%
16	1.815	239	241	246	rVB2	1368	1183	0.14%	0.017%
17	1.841	246	249	251	rBV3	918	550	0.07%	0.008%
18	1.857	251	254	256	rBV2	1140	614	0.07%	0.009%
19	1.873	256	259	261	rBV2	549	326	0.04%	0.005%
20	1.886	261	263	266	rVB3	1036	515	0.06%	0.007%
21	1.915	266	272	277	rVB2	2033	2693	0.33%	0.038%
22	1.944	277	281	288	rBV2	654	634	0.08%	0.009%
23	1.979	288	292	298	rBV2	790	739	0.09%	0.011%
24	2.008	298	301	304	rVB	1403	886	0.11%	0.013%
25	2.060	304	317	329	rBV	154321	226168	27.61%	3.228%
26	2.111	331	333	337	rVB2	1216	698	0.09%	0.010%
27	2.159	342	348	351	rBV	2879	3003	0.37%	0.043%
28	2.182	351	355	356	rBV	1544	1224	0.15%	0.017%
29	2.240	360	373	375	rBV4	5040	9248	1.13%	0.132%
30	2.333	399	402	405	rBV3	1272	911	0.11%	0.013%
31	2.429	429	432	434	rBV	1531	1149	0.14%	0.016%
32	2.561	469	473	482	rVB2	4456	5915	0.72%	0.084%
33	2.619	488	491	494	rVB	1678	1071	0.13%	0.015%
34	2.876	568	571	572	rBV	1178	766	0.09%	0.011%
35	3.114	642	645	648	rVB2	1256	768	0.09%	0.011%
36	3.211	672	675	677	rBV	1391	910	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033142.D
 Acq On : 07 Dec 2023 13:29
 Operator : SY/MD
 Sample : 05644-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	3.404	733	735	738	rVB	1126	560	0.07%	0.008%
38	3.494	759	763	767	rBV	1624	1864	0.23%	0.027%
39	3.786	842	854	883	rBV3	75582	236820	28.91%	3.380%
40	4.108	952	954	958	rVB	1754	1271	0.16%	0.018%
41	4.249	982	998	1024	rBV2	136719	351688	42.93%	5.019%
42	4.378	1036	1038	1039	rBV	1449	650	0.08%	0.009%
43	4.616	1109	1112	1115	rBV	974	662	0.08%	0.009%
44	4.812	1171	1173	1176	rBV2	893	468	0.06%	0.007%
45	4.847	1181	1184	1187	rVB	1126	715	0.09%	0.010%
46	4.867	1188	1190	1193	rBV	1098	661	0.08%	0.009%
47	4.957	1202	1218	1245	rBV3	298947	802711	97.99%	11.456%
48	5.532	1386	1397	1426	rBV	313815	646162	78.88%	9.222%
49	5.757	1461	1467	1470	rBV	2399	2905	0.35%	0.041%
50	5.828	1479	1489	1509	rBV3	16406	33878	4.14%	0.483%
51	5.989	1527	1539	1561	rBV	174363	354652	43.29%	5.061%
52	6.516	1701	1703	1705	rBV	1001	408	0.05%	0.006%
53	6.770	1779	1782	1784	rBV2	1181	649	0.08%	0.009%
54	6.783	1784	1786	1788	rVV	951	468	0.06%	0.007%
55	6.854	1806	1808	1812	rBV	1113	787	0.10%	0.011%
56	6.915	1817	1827	1844	rBV	96235	179148	21.87%	2.557%
57	7.201	1914	1916	1918	rBV	979	559	0.07%	0.008%
58	7.243	1918	1929	1951	rBV	361188	647102	79.00%	9.235%
59	7.555	2017	2026	2047	rBV3	69220	127993	15.62%	1.827%
60	7.825	2107	2110	2111	rBV2	1082	660	0.08%	0.009%
61	7.953	2147	2150	2155	rBV2	1322	1257	0.15%	0.018%
62	7.976	2155	2157	2161	rVB	1290	833	0.10%	0.012%
63	8.024	2163	2172	2204	rBV	191624	377032	46.03%	5.381%
64	8.783	2398	2408	2429	rBV	494496	811371	99.05%	11.579%
65	9.860	2741	2743	2746	rBV	1188	735	0.09%	0.010%
66	9.905	2754	2757	2761	rBV2	1128	752	0.09%	0.011%
67	9.950	2768	2771	2773	rBV	1688	790	0.10%	0.011%
68	9.963	2773	2775	2777	rBV	893	426	0.05%	0.006%
69	10.153	2822	2834	2853	rBV	257249	400019	48.83%	5.709%
70	10.651	2984	2989	2991	rBV	1312	1236	0.15%	0.018%
71	10.854	3050	3052	3059	rVB	1774	2031	0.25%	0.029%
72	11.079	3118	3122	3123	rBV	2046	1526	0.19%	0.022%
73	11.185	3145	3155	3174	rBV	532370	819165	100.00%	11.691%
74	11.561	3261	3272	3290	rBV	451588	707084	86.32%	10.091%
75	12.162	3456	3459	3460	rBV	1131	668	0.08%	0.010%
76	12.461	3549	3552	3555	rBV	1471	1119	0.14%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033142.D
 Acq On : 07 Dec 2023 13:29
 Operator : SY/MD
 Sample : 05644-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.532	3572	3574	3578	rBV	1169	787	0.10%	0.011%
78	12.712	3627	3630	3633	rBV	1626	1384	0.17%	0.020%
79	12.870	3674	3679	3682	rBV	1976	1763	0.22%	0.025%
80	12.934	3696	3699	3703	rBV	968	782	0.10%	0.011%
81	13.043	3730	3733	3736	rBV	1959	1539	0.19%	0.022%
82	13.091	3745	3748	3752	rVB	1421	863	0.11%	0.012%
83	13.188	3773	3778	3781	rBV	2079	2202	0.27%	0.031%
84	13.336	3821	3824	3827	rBV	1217	1092	0.13%	0.016%
85	13.506	3873	3877	3880	rBV2	1738	1519	0.19%	0.022%
86	13.763	3954	3957	3959	rBV	1679	1088	0.13%	0.016%
87	13.796	3965	3967	3970	rVB	1195	597	0.07%	0.009%
88	14.078	4053	4055	4056	rBV	1307	668	0.08%	0.010%
89	14.226	4097	4101	4105	rBV	2350	2022	0.25%	0.029%
90	14.252	4105	4109	4111	rVV	1278	993	0.12%	0.014%
91	14.680	4240	4242	4247	rVB	1648	1076	0.13%	0.015%
92	14.953	4323	4327	4330	rBV	1782	1726	0.21%	0.025%
93	15.017	4345	4347	4350	rBV	936	525	0.06%	0.007%
94	15.123	4377	4380	4384	rBV	1526	1506	0.18%	0.021%
95	15.275	4422	4427	4429	rBV2	2344	2322	0.28%	0.033%
96	15.693	4554	4557	4560	rBV3	1918	1518	0.19%	0.022%
97	16.156	4698	4701	4705	rBV	2235	2149	0.26%	0.031%
98	16.191	4709	4712	4715	rBV	2476	1461	0.18%	0.021%
99	16.249	4727	4730	4732	rBV4	1654	1123	0.14%	0.016%
100	16.770	4889	4892	4896	rBV	3246	2323	0.28%	0.033%




Sum of corrected areas: 7006968

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033142.D
Acq On : 07 Dec 2023 13:29
Operator : SY/MD
Sample : 05644-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

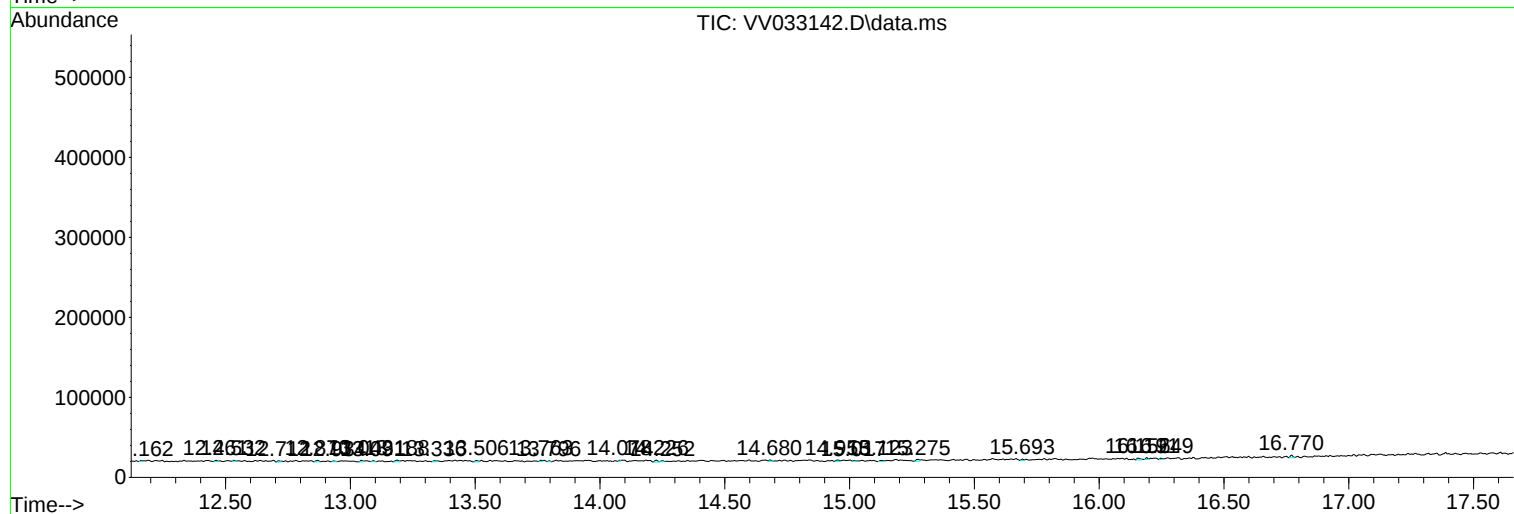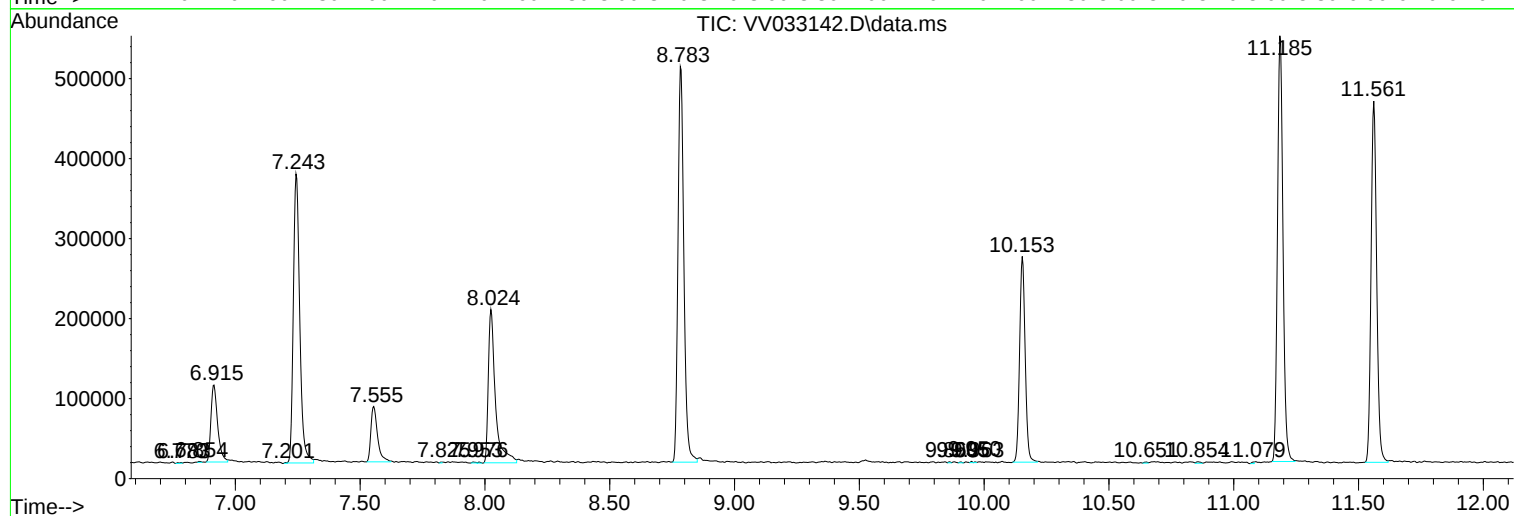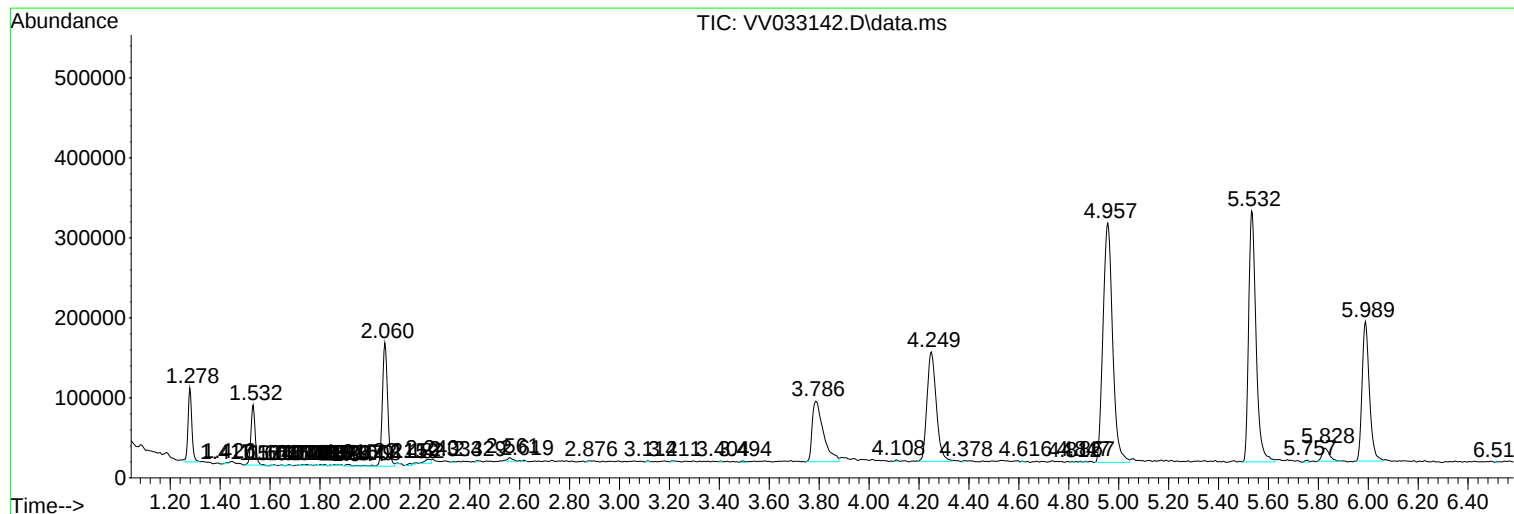

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033142.D
Acq On : 07 Dec 2023 13:29
Operator : SY/MD
Sample : 05644-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033142.D
Acq On : 07 Dec 2023 13:29
Operator : SY/MD
Sample : 05644-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc