

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033143.D
 Acq On : 07 Dec 2023 13:53
 Operator : SY/MD
 Sample : 05644-02DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G18DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	94811	101216	12.53%	1.368%
2	1.368	100	102	105	rVB	1188	649	0.08%	0.009%
3	1.426	114	120	130	rVB3	5043	8413	1.04%	0.114%
4	1.465	130	132	133	rBV	696	353	0.04%	0.005%
5	1.532	144	153	164	rVV	75021	86746	10.74%	1.172%
6	1.577	164	167	173	rVB3	1382	1259	0.16%	0.017%
7	1.639	180	186	189	rBV2	1635	2139	0.26%	0.029%
8	1.655	189	191	199	rVV2	1241	1640	0.20%	0.022%
9	1.687	199	201	205	rVB2	917	706	0.09%	0.010%
10	1.709	205	208	209	rBV2	664	353	0.04%	0.005%
11	1.738	214	217	218	rVV2	1029	677	0.08%	0.009%
12	1.767	222	226	230	rVB2	777	732	0.09%	0.010%
13	1.793	230	234	237	rVB	1532	1162	0.14%	0.016%
14	1.812	237	240	245	rBV	1896	1289	0.16%	0.017%
15	1.838	245	248	252	rBV3	1096	1006	0.12%	0.014%
16	1.867	252	257	259	rBV2	758	814	0.10%	0.011%
17	1.905	266	269	271	rBV2	482	301	0.04%	0.004%
18	1.918	271	273	274	rBV2	172	40	0.00%	0.001%
19	1.950	278	283	289	rBV2	951	1342	0.17%	0.018%
20	1.976	289	291	295	rVB3	1203	660	0.08%	0.009%
21	1.992	295	296	298	rBV	199	87	0.01%	0.001%
22	2.011	298	302	304	rBV3	1205	802	0.10%	0.011%
23	2.060	307	317	330	rBV2	159851	239242	29.63%	3.233%
24	2.108	330	332	344	rVB5	2304	2875	0.36%	0.039%
25	2.195	344	359	361	rBV	3953	9381	1.16%	0.127%
26	2.237	365	372	374	rBV2	2897	3269	0.40%	0.044%
27	2.423	428	430	433	rBV	1549	780	0.10%	0.011%
28	2.616	488	490	495	rBV2	1157	921	0.11%	0.012%
29	2.938	587	590	595	rBV	1646	1987	0.25%	0.027%
30	3.028	615	618	620	rBV2	1695	1310	0.16%	0.018%
31	3.066	628	630	633	rBV	980	772	0.10%	0.010%
32	3.786	844	854	884	rBV2	56372	190616	23.61%	2.576%
33	4.060	937	939	942	rVB	1495	720	0.09%	0.010%
34	4.249	984	998	1020	rBV2	136257	343225	42.50%	4.638%
35	4.471	1064	1067	1069	rBV2	1401	1016	0.13%	0.014%
36	4.513	1072	1080	1082	rBV4	6163	8135	1.01%	0.110%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033143.D
 Acq On : 07 Dec 2023 13:53
 Operator : SY/MD
 Sample : 05644-02DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G18DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.957	1202	1218	1241	rBV2	303229	807505	100.00%	10.911%
38	5.150	1275	1278	1281	rVB3	1616	1030	0.13%	0.014%
39	5.362	1342	1344	1347	rBV	1046	571	0.07%	0.008%
40	5.455	1370	1373	1375	rBV2	1078	762	0.09%	0.010%
41	5.532	1386	1397	1426	rBV	302146	630891	78.13%	8.524%
42	5.834	1477	1491	1512	rBV2	242502	502881	62.28%	6.795%
43	5.989	1527	1539	1565	rBV	174992	360022	44.58%	4.864%
44	6.613	1730	1733	1734	rBV2	1084	694	0.09%	0.009%
45	6.687	1753	1756	1758	rBV	1161	816	0.10%	0.011%
46	6.706	1759	1762	1765	rVV2	1567	1079	0.13%	0.015%
47	6.777	1782	1784	1787	rBV2	1180	834	0.10%	0.011%
48	6.834	1799	1802	1805	rVB2	1270	765	0.09%	0.010%
49	6.915	1817	1827	1844	rBV	98243	184568	22.86%	2.494%
50	7.066	1872	1874	1877	rBV	1691	942	0.12%	0.013%
51	7.243	1918	1929	1959	rBV	360900	660303	81.77%	8.922%
52	7.555	2016	2026	2044	rBV	72751	131514	16.29%	1.777%
53	7.703	2070	2072	2076	rBV	1385	827	0.10%	0.011%
54	7.902	2128	2134	2136	rBV2	1859	2171	0.27%	0.029%
55	8.024	2163	2172	2190	rBV	187711	344841	42.70%	4.659%
56	8.429	2293	2298	2300	rBV	2125	2002	0.25%	0.027%
57	8.786	2395	2409	2431	rBV	482619	796804	98.67%	10.766%
58	8.931	2451	2454	2458	rVB	2710	1940	0.24%	0.026%
59	9.040	2485	2488	2490	rBV2	1199	862	0.11%	0.012%
60	9.545	2642	2645	2647	rBV2	1274	681	0.08%	0.009%
61	10.153	2823	2834	2854	rVB	260880	411261	50.93%	5.557%
62	10.262	2866	2868	2874	rVB	1667	1330	0.16%	0.018%
63	10.487	2935	2938	2944	rBV	1096	1085	0.13%	0.015%
64	10.686	2997	3000	3001	rBV	1047	630	0.08%	0.009%
65	10.802	3031	3036	3040	rBV	2170	2830	0.35%	0.038%
66	10.979	3088	3091	3092	rBV	1367	716	0.09%	0.010%
67	11.050	3110	3113	3118	rBV	1455	1275	0.16%	0.017%
68	11.185	3144	3155	3175	rBV	511838	796457	98.63%	10.761%
69	11.278	3181	3184	3188	rVB	2411	1586	0.20%	0.021%
70	11.561	3261	3272	3290	rBV	456246	708071	87.69%	9.567%
71	11.857	3361	3364	3366	rBV	1228	886	0.11%	0.012%
72	12.374	3523	3525	3528	rBV	1068	608	0.08%	0.008%
73	12.927	3692	3697	3700	rBV2	1725	1933	0.24%	0.026%
74	13.001	3718	3720	3723	rVB	1245	589	0.07%	0.008%
75	13.178	3772	3775	3778	rBV	1790	1167	0.14%	0.016%
76	13.526	3877	3883	3888	rBV	2558	3369	0.42%	0.046%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033143.D
Acq On : 07 Dec 2023 13:53
Operator : SY/MD
Sample : 05644-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G18DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

77	13.763	3954	3957	3959	rBV	1645	1020	0.13%	0.014%
78	13.985	4023	4026	4032	rBV	1474	1413	0.17%	0.019%
79	14.339	4133	4136	4140	rVB	2018	1446	0.18%	0.020%
80	14.480	4177	4180	4183	rBV2	1998	1177	0.15%	0.016%
81	14.606	4215	4219	4221	rBV2	1915	1667	0.21%	0.023%
82	14.667	4235	4238	4243	rBV	1731	1554	0.19%	0.021%
83	14.741	4259	4261	4266	rBV	1758	1321	0.16%	0.018%
84	15.246	4416	4418	4423	rVB2	1741	1172	0.15%	0.016%
85	15.509	4496	4500	4505	rBV2	2451	2901	0.36%	0.039%
86	16.287	4739	4742	4746	rBV2	2130	1645	0.20%	0.022%


Sum of corrected areas: 7401049

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033143.D
Acq On : 07 Dec 2023 13:53
Operator : SY/MD
Sample : 05644-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G18DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

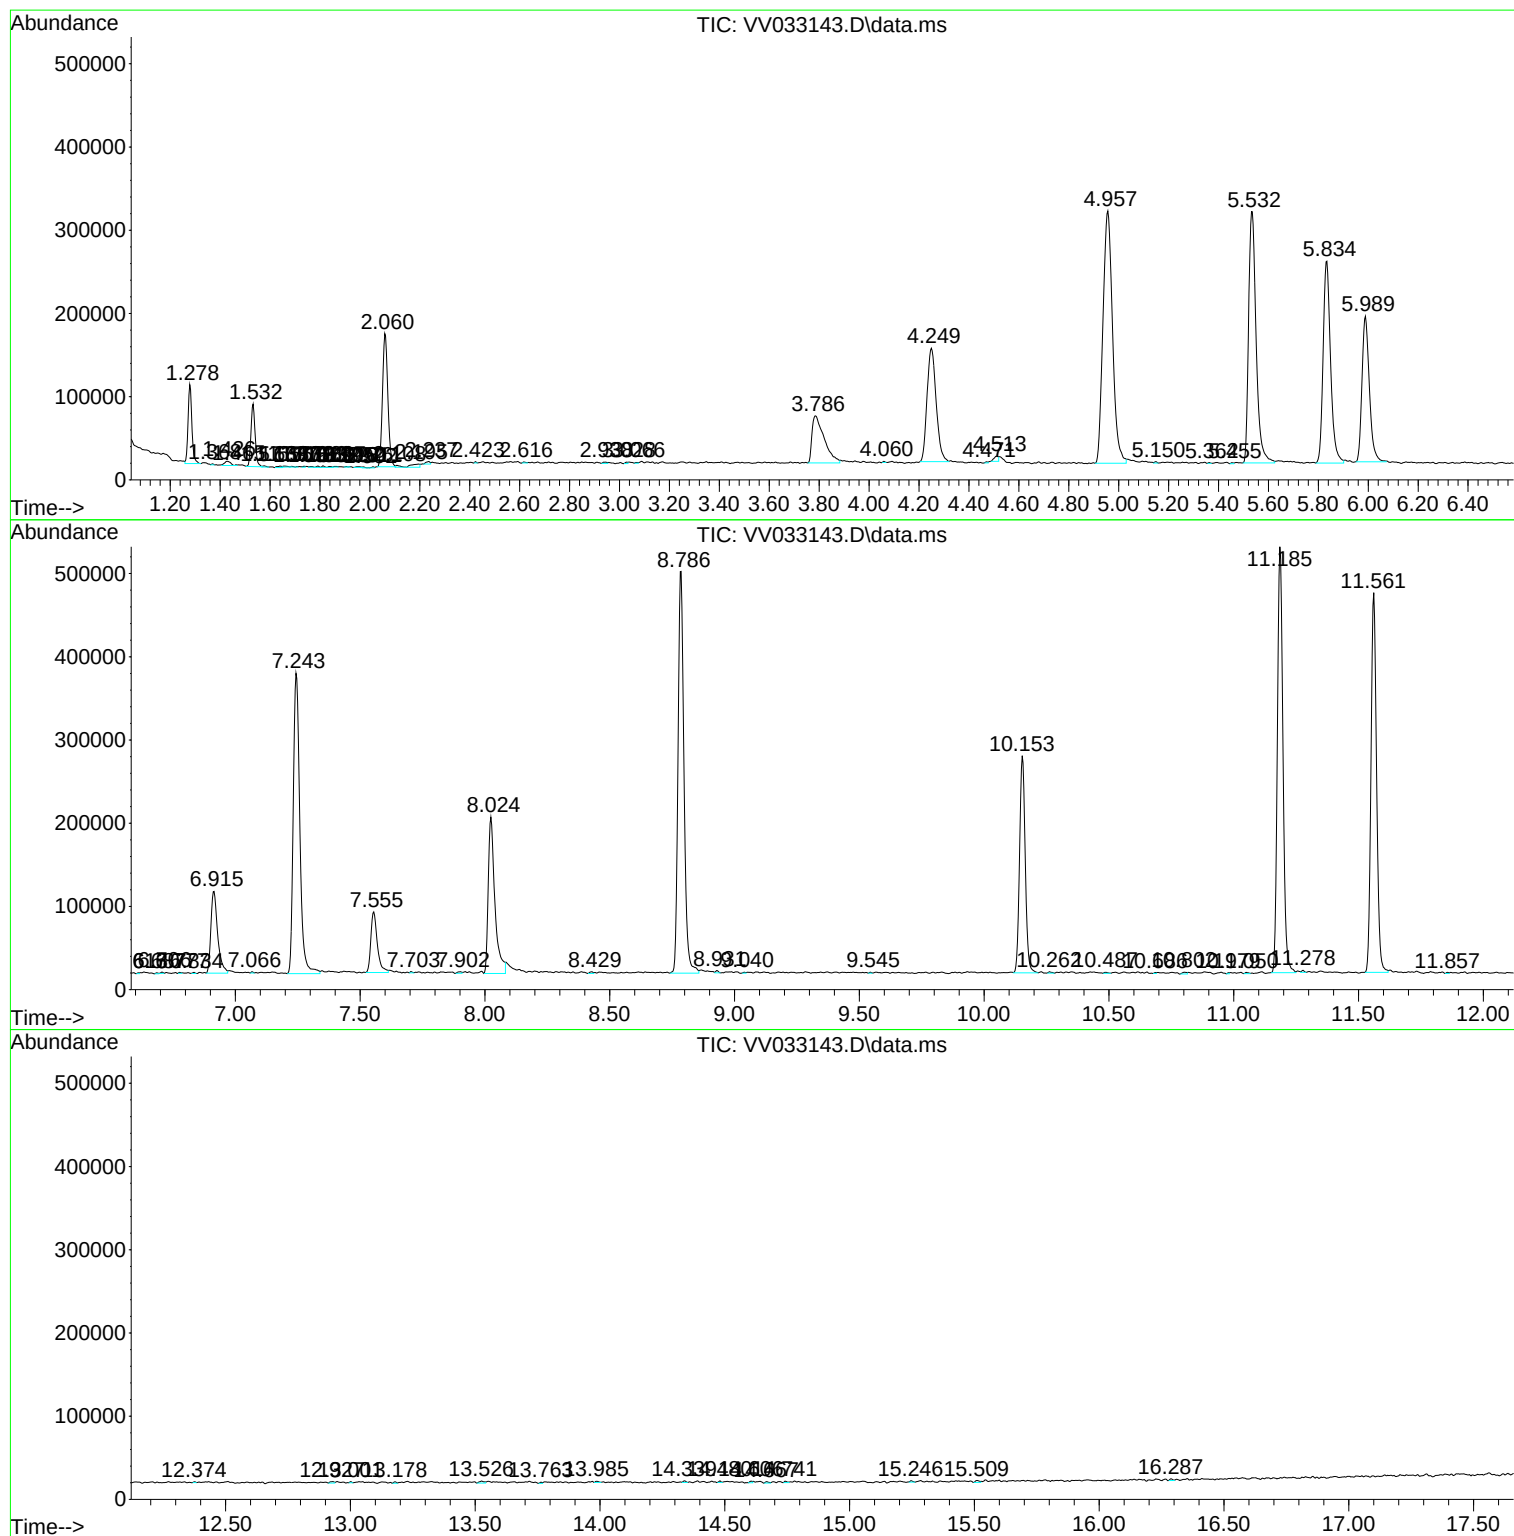

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033143.D
Acq On : 07 Dec 2023 13:53
Operator : SY/MD
Sample : 05644-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G18DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033143.D
Acq On : 07 Dec 2023 13:53
Operator : SY/MD
Sample : 05644-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G18DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------