

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033144.D
 Acq On : 07 Dec 2023 14:16
 Operator : SY/MD
 Sample : 05673-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033144.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	102278	104858	12.26%	1.448%
2	1.420	108	118	123	rBV2	4794	7000	0.82%	0.097%
3	1.487	136	139	142	rVV	1109	832	0.10%	0.011%
4	1.532	144	153	168	rVB	77165	96114	11.24%	1.327%
5	1.590	168	171	174	rBV	1451	947	0.11%	0.013%
6	1.629	180	183	185	rVV	1375	961	0.11%	0.013%
7	1.973	286	290	293	rBV	1180	953	0.11%	0.013%
8	1.992	293	296	301	rVB3	904	934	0.11%	0.013%
9	2.060	304	317	330	rBV	156958	231751	27.10%	3.200%
10	2.108	330	332	341	rVB5	3807	3961	0.46%	0.055%
11	2.153	341	346	349	rBV	2302	2098	0.25%	0.029%
12	2.175	349	353	355	rBV	2332	1907	0.22%	0.026%
13	2.217	361	366	373	rBV4	3337	4873	0.57%	0.067%
14	2.378	413	416	417	rBV	1546	941	0.11%	0.013%
15	3.346	713	717	720	rBV	1812	1486	0.17%	0.021%
16	3.378	724	727	734	rVV	1385	1652	0.19%	0.023%
17	3.606	795	798	801	rBV3	1378	860	0.10%	0.012%
18	3.654	808	813	818	rVB	1536	1743	0.20%	0.024%
19	3.780	844	852	876	rBV	54092	142072	16.61%	1.962%
20	3.992	912	918	920	rBV3	1646	1871	0.22%	0.026%
21	4.092	946	949	953	rBV2	1333	1373	0.16%	0.019%
22	4.249	983	998	1019	rBV	143230	364324	42.60%	5.031%
23	4.494	1071	1074	1077	rBV	1195	1037	0.12%	0.014%
24	4.957	1199	1218	1242	rBV2	314705	845455	98.86%	11.674%
25	5.207	1294	1296	1303	rVB	1349	1095	0.13%	0.015%
26	5.371	1345	1347	1351	rVB	2774	1918	0.22%	0.026%
27	5.404	1353	1357	1360	rBV2	1922	1609	0.19%	0.022%
28	5.532	1386	1397	1425	rVV	317434	656856	76.81%	9.070%
29	5.780	1472	1474	1477	rVB2	1508	837	0.10%	0.012%
30	5.828	1479	1489	1501	rBV4	17395	37719	4.41%	0.521%
31	5.989	1526	1539	1562	rBV	178189	369501	43.21%	5.102%
32	6.224	1608	1612	1615	rBV	1399	1544	0.18%	0.021%
33	6.619	1732	1735	1738	rBV	1458	1004	0.12%	0.014%
34	6.728	1766	1769	1772	rVB	1670	974	0.11%	0.013%
35	6.873	1811	1814	1817	rBV	1951	1513	0.18%	0.021%
36	6.912	1817	1826	1843	rBV	103298	190935	22.33%	2.636%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033144.D
 Acq On : 07 Dec 2023 14:16
 Operator : SY/MD
 Sample : 05673-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	7.063	1871	1873	1877	rBV	1625	1168	0.14%	0.016%
38	7.243	1918	1929	1952	rBV	380366	674147	78.83%	9.309%
39	7.551	2017	2025	2045	rBV	77157	138651	16.21%	1.914%
40	7.709	2071	2074	2077	rBV	1374	987	0.12%	0.014%
41	7.966	2149	2154	2156	rBV2	1283	1134	0.13%	0.016%
42	7.979	2156	2158	2163	rVB2	1711	1130	0.13%	0.016%
43	8.024	2163	2172	2205	rBV	185384	370011	43.27%	5.109%
44	8.259	2237	2245	2255	rVB2	1959	3864	0.45%	0.053%
45	8.510	2319	2323	2327	rBV	2034	1712	0.20%	0.024%
46	8.535	2328	2331	2335	rVV	1485	1245	0.15%	0.017%
47	8.590	2346	2348	2354	rVB	1787	1431	0.17%	0.020%
48	8.783	2397	2408	2430	rBV	512106	835601	97.71%	11.538%
49	8.957	2459	2462	2471	rVB3	3444	4301	0.50%	0.059%
50	9.011	2476	2479	2484	rVB2	1732	1629	0.19%	0.022%
51	9.040	2485	2488	2492	rBV	1712	1184	0.14%	0.016%
52	9.075	2492	2499	2501	rBV3	9374	9571	1.12%	0.132%
53	9.342	2579	2582	2584	rBV	1345	994	0.12%	0.014%
54	9.487	2621	2627	2640	rVB6	6251	10149	1.19%	0.140%
55	9.911	2756	2759	2761	rBV2	1225	994	0.12%	0.014%
56	10.018	2788	2792	2795	rBV	1327	1276	0.15%	0.018%
57	10.153	2823	2834	2855	rBV	273379	425663	49.77%	5.878%
58	10.329	2882	2889	2893	rBV4	4813	6488	0.76%	0.090%
59	10.667	2991	2994	2998	rBV	1812	1686	0.20%	0.023%
60	10.857	3049	3053	3057	rBV2	1971	1799	0.21%	0.025%
61	11.040	3107	3110	3114	rBV	1246	1093	0.13%	0.015%
62	11.088	3123	3125	3129	rVB	1220	870	0.10%	0.012%
63	11.185	3143	3155	3176	rBV	561559	855206	100.00%	11.809%
64	11.371	3210	3213	3219	rBV	2157	1955	0.23%	0.027%
65	11.500	3247	3253	3255	rBV4	4950	5245	0.61%	0.072%
66	11.561	3261	3272	3291	rVB	479405	748559	87.53%	10.336%
67	11.735	3322	3326	3335	rBV2	1863	2754	0.32%	0.038%
68	11.953	3391	3394	3397	rBV	1731	1070	0.13%	0.015%
69	12.114	3441	3444	3451	rBV	1706	2377	0.28%	0.033%
70	12.159	3455	3458	3462	rBV3	1351	1407	0.16%	0.019%
71	12.384	3526	3528	3534	rVB	1795	1337	0.16%	0.018%
72	12.477	3553	3557	3560	rBV	1636	1239	0.14%	0.017%
73	12.780	3649	3651	3655	rBV	1218	968	0.11%	0.013%
74	13.046	3731	3734	3739	rVB	1682	1086	0.13%	0.015%
75	13.114	3752	3755	3760	rVB	1580	1310	0.15%	0.018%
76	13.156	3765	3768	3773	rVB	1360	1332	0.16%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033144.D
 Acq On : 07 Dec 2023 14:16
 Operator : SY/MD
 Sample : 05673-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	13.233	3789	3792	3797	rVB	1861	1170	0.14%	0.016%
78	13.262	3798	3801	3803	rBV	1250	840	0.10%	0.012%
79	13.400	3841	3844	3847	rBV2	1464	1264	0.15%	0.017%
80	13.606	3906	3908	3911	rBV	1297	807	0.09%	0.011%
81	13.635	3914	3917	3922	rVB	1500	1539	0.18%	0.021%
82	13.886	3991	3995	3998	rBV	1596	1596	0.19%	0.022%
83	13.972	4016	4022	4025	rBV2	1782	2265	0.26%	0.031%
84	14.181	4083	4087	4091	rBV	1678	1601	0.19%	0.022%
85	14.304	4121	4125	4129	rBV4	1771	1718	0.20%	0.024%
86	14.365	4142	4144	4147	rBV3	1435	1041	0.12%	0.014%
87	14.542	4195	4199	4201	rBV	1992	1376	0.16%	0.019%
88	14.847	4289	4294	4298	rBV2	1979	2387	0.28%	0.033%
89	14.905	4309	4312	4314	rBV2	1528	1025	0.12%	0.014%
90	14.976	4330	4334	4336	rBV5	1354	1252	0.15%	0.017%
91	15.001	4340	4342	4345	rVB	1665	860	0.10%	0.012%
92	15.082	4363	4367	4370	rBV3	1470	1180	0.14%	0.016%
93	15.339	4445	4447	4453	rVB4	1412	1304	0.15%	0.018%
94	15.368	4453	4456	4462	rBV	1805	1929	0.23%	0.027%
95	15.451	4480	4482	4485	rBV3	1322	820	0.10%	0.011%
96	15.535	4505	4508	4510	rBV2	1756	1068	0.12%	0.015%
97	15.693	4554	4557	4558	rBV	1477	880	0.10%	0.012%
98	15.953	4635	4638	4640	rBV2	1602	1037	0.12%	0.014%
99	16.210	4716	4718	4721	rBV4	1759	1179	0.14%	0.016%
100	16.355	4759	4763	4765	rBV5	2163	1942	0.23%	0.027%




Sum of corrected areas: 7242211

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033144.D
Acq On : 07 Dec 2023 14:16
Operator : SY/MD
Sample : 05673-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEJ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

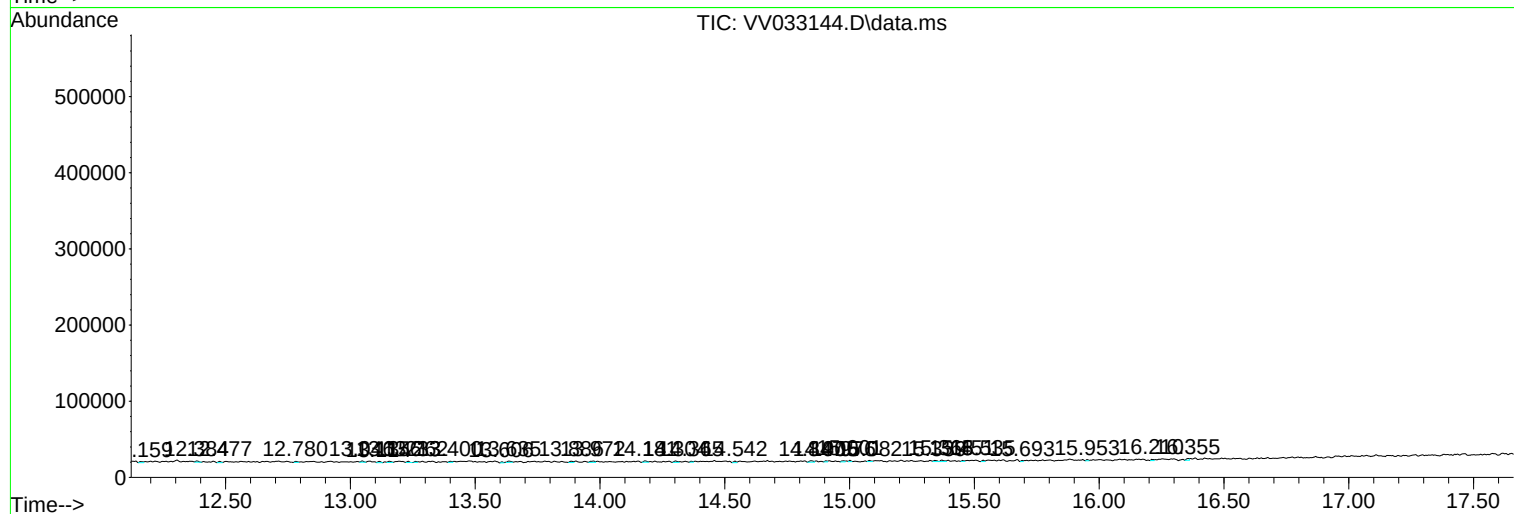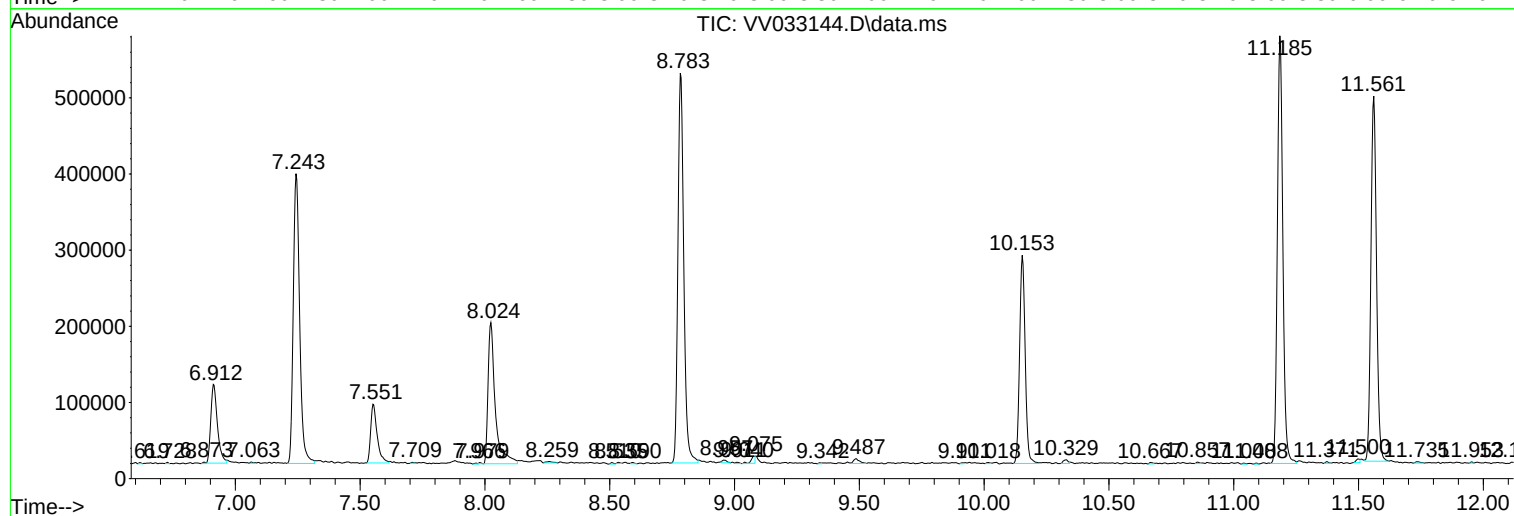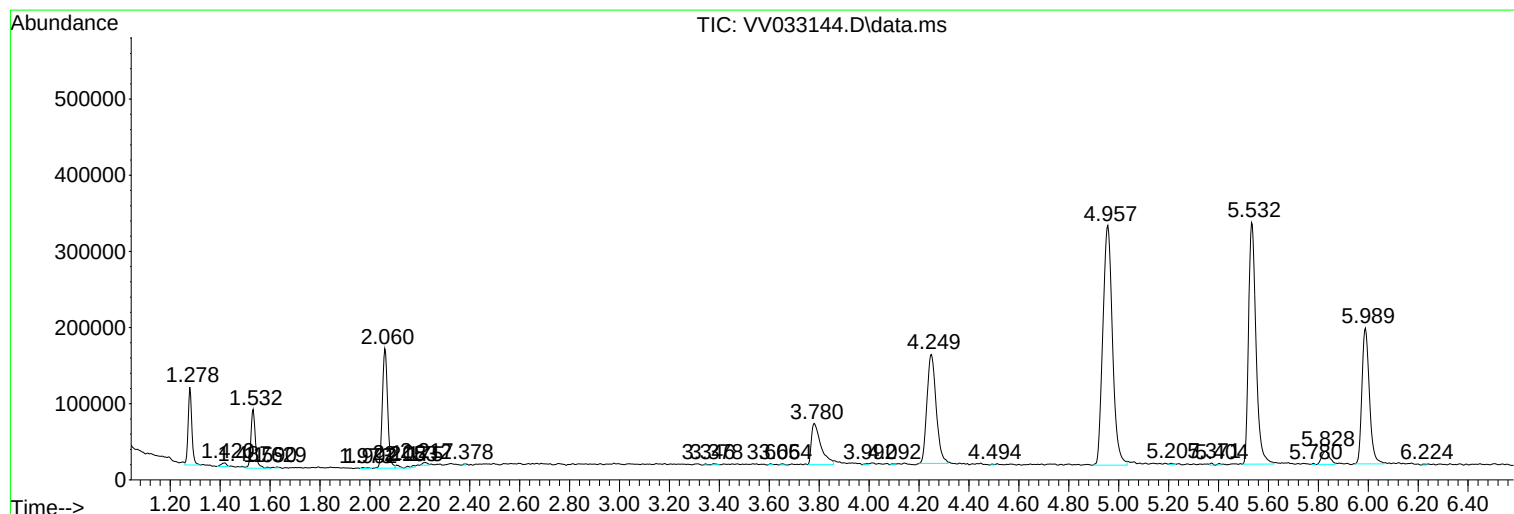

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033144.D
Acq On : 07 Dec 2023 14:16
Operator : SY/MD
Sample : 05673-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEJ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033144.D
Acq On : 07 Dec 2023 14:16
Operator : SY/MD
Sample : 05673-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEJ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------