

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033145.D
 Acq On : 07 Dec 2023 14:39
 Operator : SY/MD
 Sample : 05673-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	93582	103166	12.24%	1.467%
2	1.372	101	103	106	rBV2	991	588	0.07%	0.008%
3	1.436	119	123	127	rBV4	2296	2769	0.33%	0.039%
4	1.497	140	142	144	rBV	638	300	0.04%	0.004%
5	1.532	145	153	164	rVB	73112	85078	10.09%	1.210%
6	1.619	174	180	187	rVB	2058	2754	0.33%	0.039%
7	1.661	187	193	197	rBV2	1525	1868	0.22%	0.027%
8	1.680	197	199	200	rBV	556	209	0.02%	0.003%
9	1.706	205	207	210	rBV3	1373	693	0.08%	0.010%
10	1.732	213	215	219	rBV2	1160	759	0.09%	0.011%
11	1.767	224	226	230	rVB	1055	828	0.10%	0.012%
12	1.793	230	234	238	rBV2	1198	1015	0.12%	0.014%
13	1.818	238	242	244	rBV2	1081	934	0.11%	0.013%
14	1.863	254	256	259	rVB2	683	337	0.04%	0.005%
15	1.880	259	261	265	rVB	1033	655	0.08%	0.009%
16	1.899	265	267	269	rVB	1197	511	0.06%	0.007%
17	1.921	269	274	278	rVB3	1419	1366	0.16%	0.019%
18	1.950	278	283	287	rBV	1327	1286	0.15%	0.018%
19	1.986	291	294	296	rBV2	528	319	0.04%	0.005%
20	2.002	296	299	305	rVB	1310	1357	0.16%	0.019%
21	2.060	305	317	332	rBV	153457	227520	26.99%	3.236%
22	2.130	337	339	341	rBV	577	343	0.04%	0.005%
23	2.162	341	349	351	rBV	2173	2994	0.36%	0.043%
24	2.179	352	354	356	rVB	867	341	0.04%	0.005%
25	2.191	356	358	360	rBV	977	609	0.07%	0.009%
26	2.426	426	431	435	rBV	2089	2115	0.25%	0.030%
27	2.452	435	439	442	rBV2	1704	1823	0.22%	0.026%
28	3.060	626	628	632	rVB	2272	1332	0.16%	0.019%
29	3.088	632	637	641	rBV2	1513	1851	0.22%	0.026%
30	3.153	654	657	659	rBV2	1487	1168	0.14%	0.017%
31	3.783	845	853	876	rBV	51924	138160	16.39%	1.965%
32	4.249	983	998	1022	rBV	139740	361453	42.88%	5.141%
33	4.580	1098	1101	1104	rBV	1522	1016	0.12%	0.014%
34	4.957	1202	1218	1249	rBV2	303704	814512	96.63%	11.584%
35	5.104	1262	1264	1270	rVB4	2317	1673	0.20%	0.024%
36	5.535	1386	1398	1425	rBV	319344	658177	78.08%	9.361%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033145.D
 Acq On : 07 Dec 2023 14:39
 Operator : SY/MD
 Sample : 05673-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.828	1480	1489	1505	rVB5	18316	38377	4.55%	0.546%
38	5.989	1526	1539	1561	rBV	175191	359893	42.70%	5.118%
39	6.272	1624	1627	1629	rBV3	1318	908	0.11%	0.013%
40	6.313	1637	1640	1641	rBV2	1652	929	0.11%	0.013%
41	6.375	1657	1659	1661	rBV	1005	506	0.06%	0.007%
42	6.551	1711	1714	1716	rBV	1103	804	0.10%	0.011%
43	6.751	1773	1776	1780	rVB	1593	1220	0.14%	0.017%
44	6.915	1814	1827	1844	rBV	99529	190427	22.59%	2.708%
45	7.182	1905	1910	1916	rBV	2469	3046	0.36%	0.043%
46	7.243	1919	1929	1951	rVV	366379	640230	75.95%	9.105%
47	7.555	2017	2026	2046	rBV	72281	133683	15.86%	1.901%
48	8.024	2163	2172	2202	rBV	189060	367006	43.54%	5.220%
49	8.786	2398	2409	2431	rBV	504869	829218	98.37%	11.793%
50	8.985	2469	2471	2474	rBV	1124	563	0.07%	0.008%
51	9.416	2603	2605	2609	rVB	1470	916	0.11%	0.013%
52	9.458	2616	2618	2621	rBV	1202	757	0.09%	0.011%
53	9.526	2637	2639	2642	rBV	1194	1005	0.12%	0.014%
54	9.786	2716	2720	2722	rBV	1509	1245	0.15%	0.018%
55	9.953	2768	2772	2774	rBV	1731	1418	0.17%	0.020%
56	10.053	2801	2803	2809	rVB	1246	905	0.11%	0.013%
57	10.153	2823	2834	2853	rBV	256783	407121	48.30%	5.790%
58	10.313	2880	2884	2888	rBV2	2459	2509	0.30%	0.036%
59	10.371	2900	2902	2904	rBV2	895	550	0.07%	0.008%
60	10.529	2949	2951	2954	rVB	1190	679	0.08%	0.010%
61	10.548	2954	2957	2959	rBV	1460	811	0.10%	0.012%
62	10.870	3055	3057	3060	rBV	1309	834	0.10%	0.012%
63	10.953	3078	3083	3084	rBV2	1349	1295	0.15%	0.018%
64	11.185	3144	3155	3180	rBV	547383	842938	100.00%	11.988%
65	11.300	3189	3191	3193	rBV	1101	622	0.07%	0.009%
66	11.500	3244	3253	3261	rBV4	9292	21237	2.52%	0.302%
67	11.561	3262	3272	3289	rVB	457241	722249	85.68%	10.272%
68	11.982	3400	3403	3407	rVB	1930	1446	0.17%	0.021%
69	12.059	3425	3427	3431	rVB	1989	1246	0.15%	0.018%
70	12.220	3474	3477	3484	rVB	2599	2845	0.34%	0.040%
71	12.249	3484	3486	3488	rBV	1298	775	0.09%	0.011%
72	12.336	3511	3513	3518	rVB	1678	1221	0.14%	0.017%
73	12.365	3518	3522	3526	rBV	1769	1638	0.19%	0.023%
74	12.609	3595	3598	3600	rBV	1029	743	0.09%	0.011%
75	12.654	3610	3612	3613	rBV	1150	573	0.07%	0.008%
76	12.680	3617	3620	3624	rVB	1516	1312	0.16%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033145.D
 Acq On : 07 Dec 2023 14:39
 Operator : SY/MD
 Sample : 05673-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEJO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.889	3682	3685	3687	rBV	1652	1105	0.13%	0.016%
78	13.053	3734	3736	3738	rBV	1613	950	0.11%	0.014%
79	13.236	3789	3793	3796	rBV	2034	1620	0.19%	0.023%
80	13.413	3845	3848	3852	rBV	1244	1313	0.16%	0.019%
81	13.609	3906	3909	3913	rBV	1657	1356	0.16%	0.019%
82	13.657	3921	3924	3928	rBV	1212	1038	0.12%	0.015%
83	14.236	4101	4104	4107	rBV	1213	775	0.09%	0.011%
84	14.275	4113	4116	4118	rBV	1581	1059	0.13%	0.015%
85	14.512	4187	4190	4193	rBV	2130	1685	0.20%	0.024%
86	14.635	4226	4228	4231	rVB	2188	1209	0.14%	0.017%
87	14.654	4231	4234	4235	rBV	1396	902	0.11%	0.013%
88	14.802	4276	4280	4281	rBV	1432	1088	0.13%	0.015%
89	15.075	4361	4365	4367	rBV2	1650	1292	0.15%	0.018%
90	15.165	4390	4393	4394	rBV2	1227	763	0.09%	0.011%
91	15.326	4441	4443	4446	rBV2	1313	900	0.11%	0.013%
92	15.651	4541	4544	4549	rBV	1677	1357	0.16%	0.019%
93	15.718	4562	4565	4567	rBV2	1688	1051	0.12%	0.015%
94	16.255	4726	4732	4740	rBV3	2150	4279	0.51%	0.061%




Sum of corrected areas: 7031321

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033145.D
Acq On : 07 Dec 2023 14:39
Operator : SY/MD
Sample : 05673-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEJO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

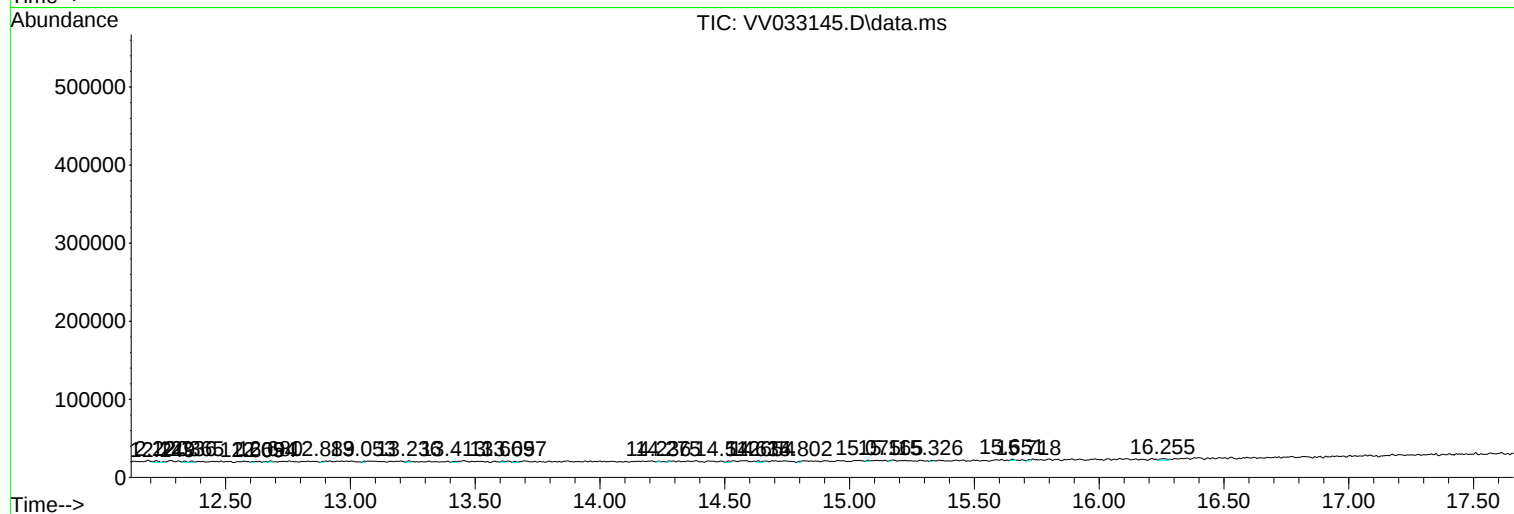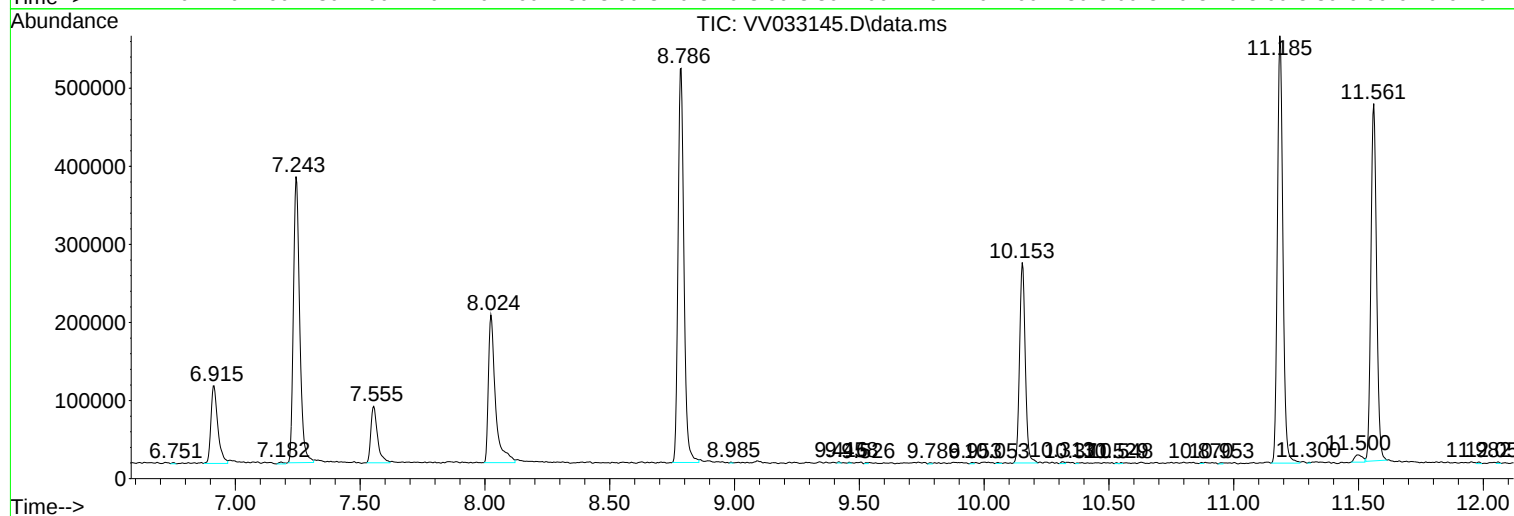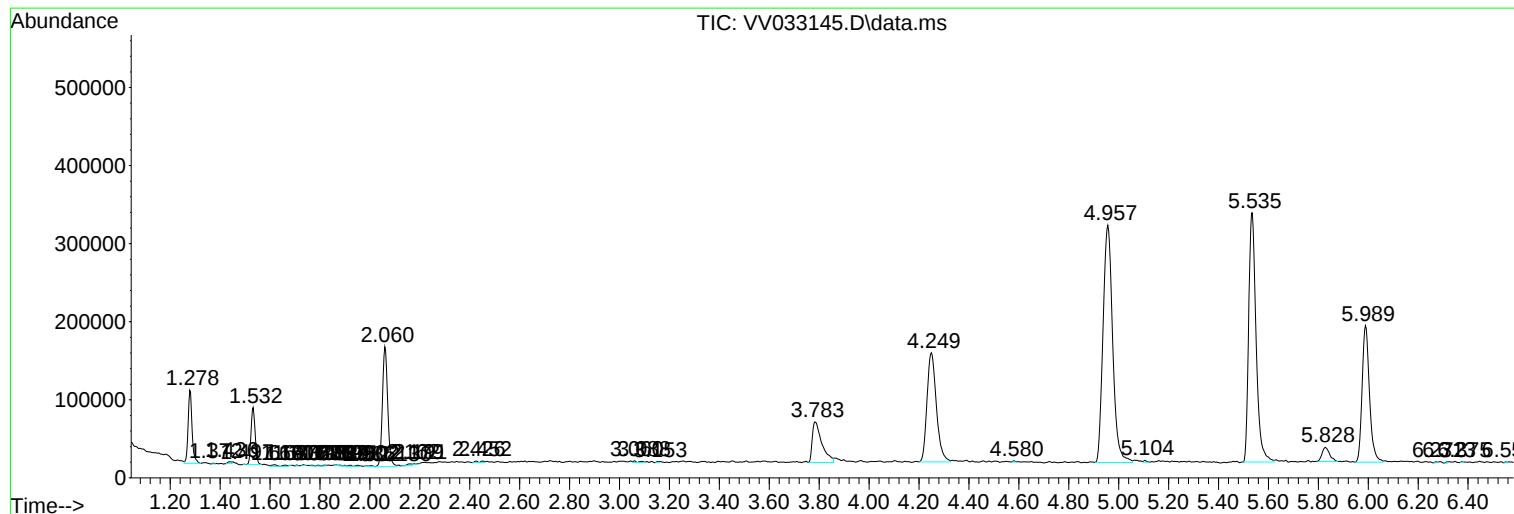

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033145.D
Acq On : 07 Dec 2023 14:39
Operator : SY/MD
Sample : 05673-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEJO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033145.D
Acq On : 07 Dec 2023 14:39
Operator : SY/MD
Sample : 05673-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEJO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------