

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033146.D
 Acq On : 07 Dec 2023 15:02
 Operator : SY/MD
 Sample : 05673-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033146.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.195	43	48	58	rVB2	24497	29742	0.61%	0.250%
2	1.278	68	74	87	rVB	94138	100805	2.06%	0.846%
3	1.416	111	117	122	rVB3	4202	4645	0.09%	0.039%
4	1.532	145	153	170	rVB	74979	91104	1.86%	0.764%
5	1.754	220	222	227	rVB2	1462	1002	0.02%	0.008%
6	1.802	233	237	240	rVB4	1117	939	0.02%	0.008%
7	1.998	295	298	303	rVB	926	837	0.02%	0.007%
8	2.060	303	317	329	rBV	151431	220304	4.50%	1.848%
9	2.162	341	349	351	rBV2	1732	2303	0.05%	0.019%
10	2.217	351	366	372	rBV2	5072	11298	0.23%	0.095%
11	2.362	407	411	412	rBV2	1513	978	0.02%	0.008%
12	2.548	467	469	472	rVB	2130	1267	0.03%	0.011%
13	2.944	589	592	595	rBV2	1465	1235	0.03%	0.010%
14	2.963	596	598	602	rVV2	1458	1107	0.02%	0.009%
15	3.326	708	711	715	rVB	1957	1334	0.03%	0.011%
16	3.349	715	718	720	rBV2	1329	926	0.02%	0.008%
17	3.439	742	746	750	rBV2	1735	2039	0.04%	0.017%
18	3.786	844	854	856	rBV	56780	84275	1.72%	0.707%
19	4.249	984	998	1023	rBV2	139539	357493	7.30%	3.000%
20	4.365	1031	1034	1039	rBV	1361	994	0.02%	0.008%
21	4.886	1193	1196	1199	rVB	1281	844	0.02%	0.007%
22	4.957	1202	1218	1243	rVV3	299059	802698	16.39%	6.735%
23	5.214	1295	1298	1304	rBV3	1198	1284	0.03%	0.011%
24	5.432	1361	1366	1374	rBV2	1242	1783	0.04%	0.015%
25	5.468	1374	1377	1382	rVB3	1441	1115	0.02%	0.009%
26	5.532	1387	1397	1420	rBV	308203	635633	12.98%	5.333%
27	5.677	1440	1442	1445	rBV2	1747	918	0.02%	0.008%
28	5.834	1480	1491	1512	rVB4	46403	106712	2.18%	0.895%
29	5.989	1527	1539	1559	rBV	173949	354124	7.23%	2.971%
30	6.230	1611	1614	1619	rBV	1448	1202	0.02%	0.010%
31	6.455	1682	1684	1691	rBV	881	1061	0.02%	0.009%
32	6.510	1695	1701	1704	rBV	1735	2144	0.04%	0.018%
33	6.754	1774	1777	1780	rBV	1585	1064	0.02%	0.009%
34	6.847	1803	1806	1810	rVB	1566	1256	0.03%	0.011%
35	6.915	1816	1827	1842	rBV	99596	183830	3.75%	1.542%
36	7.082	1876	1879	1883	rBV2	1305	1156	0.02%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033146.D
 Acq On : 07 Dec 2023 15:02
 Operator : SY/MD
 Sample : 05673-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	7.175	1904	1908	1911	rBV	1786	1496	0.03%	0.013%
38	7.243	1918	1929	1955	rBV	366559	649601	13.27%	5.450%
39	7.394	1973	1976	1986	rVB2	2772	3497	0.07%	0.029%
40	7.497	2004	2008	2012	rBV2	1831	1551	0.03%	0.013%
41	7.551	2017	2025	2046	rBV	74539	136167	2.78%	1.142%
42	7.718	2075	2077	2083	rVB	1387	1436	0.03%	0.012%
43	7.905	2121	2135	2163	rBV	2947398	4896176	100.00%	41.081%
44	8.024	2163	2172	2200	rVB	190837	358709	7.33%	3.010%
45	8.255	2241	2244	2246	rBV	1519	1063	0.02%	0.009%
46	8.294	2253	2256	2261	rVB	1831	1226	0.03%	0.010%
47	8.455	2301	2306	2308	rBV	1702	1671	0.03%	0.014%
48	8.683	2374	2377	2385	rVB2	2048	2008	0.04%	0.017%
49	8.722	2385	2389	2391	rBV	1547	1215	0.02%	0.010%
50	8.786	2398	2409	2428	rBV	498517	813794	16.62%	6.828%
51	8.895	2441	2443	2446	rBV	1364	861	0.02%	0.007%
52	8.995	2471	2474	2477	rBV	1389	1089	0.02%	0.009%
53	9.095	2502	2505	2507	rBV	1333	975	0.02%	0.008%
54	9.149	2517	2522	2526	rBV	2072	2457	0.05%	0.021%
55	9.349	2581	2584	2588	rBV	1330	1349	0.03%	0.011%
56	9.387	2593	2596	2604	rVB	1711	1987	0.04%	0.017%
57	9.606	2659	2664	2666	rBV	2723	2562	0.05%	0.021%
58	10.056	2799	2804	2806	rBV2	1268	1307	0.03%	0.011%
59	10.152	2823	2834	2853	rBV	262050	413157	8.44%	3.467%
60	10.313	2881	2884	2886	rBV2	1201	886	0.02%	0.007%
61	10.866	3053	3056	3058	rBV	1613	869	0.02%	0.007%
62	10.940	3075	3079	3087	rBV2	1434	1883	0.04%	0.016%
63	11.043	3108	3111	3113	rBV	1575	1130	0.02%	0.009%
64	11.185	3145	3155	3174	rBV	532746	827188	16.89%	6.940%
65	11.336	3197	3202	3208	rVB2	1834	1983	0.04%	0.017%
66	11.471	3241	3244	3246	rBV	1413	875	0.02%	0.007%
67	11.506	3249	3255	3261	rVV4	4966	8130	0.17%	0.068%
68	11.561	3262	3272	3292	rVB	465180	724809	14.80%	6.081%
69	12.008	3408	3411	3414	rBV	2046	1522	0.03%	0.013%
70	12.082	3431	3434	3438	rVB	1618	947	0.02%	0.008%
71	12.242	3480	3484	3490	rBV	2259	2497	0.05%	0.021%
72	12.439	3541	3545	3547	rBV	1061	1026	0.02%	0.009%
73	12.738	3635	3638	3640	rBV2	1247	931	0.02%	0.008%
74	12.866	3676	3678	3684	rVB	1570	1155	0.02%	0.010%
75	13.082	3741	3745	3750	rVB	2488	2661	0.05%	0.022%
76	13.111	3750	3754	3756	rBV2	1926	1778	0.04%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033146.D
 Acq On : 07 Dec 2023 15:02
 Operator : SY/MD
 Sample : 05673-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	13.149	3763	3766	3768	rBV2	1355	888	0.02%	0.007%
78	13.336	3821	3824	3826	rBV	1630	1104	0.02%	0.009%
79	13.352	3827	3829	3833	rVB	1314	865	0.02%	0.007%
80	13.439	3853	3856	3860	rBV4	1349	1504	0.03%	0.013%
81	13.529	3882	3884	3888	rVB	1465	822	0.02%	0.007%
82	13.625	3911	3914	3917	rVB	1712	1127	0.02%	0.009%
83	13.657	3917	3924	3927	rBV	1953	2320	0.05%	0.019%
84	13.773	3957	3960	3967	rVB	2692	2852	0.06%	0.024%
85	13.805	3967	3970	3973	rBV	1160	903	0.02%	0.008%
86	13.840	3978	3981	3984	rBV3	1612	1188	0.02%	0.010%
87	13.992	4025	4028	4031	rBV2	1356	967	0.02%	0.008%
88	14.168	4077	4083	4088	rBV	1620	2279	0.05%	0.019%
89	14.384	4147	4150	4155	rBV3	1672	1504	0.03%	0.013%
90	14.435	4162	4166	4169	rVB	1636	1214	0.02%	0.010%
91	14.455	4169	4172	4175	rBV	1373	931	0.02%	0.008%
92	14.583	4208	4212	4216	rBV	1159	1192	0.02%	0.010%
93	14.667	4236	4238	4240	rBV2	1210	827	0.02%	0.007%
94	14.747	4260	4263	4267	rVB	1763	1333	0.03%	0.011%
95	14.773	4267	4271	4272	rBV2	1481	1120	0.02%	0.009%
96	14.889	4304	4307	4312	rBV	1559	1360	0.03%	0.011%
97	15.345	4445	4449	4452	rBV3	1714	1828	0.04%	0.015%
98	15.429	4472	4475	4477	rBV	1836	1298	0.03%	0.011%
99	15.712	4561	4563	4567	rBV4	1372	943	0.02%	0.008%
100	15.982	4645	4647	4650	rBV	1724	967	0.02%	0.008%




Sum of corrected areas: 11918411

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033146.D
Acq On : 07 Dec 2023 15:02
Operator : SY/MD
Sample : 05673-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEH8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

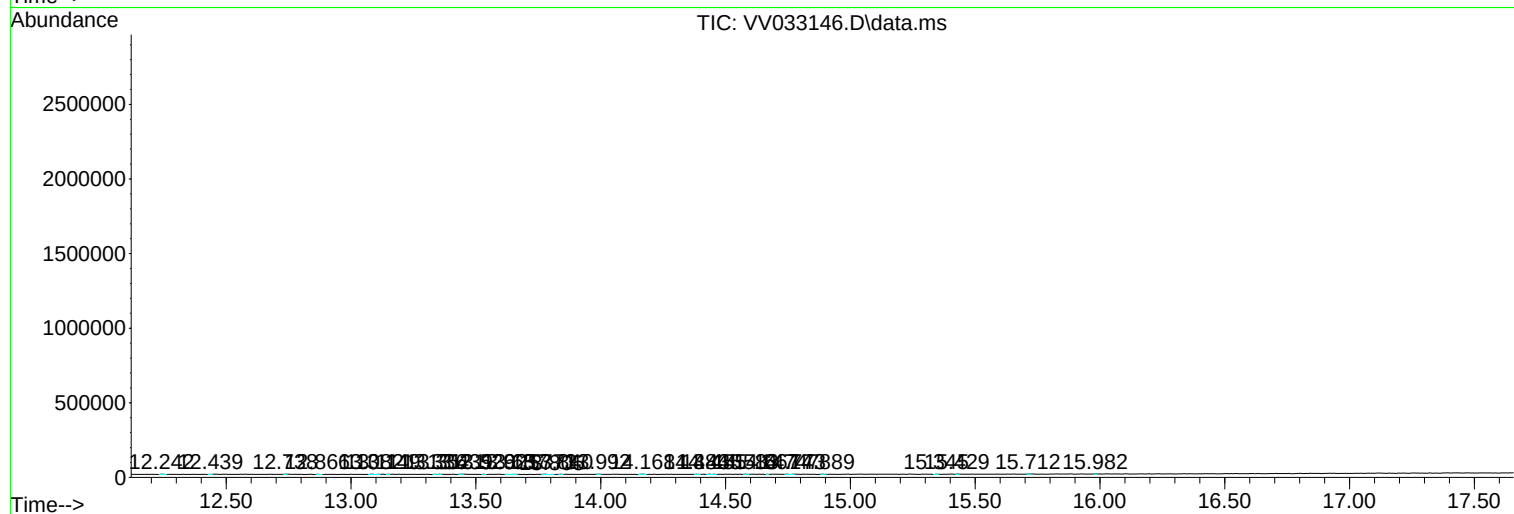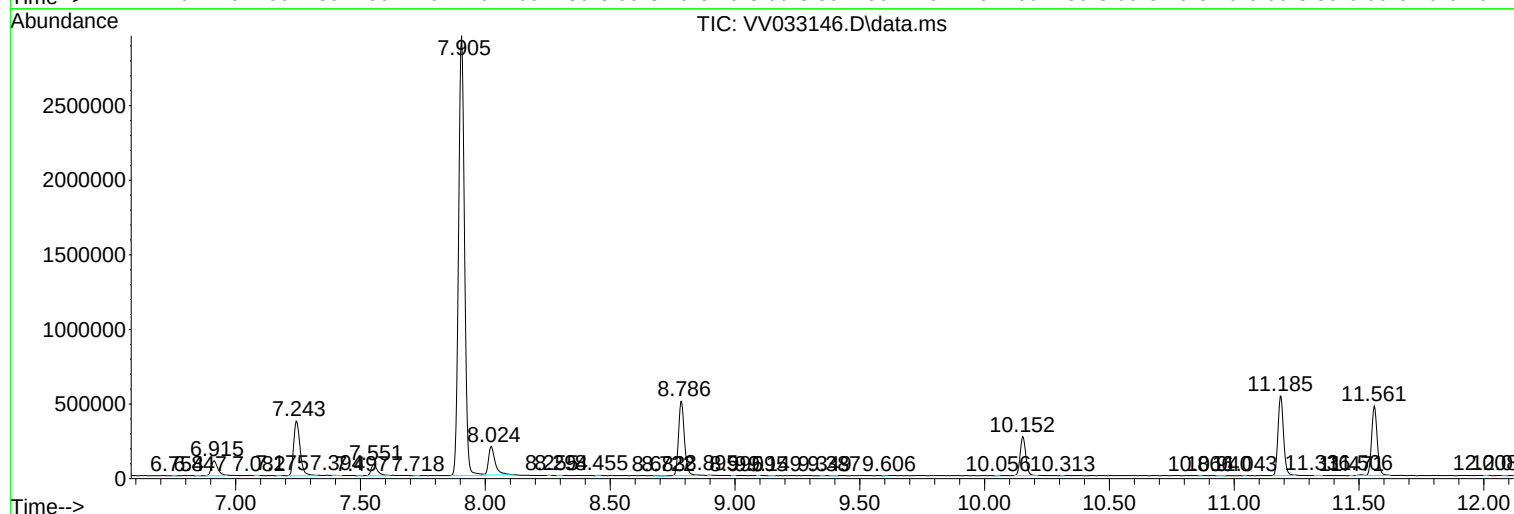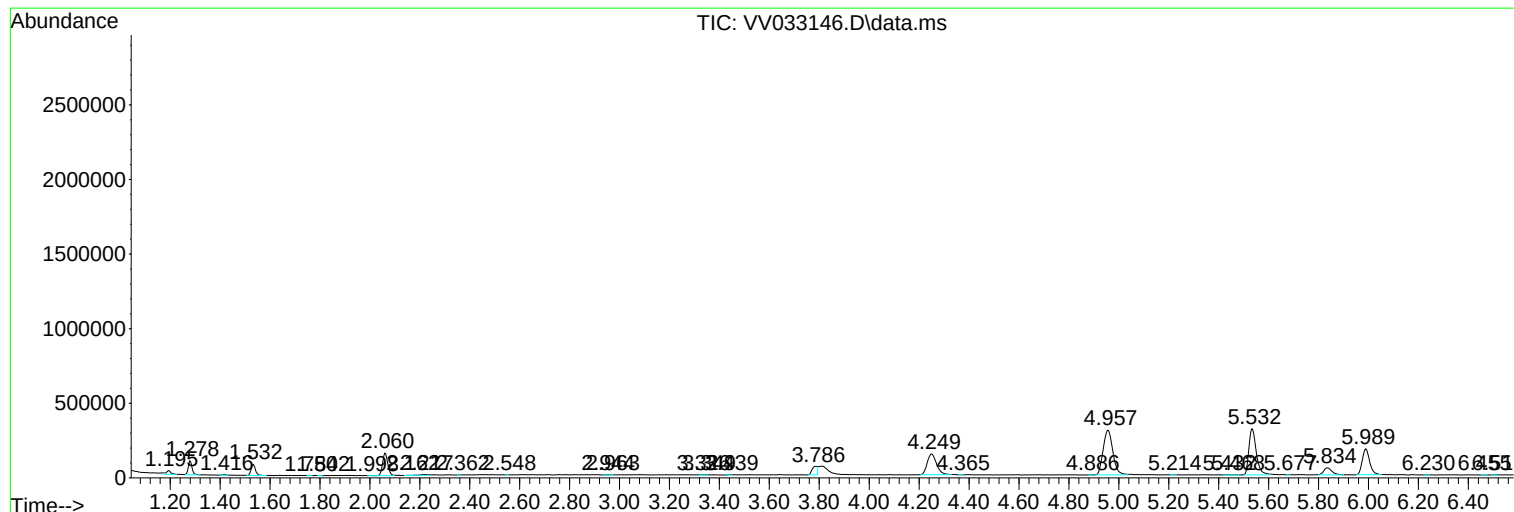

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033146.D
Acq On : 07 Dec 2023 15:02
Operator : SY/MD
Sample : 05673-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEH8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033146.D
Acq On : 07 Dec 2023 15:02
Operator : SY/MD
Sample : 05673-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEH8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------