

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033148.D
 Acq On : 07 Dec 2023 15:49
 Operator : SY/MD
 Sample : 05645-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033148.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	84	rVB	93965	96490	11.65%	1.380%
2	1.420	113	118	125	rVB3	6102	6577	0.79%	0.094%
3	1.481	134	137	139	rBV2	1651	1055	0.13%	0.015%
4	1.532	145	153	171	rVB	74801	89176	10.77%	1.275%
5	1.603	172	175	180	rVB	1941	1720	0.21%	0.025%
6	1.629	180	183	185	rBV2	1368	896	0.11%	0.013%
7	1.645	185	188	191	rVB3	982	646	0.08%	0.009%
8	1.680	196	199	203	rBV3	1023	928	0.11%	0.013%
9	1.780	227	230	236	rVB2	891	956	0.12%	0.014%
10	1.828	241	245	249	rVB	1912	1833	0.22%	0.026%
11	1.860	249	255	259	rBV3	555	696	0.08%	0.010%
12	1.912	268	271	275	rVB2	1004	903	0.11%	0.013%
13	1.934	275	278	281	rVB	2065	1298	0.16%	0.019%
14	1.979	285	292	297	rVB	1339	1889	0.23%	0.027%
15	2.060	305	317	331	rBV	150849	224381	27.10%	3.208%
16	2.137	337	341	344	rBV5	799	678	0.08%	0.010%
17	2.178	344	354	356	rBV	2790	4398	0.53%	0.063%
18	2.217	360	366	373	rVV2	6507	11111	1.34%	0.159%
19	2.532	460	464	466	rBV	1785	1251	0.15%	0.018%
20	2.551	466	470	474	rBV2	1974	2200	0.27%	0.031%
21	2.960	595	597	602	rVB2	1557	1301	0.16%	0.019%
22	3.127	646	649	653	rBV	1590	1368	0.17%	0.020%
23	3.191	666	669	674	rBV	1461	1524	0.18%	0.022%
24	3.574	785	788	792	rBV	1566	1325	0.16%	0.019%
25	3.725	832	835	839	rBV	1337	1270	0.15%	0.018%
26	3.780	844	852	881	rVV2	56230	151692	18.32%	2.169%
27	4.092	942	949	952	rBV3	2173	2895	0.35%	0.041%
28	4.249	982	998	1022	rBV	142426	367773	44.42%	5.258%
29	4.384	1038	1040	1046	rBV2	1269	1170	0.14%	0.017%
30	4.468	1063	1066	1070	rBV2	1445	1131	0.14%	0.016%
31	4.542	1087	1089	1094	rVB	1601	1288	0.16%	0.018%
32	4.828	1175	1178	1181	rBV2	1339	831	0.10%	0.012%
33	4.886	1193	1196	1202	rBV2	1454	1511	0.18%	0.022%
34	4.957	1202	1218	1250	rVV2	304183	827990	100.00%	11.838%
35	5.252	1307	1310	1314	rBV3	1304	1107	0.13%	0.016%
36	5.320	1328	1331	1332	rBV2	1248	716	0.09%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120723\
 Data File : VW033148.D
 Acq On : 07 Dec 2023 15:49
 Operator : SY/MD
 Sample : 05645-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.532	1387	1397	1424	rBV	299777	612772	74.01%	8.761%
38	5.731	1456	1459	1464	rVB2	1866	1215	0.15%	0.017%
39	5.831	1479	1490	1503	rBV4	12458	26651	3.22%	0.381%
40	5.989	1527	1539	1563	rBV	175860	360558	43.55%	5.155%
41	6.333	1642	1646	1648	rBV	1264	1171	0.14%	0.017%
42	6.542	1709	1711	1714	rBV	1207	809	0.10%	0.012%
43	6.731	1767	1770	1772	rBV	1322	973	0.12%	0.014%
44	6.834	1799	1802	1805	rVB	1774	1247	0.15%	0.018%
45	6.911	1816	1826	1848	rVV	100213	190653	23.03%	2.726%
46	7.120	1888	1891	1894	rVB	1792	1161	0.14%	0.017%
47	7.140	1894	1897	1900	rBV2	1981	1644	0.20%	0.024%
48	7.198	1913	1915	1918	rVB	1357	683	0.08%	0.010%
49	7.243	1918	1929	1958	rBV	373554	667732	80.64%	9.547%
50	7.345	1958	1961	1963	rBV	2138	1431	0.17%	0.020%
51	7.387	1972	1974	1977	rVB2	1350	650	0.08%	0.009%
52	7.554	2017	2026	2045	rBV	74754	131864	15.93%	1.885%
53	7.767	2090	2092	2095	rBV	1189	701	0.08%	0.010%
54	7.908	2130	2136	2154	rVB5	9479	18211	2.20%	0.260%
55	8.024	2163	2172	2205	rBV	194549	376083	45.42%	5.377%
56	8.259	2243	2245	2247	rBV2	1444	848	0.10%	0.012%
57	8.480	2310	2314	2317	rBV3	1572	1720	0.21%	0.025%
58	8.783	2398	2408	2433	rBV	466041	770892	93.10%	11.022%
59	9.008	2473	2478	2481	rBV2	1775	1684	0.20%	0.024%
60	9.152	2519	2523	2527	rBV	1908	1417	0.17%	0.020%
61	9.275	2558	2561	2565	rBV	1531	970	0.12%	0.014%
62	9.333	2577	2579	2584	rBV2	1069	739	0.09%	0.011%
63	9.738	2700	2705	2711	rBV	1691	2806	0.34%	0.040%
64	10.053	2800	2803	2810	rVB	2050	2153	0.26%	0.031%
65	10.085	2810	2813	2818	rBV	1926	2110	0.25%	0.030%
66	10.152	2823	2834	2855	rBV	272565	435473	52.59%	6.226%
67	10.413	2912	2915	2918	rBV	1272	914	0.11%	0.013%
68	10.451	2925	2927	2931	rVB2	1327	906	0.11%	0.013%
69	10.522	2945	2949	2956	rBV	2240	2745	0.33%	0.039%
70	10.564	2960	2962	2965	rBV	1091	641	0.08%	0.009%
71	10.673	2993	2996	2999	rBV	1400	858	0.10%	0.012%
72	10.696	3000	3003	3004	rBV	1311	811	0.10%	0.012%
73	10.828	3041	3044	3046	rBV	1492	977	0.12%	0.014%
74	10.844	3046	3049	3052	rVV2	1507	1054	0.13%	0.015%
75	10.943	3077	3080	3082	rBV2	1248	802	0.10%	0.011%
76	10.982	3089	3092	3095	rBV	1403	1012	0.12%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033148.D
 Acq On : 07 Dec 2023 15:49
 Operator : SY/MD
 Sample : 05645-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.185	3144	3155	3175	rBV	505100	793935	95.89%	11.351%
78	11.377	3209	3215	3219	rBV2	1584	2111	0.25%	0.030%
79	11.519	3257	3259	3261	rBV	1182	737	0.09%	0.011%
80	11.561	3261	3272	3289	rVV	462666	731089	88.30%	10.453%
81	12.162	3457	3459	3462	rVB	1321	680	0.08%	0.010%
82	12.638	3602	3607	3610	rBV	1591	1596	0.19%	0.023%
83	12.821	3661	3664	3666	rBV	1747	1142	0.14%	0.016%
84	12.905	3687	3690	3693	rBV2	1752	1124	0.14%	0.016%
85	13.181	3773	3776	3782	rBV	1615	2060	0.25%	0.029%
86	13.262	3798	3801	3805	rBV2	1547	1597	0.19%	0.023%
87	13.467	3861	3865	3867	rBV	1591	1176	0.14%	0.017%
88	13.503	3872	3876	3880	rVV2	1343	1350	0.16%	0.019%
89	14.117	4065	4067	4070	rVB	1459	731	0.09%	0.010%
90	14.136	4070	4073	4076	rVB	1285	725	0.09%	0.010%
91	14.313	4124	4128	4129	rBV2	1723	1106	0.13%	0.016%
92	14.400	4152	4155	4158	rBV3	1438	998	0.12%	0.014%
93	14.966	4328	4331	4333	rBV2	1456	924	0.11%	0.013%
94	15.139	4382	4385	4387	rBV	1423	935	0.11%	0.013%
95	15.242	4414	4417	4418	rBV2	1192	670	0.08%	0.010%
96	15.300	4431	4435	4437	rBV	1949	1326	0.16%	0.019%
97	15.612	4530	4532	4541	rVB	1843	2199	0.27%	0.031%
98	15.744	4569	4573	4579	rVB	2036	2037	0.25%	0.029%
99	15.799	4587	4590	4591	rBV2	1630	913	0.11%	0.013%
100	16.464	4794	4797	4799	rBV4	1734	1258	0.15%	0.018%




Sum of corrected areas: 6994134

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033148.D
Acq On : 07 Dec 2023 15:49
Operator : SY/MD
Sample : 05645-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

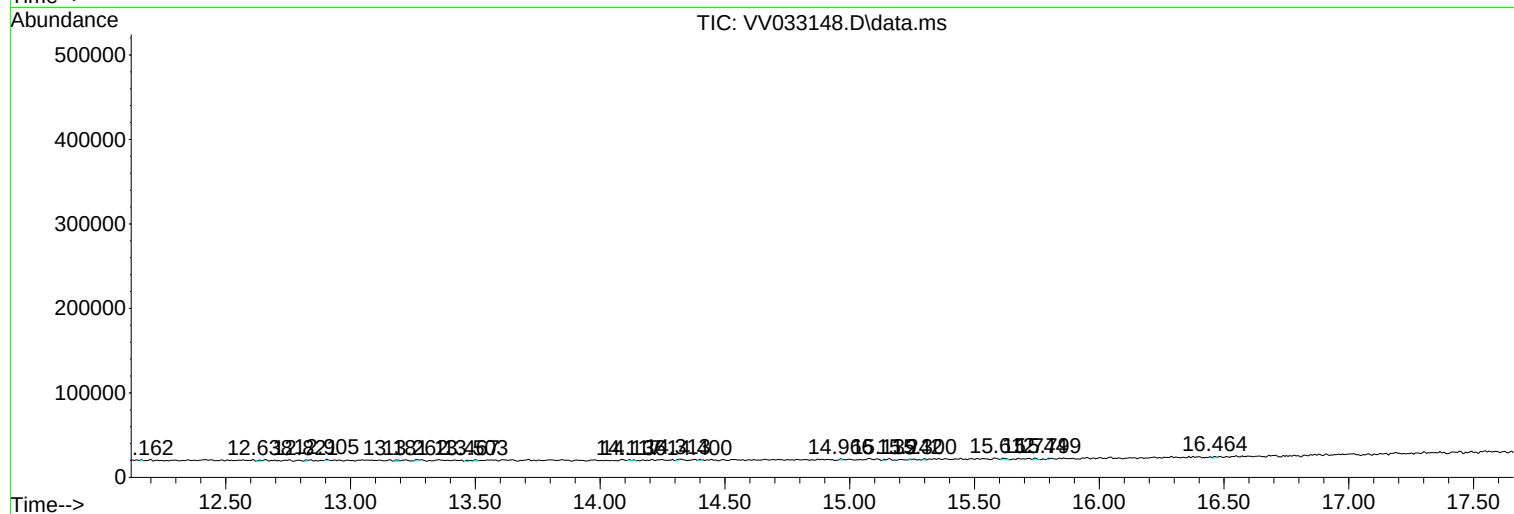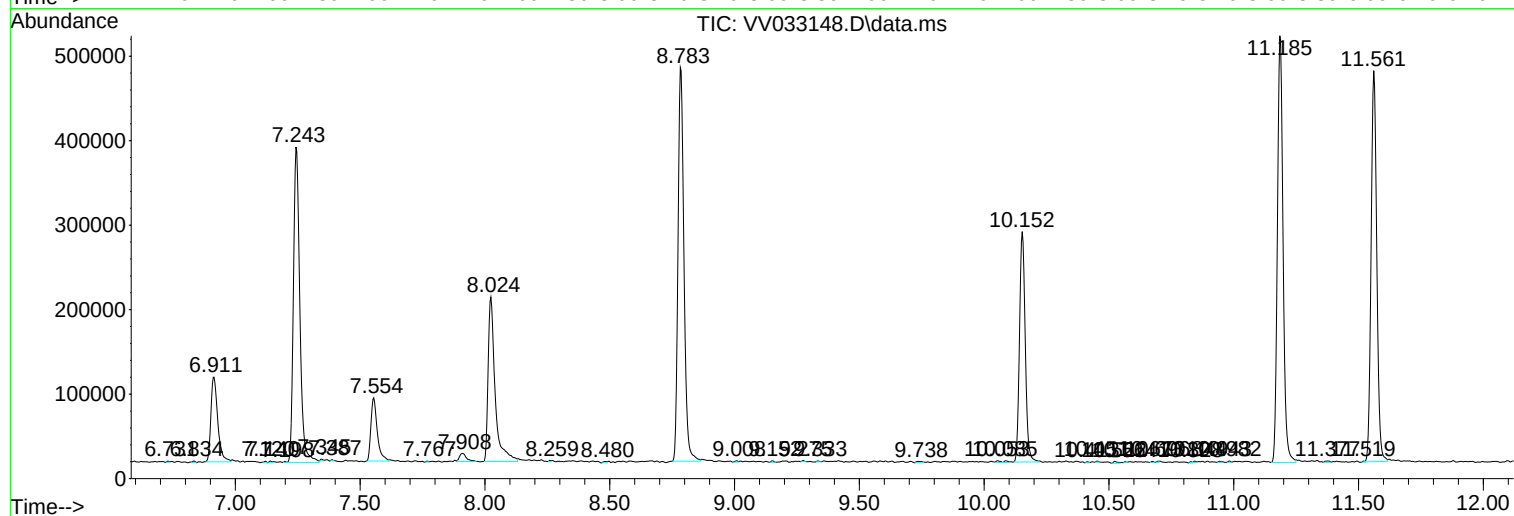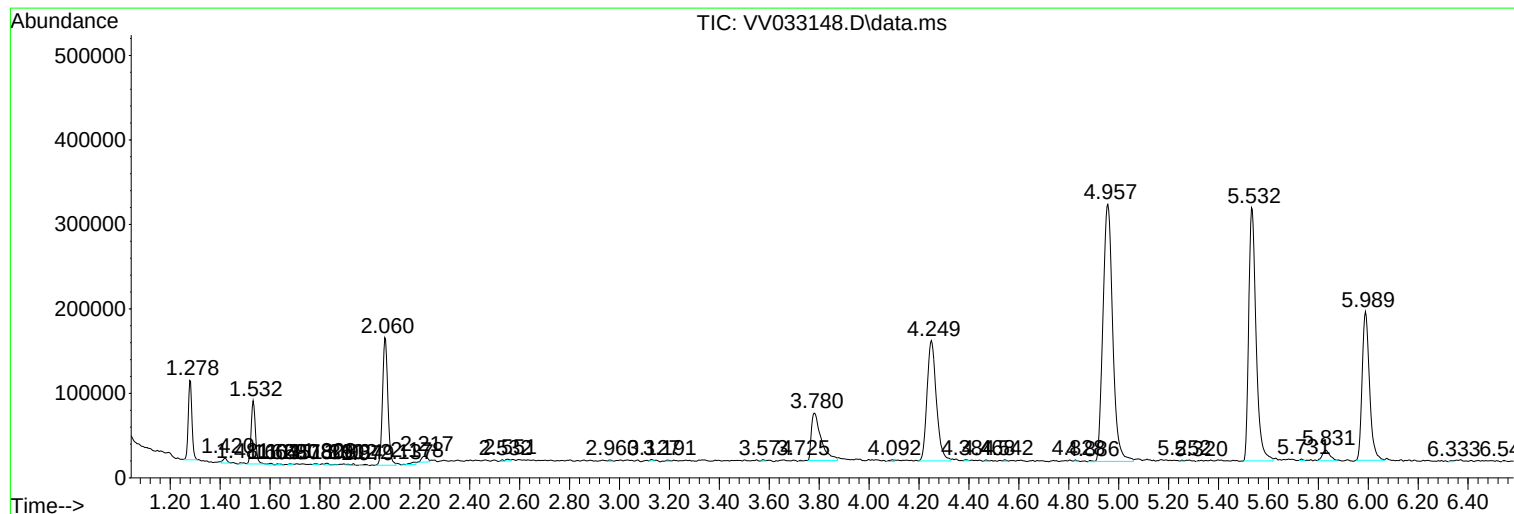

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033148.D
Acq On : 07 Dec 2023 15:49
Operator : SY/MD
Sample : 05645-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033148.D
Acq On : 07 Dec 2023 15:49
Operator : SY/MD
Sample : 05645-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------