

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033149.D
 Acq On : 07 Dec 2023 16:12
 Operator : SY/MD
 Sample : 05645-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

Signal : TIC: VV033149.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	93	rVB	89017	101582	12.40%	1.454%
2	1.349	94	96	99	rVB	1475	798	0.10%	0.011%
3	1.388	105	108	109	rBV2	1239	681	0.08%	0.010%
4	1.417	111	117	127	rVB3	5534	7979	0.97%	0.114%
5	1.532	145	153	166	rVB	71232	83406	10.18%	1.193%
6	1.613	174	178	184	rVB2	1544	1922	0.23%	0.028%
7	1.642	184	187	188	rBV	1038	603	0.07%	0.009%
8	1.664	192	194	196	rVV2	923	623	0.08%	0.009%
9	1.677	196	198	201	rVV	1918	1047	0.13%	0.015%
10	1.696	201	204	207	rVV2	1502	1068	0.13%	0.015%
11	1.728	207	214	220	rVV2	1311	2448	0.30%	0.035%
12	1.761	220	224	227	rVV2	1741	1478	0.18%	0.021%
13	1.783	227	231	233	rVV2	1256	1179	0.14%	0.017%
14	1.809	237	239	241	rVV2	1075	623	0.08%	0.009%
15	1.822	241	243	246	rVV	1194	672	0.08%	0.010%
16	1.838	246	248	251	rVB2	741	426	0.05%	0.006%
17	1.851	251	252	254	rBV	263	94	0.01%	0.001%
18	1.864	254	256	259	rBV	797	360	0.04%	0.005%
19	1.880	259	261	264	rVB2	324	179	0.02%	0.003%
20	1.902	264	268	276	rBV	1568	1671	0.20%	0.024%
21	1.937	276	279	284	rVB	813	578	0.07%	0.008%
22	1.963	284	287	290	rBV	765	631	0.08%	0.009%
23	1.992	295	296	299	rVB2	1406	558	0.07%	0.008%
24	2.008	299	301	304	rBV4	1087	767	0.09%	0.011%
25	2.021	304	305	306	rBV4	456	171	0.02%	0.002%
26	2.060	306	317	331	rBV	149753	224665	27.42%	3.215%
27	2.153	342	346	347	rBV2	2759	1710	0.21%	0.024%
28	2.217	359	366	376	rBV3	7763	14715	1.80%	0.211%
29	2.442	432	436	440	rBV2	1772	1993	0.24%	0.029%
30	2.548	465	469	470	rBV3	1612	1195	0.15%	0.017%
31	2.786	540	543	547	rBV	1497	1563	0.19%	0.022%
32	3.156	654	658	664	rBV	1840	2060	0.25%	0.029%
33	3.185	665	667	669	rBV	1383	859	0.10%	0.012%
34	3.529	771	774	776	rBV	1492	979	0.12%	0.014%
35	3.648	809	811	814	rVB	2039	1199	0.15%	0.017%
36	3.667	814	817	819	rBV	1371	933	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033149.D
 Acq On : 07 Dec 2023 16:12
 Operator : SY/MD
 Sample : 05645-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	3.780	844	852	878	rBV	53387	145541	17.76%	2.083%
38	4.249	983	998	1024	rBV	137397	349766	42.68%	5.005%
39	4.391	1039	1042	1043	rBV	1476	871	0.11%	0.012%
40	4.571	1095	1098	1101	rBV	1834	1376	0.17%	0.020%
41	4.770	1156	1160	1163	rVB	1979	1645	0.20%	0.024%
42	4.828	1172	1178	1185	rBV	1926	2751	0.34%	0.039%
43	4.957	1202	1218	1245	rBV2	294172	793891	96.88%	11.360%
44	5.140	1273	1275	1278	rBB2	1126	474	0.06%	0.007%
45	5.532	1386	1397	1425	rBV	307308	633147	77.26%	9.060%
46	5.834	1480	1491	1516	rVB6	61230	137610	16.79%	1.969%
47	5.989	1527	1539	1560	rBV2	170313	354120	43.21%	5.067%
48	6.317	1638	1641	1643	rBV	1349	1085	0.13%	0.016%
49	6.420	1670	1673	1676	rBV2	1261	1005	0.12%	0.014%
50	6.574	1718	1721	1722	rBV2	1581	856	0.10%	0.012%
51	6.622	1732	1736	1742	rVB2	1964	2219	0.27%	0.032%
52	6.670	1748	1751	1754	rBV	1362	952	0.12%	0.014%
53	6.709	1761	1763	1766	rVB	1365	651	0.08%	0.009%
54	6.860	1807	1810	1814	rVB	2734	2175	0.27%	0.031%
55	6.912	1815	1826	1850	rBV2	98219	193489	23.61%	2.769%
56	7.243	1919	1929	1959	rBV	355129	627932	76.62%	8.985%
57	7.555	2017	2026	2045	rBV	72618	128792	15.72%	1.843%
58	7.658	2056	2058	2060	rBV	1236	644	0.08%	0.009%
59	7.867	2120	2123	2125	rBV2	1602	1181	0.14%	0.017%
60	7.912	2129	2137	2145	rVB4	5295	7850	0.96%	0.112%
61	7.944	2145	2147	2149	rBV2	970	525	0.06%	0.008%
62	8.024	2163	2172	2203	rBV	180805	355988	43.44%	5.094%
63	8.400	2287	2289	2297	rVB	2320	2494	0.30%	0.036%
64	8.442	2297	2302	2311	rVB	2195	3603	0.44%	0.052%
65	8.481	2311	2314	2317	rBV	2056	1725	0.21%	0.025%
66	8.747	2394	2397	2398	rBV	1880	1060	0.13%	0.015%
67	8.783	2398	2408	2431	rVV	494242	810458	98.90%	11.597%
68	8.960	2460	2463	2468	rVB	2028	1636	0.20%	0.023%
69	8.985	2468	2471	2474	rBV	1792	1182	0.14%	0.017%
70	9.185	2531	2533	2536	rBV2	1054	916	0.11%	0.013%
71	9.410	2601	2603	2606	rBV	1066	662	0.08%	0.009%
72	9.667	2680	2683	2688	rVB	1359	1030	0.13%	0.015%
73	9.744	2704	2707	2712	rBV2	1479	1469	0.18%	0.021%
74	10.153	2824	2834	2852	rBV	257308	409033	49.91%	5.853%
75	10.590	2967	2970	2974	rBV	1502	1404	0.17%	0.020%
76	10.683	2997	2999	3002	rVB	1162	643	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
 Data File : VV033149.D
 Acq On : 07 Dec 2023 16:12
 Operator : SY/MD
 Sample : 05645-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	10.725	3008	3012	3016	rBV	1552	1384	0.17%	0.020%
78	11.091	3123	3126	3129	rBV2	2048	1938	0.24%	0.028%
79	11.185	3145	3155	3174	rBV	533500	819489	100.00%	11.726%
80	11.368	3209	3212	3213	rBV	1332	850	0.10%	0.012%
81	11.471	3241	3244	3246	rBV	1452	827	0.10%	0.012%
82	11.561	3261	3272	3290	rBV	453779	705400	86.08%	10.093%
83	12.214	3472	3475	3479	rBV2	1153	910	0.11%	0.013%
84	12.294	3497	3500	3507	rBV	1381	1507	0.18%	0.022%
85	13.497	3870	3874	3877	rBV	2154	1687	0.21%	0.024%
86	13.702	3935	3938	3940	rBV	1454	879	0.11%	0.013%
87	14.162	4075	4081	4083	rBV	1421	1585	0.19%	0.023%
88	14.310	4124	4127	4131	rBV2	1713	1263	0.15%	0.018%
89	14.371	4144	4146	4149	rBV	1332	703	0.09%	0.010%
90	14.603	4216	4218	4221	rBV	1410	982	0.12%	0.014%
91	15.098	4369	4372	4376	rBV	1466	1261	0.15%	0.018%
92	15.670	4548	4550	4553	rVB2	1579	749	0.09%	0.011%




Sum of corrected areas: 6988680

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033149.D
Acq On : 07 Dec 2023 16:12
Operator : SY/MD
Sample : 05645-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

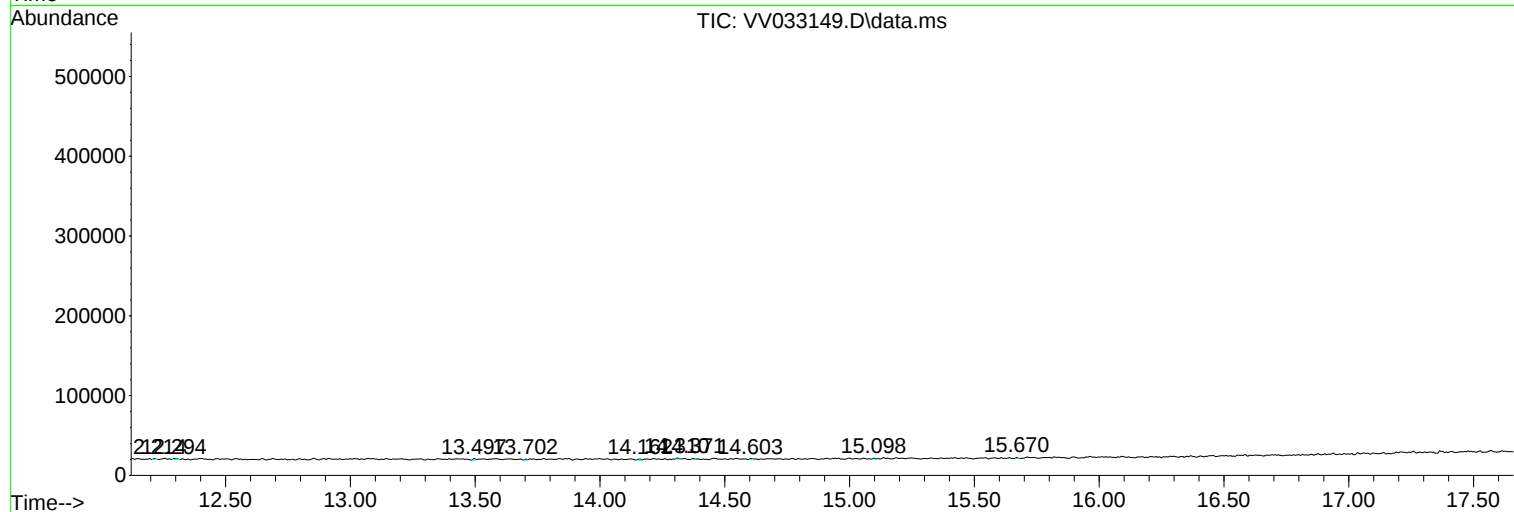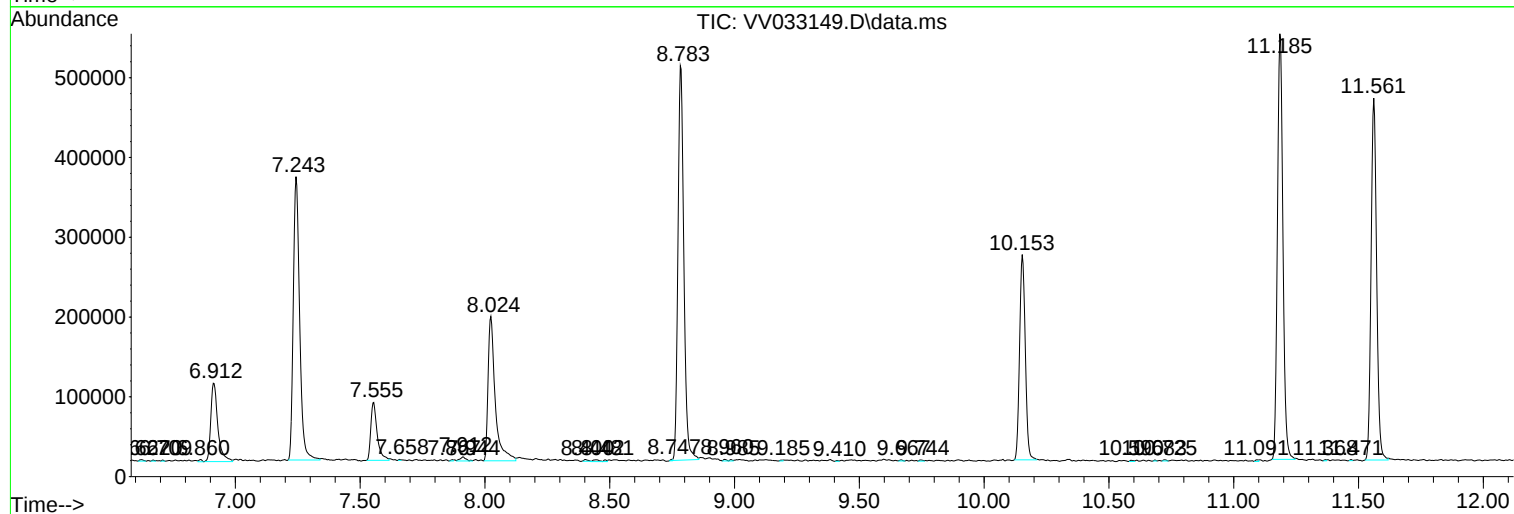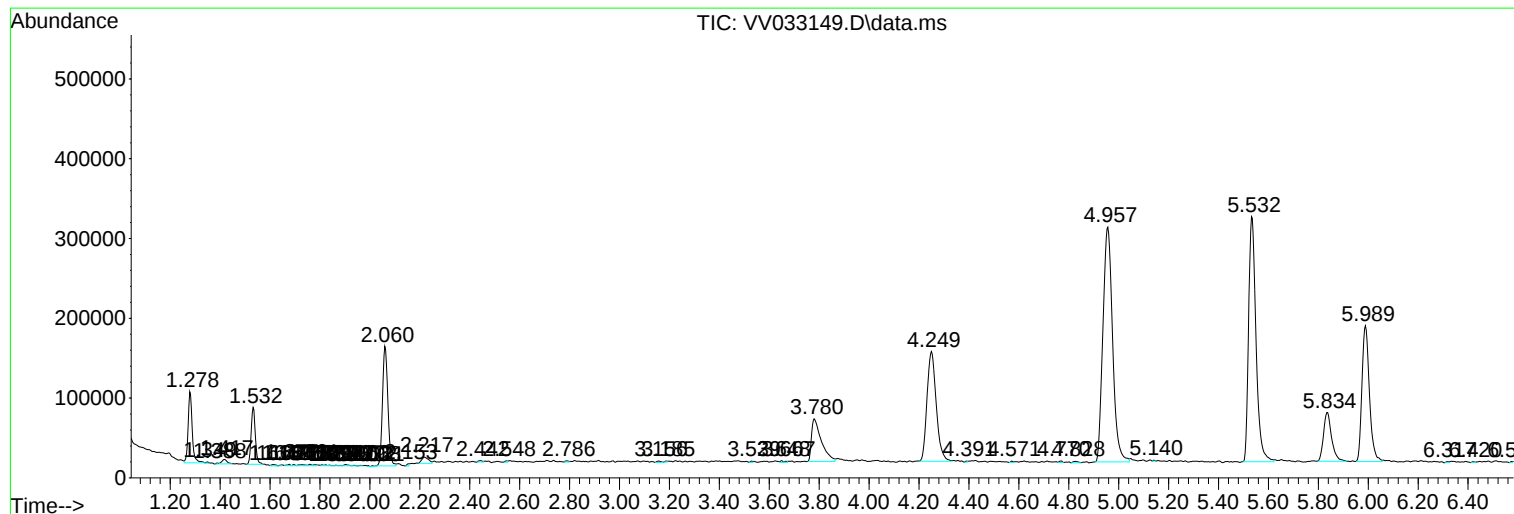

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033149.D
Acq On : 07 Dec 2023 16:12
Operator : SY/MD
Sample : 05645-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120723\
Data File : VV033149.D
Acq On : 07 Dec 2023 16:12
Operator : SY/MD
Sample : 05645-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc